

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG050721\  
 Data File : FG008010.D  
 Signal(s) : FID1A.ch  
 Acq On : 07 May 2021 10:14  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: May 07 23:06:51 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG042121.M  
 Quant Title :  
 QLast Update : Thu Apr 22 01:54:01 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.509  | 3044364  | 19.899 ug/ml |
| 12) N-OCTACOSANE            | 16.968 | 2558672  | 17.472 ug/ml |
| 13) N-TRIACONTANE           | 17.855 | 150227   | 1.051 ug/ml  |
| 14) N-DOTRIACONTANE         | 18.690 | 176417   | 1.293 ug/ml  |
| 15) N-TETRATRIACONTANE      | 19.476 | 137334   | 1.068 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG050721\  
Data File : FG008010.D  
Signal(s) : FID1A.ch  
Acq On : 07 May 2021 10:14  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: May 07 23:06:51 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG042121.M  
Quant Title :  
QLast Update : Thu Apr 22 01:54:01 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

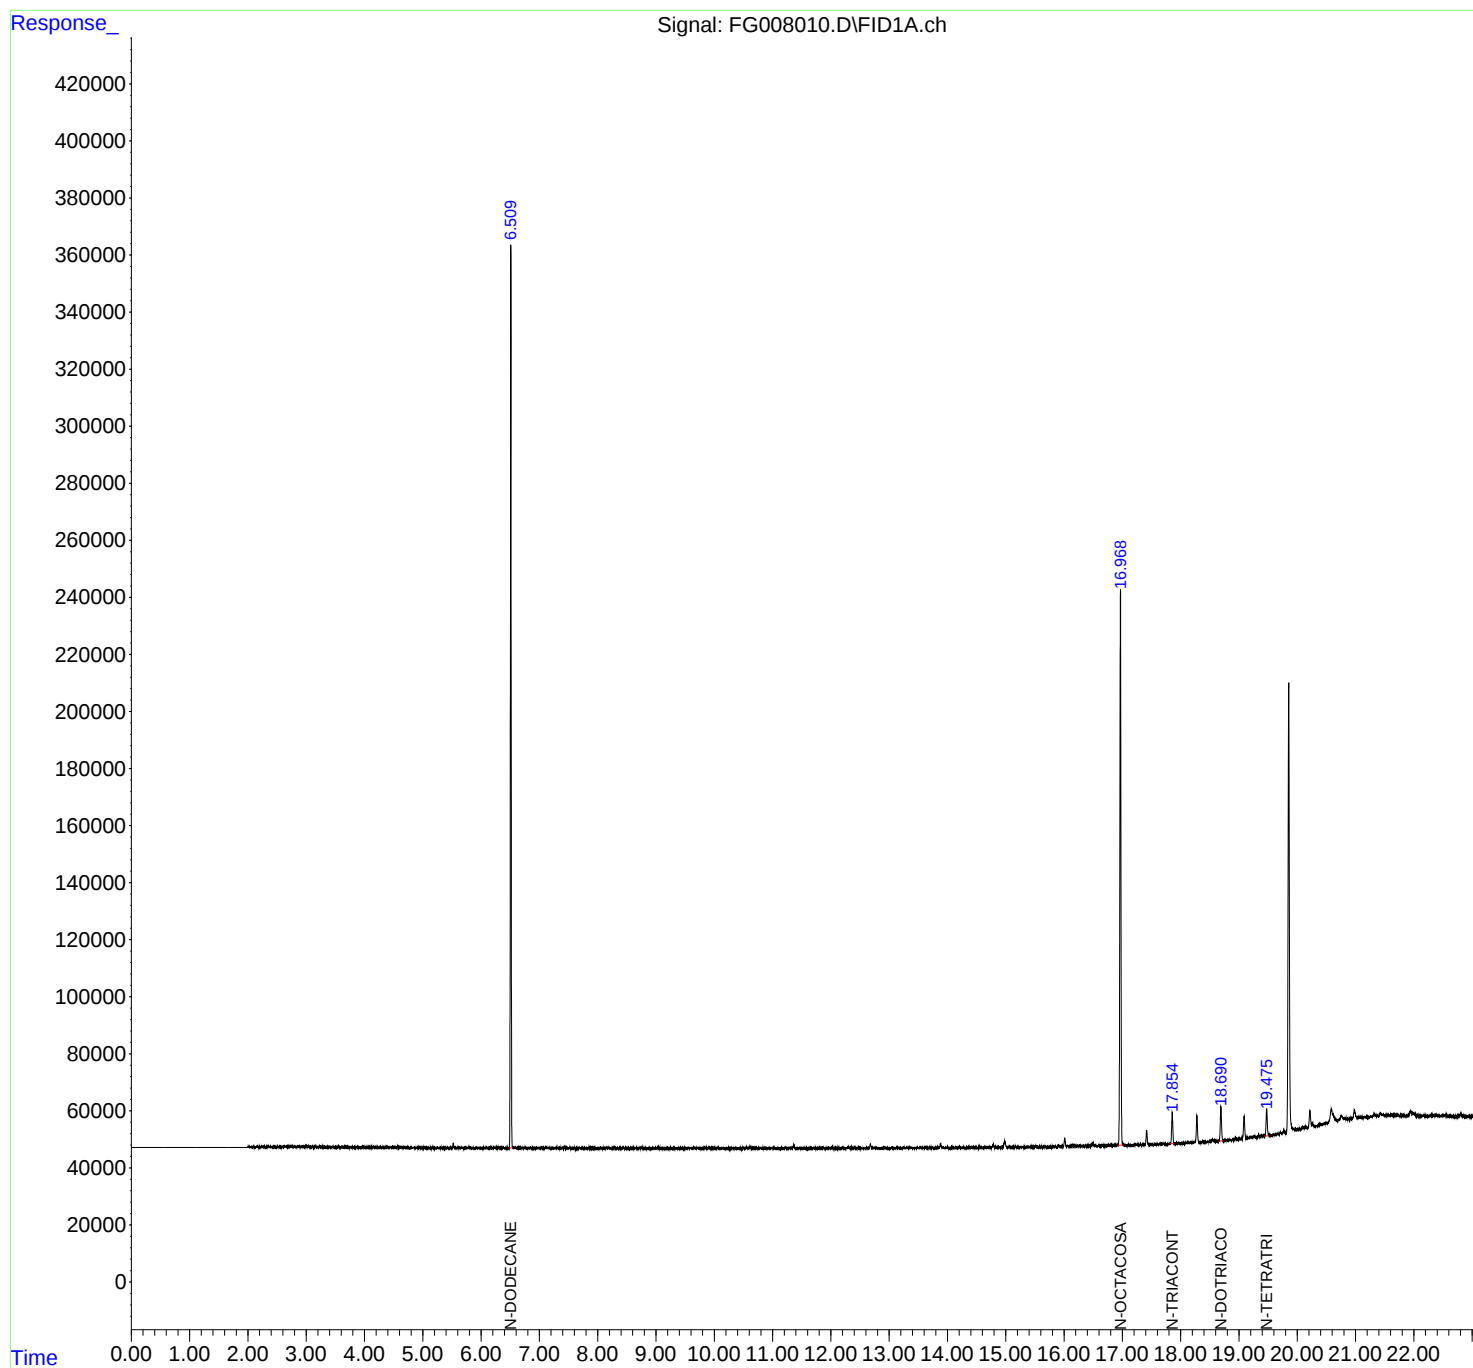


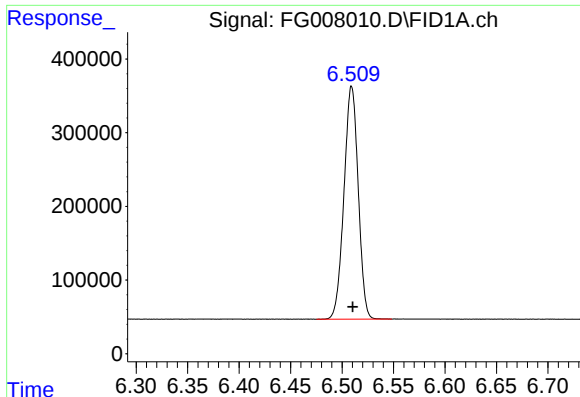

#3 N-DODECANE


R.T.: 6.509 min  
Delta R.T.: -0.001 min  
Response: 3044364  
Conc: 19.90 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

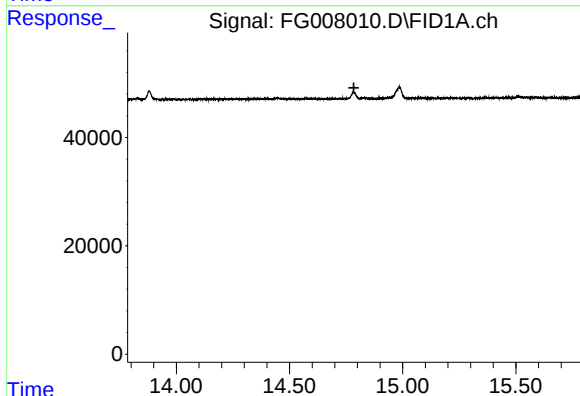


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.784 min  
Response: 0  
Conc: N.D.

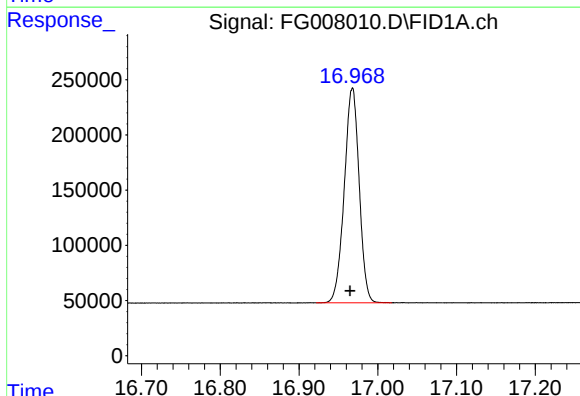


#12 N-OCTACOSANE

R.T.: 16.968 min  
Delta R.T.: 0.003 min  
Response: 2558672  
Conc: 17.47 ug/ml

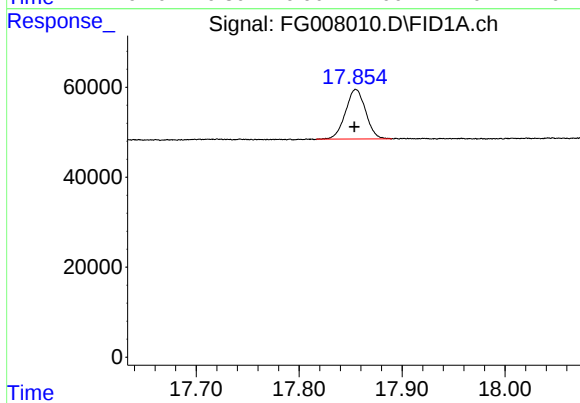

#13 N-TRIACONTANE


R.T.: 17.855 min  
Delta R.T.: 0.002 min  
Response: 150227  
Conc: 1.05 ug/ml

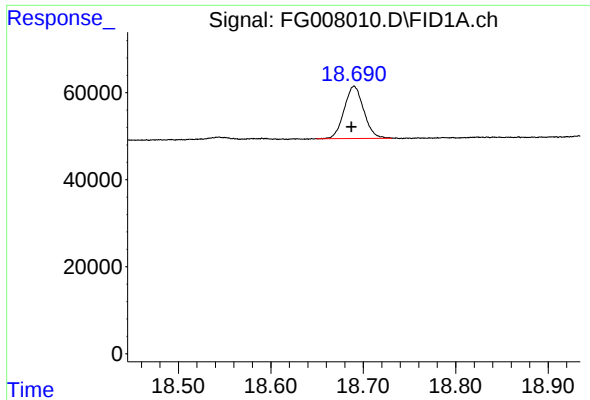

#14 N-DOTRIACONTANE

R.T.: 18.690 min  
Delta R.T.: 0.003 min  
Response: 176417  
Conc: 1.29 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

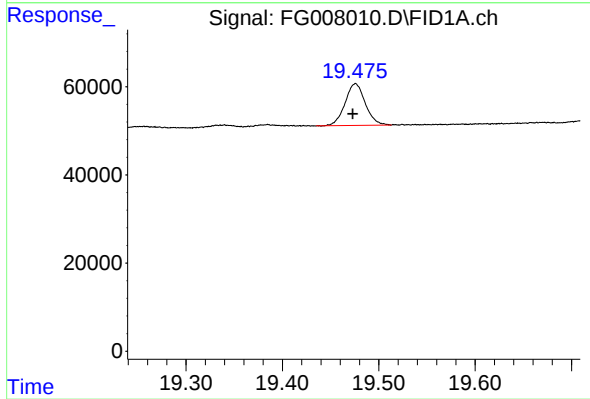

#15 N-TETRATRIACONTANE

R.T.: 19.476 min  
Delta R.T.: 0.003 min  
Response: 137334  
Conc: 1.07 ug/ml