

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050721\
 Data File : FG008017.D
 Signal(s) : FID1A.ch
 Acq On : 07 May 2021 15:20
 Operator : DD\AJ
 Sample : M2325-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 07 23:08:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
 Quant Title :
 QLast Update : Thu Apr 22 01:54:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	2304956	17.314 ug/ml
Target Compounds			
4) N-TETRADECANE	8.281	2508888	16.074 ug/ml
7) N-EICOSANE	12.679	190266	1.228 ug/ml
10) N-TETRACOSANE	14.964	321660	2.114 ug/ml
11) N-HEXACOSANE	16.027	198458	1.332 ug/ml
12) N-OCTACOSANE	16.967	130266	0.890 ug/ml
13) N-TRIACONTANE	17.856	249398	1.745 ug/ml
14) N-DOTRIACONTANE	18.685	716891	5.255 ug/ml
16) N-HEXATRIACONTANE	20.162f	1182940	10.109 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050721\
Data File : FG008017.D
Signal(s) : FID1A.ch
Acq On : 07 May 2021 15:20
Operator : DD\AJ
Sample : M2325-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 07 23:08:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

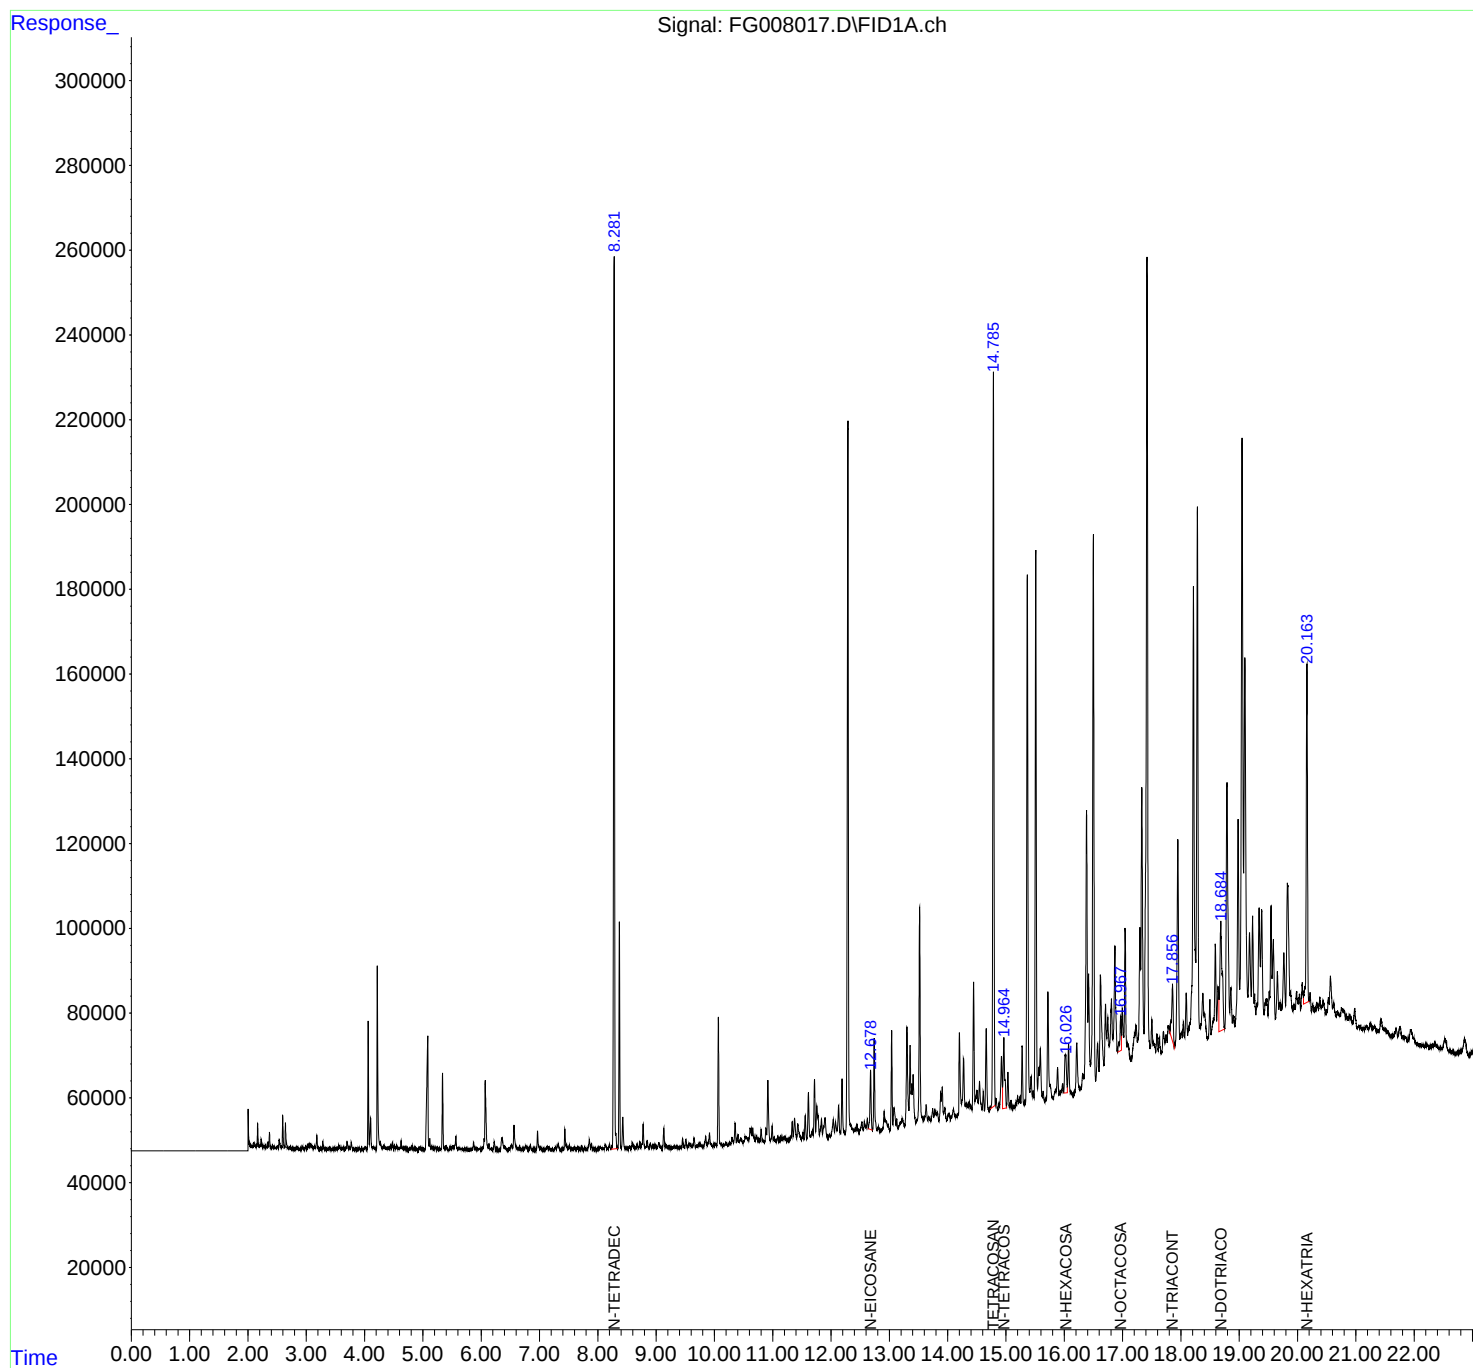


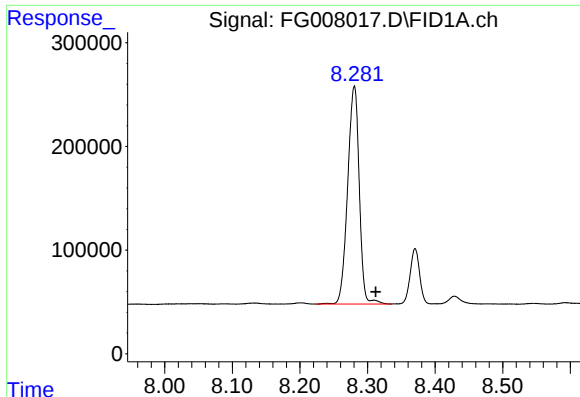

#4 N-TETRADECANE


R.T.: 8.281 min
Delta R.T.: -0.032 min
Response: 2508888
Conc: 16.07 ug/ml

Instrument :
FID_G
ClientSampleId :

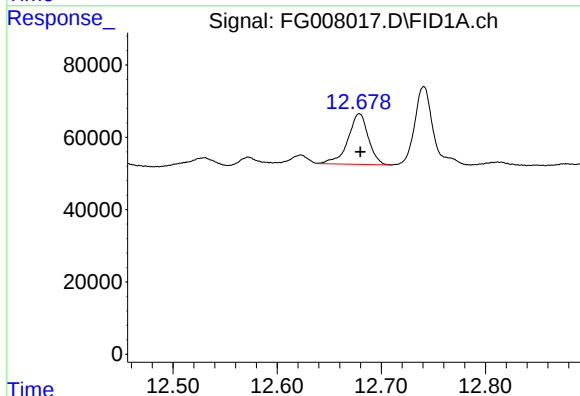


#7 N-EICOSANE

R.T.: 12.679 min
Delta R.T.: 0.000 min
Response: 190266
Conc: 1.23 ug/ml

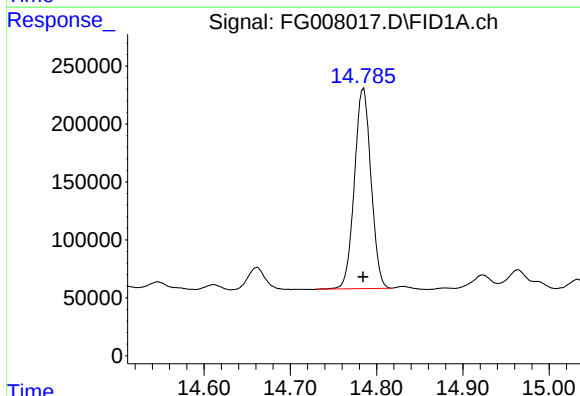


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 2304956
Conc: 17.31 ug/ml

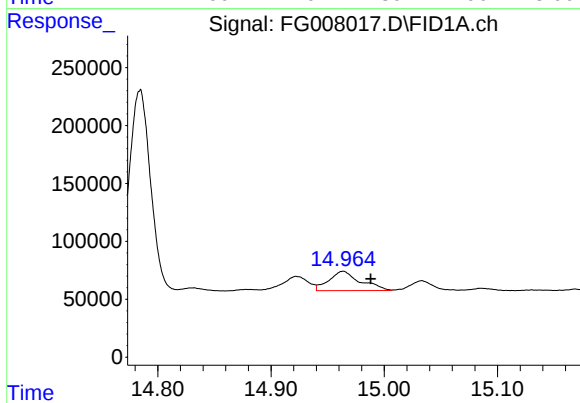

#10 N-TETRACOSANE


R.T.: 14.964 min
Delta R.T.: -0.024 min
Response: 321660
Conc: 2.11 ug/ml

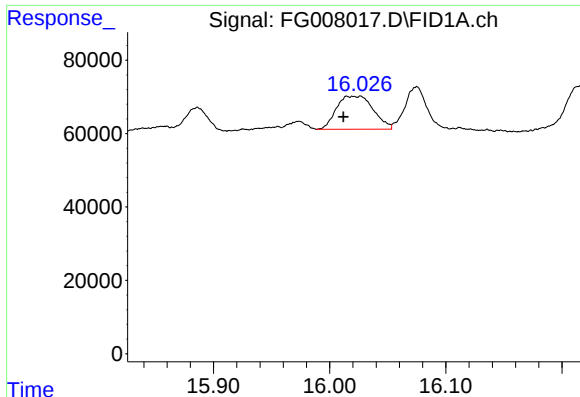

#11 N-HEXACOSANE


R.T.: 16.027 min
Delta R.T.: 0.015 min
Response: 198458
Conc: 1.33 ug/ml

Instrument :
FID_G
ClientSampleId :

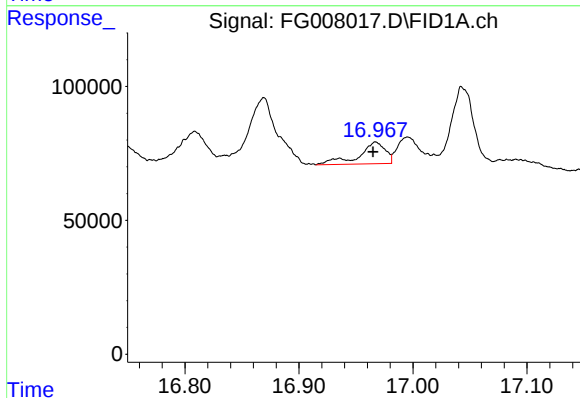


#12 N-OCTACOSANE

R.T.: 16.967 min
Delta R.T.: 0.003 min
Response: 130266
Conc: 0.89 ug/ml

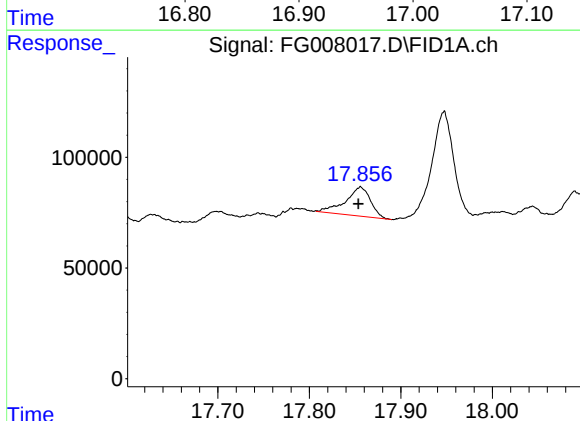


#13 N-TRIACONTANE

R.T.: 17.856 min
Delta R.T.: 0.002 min
Response: 249398
Conc: 1.74 ug/ml

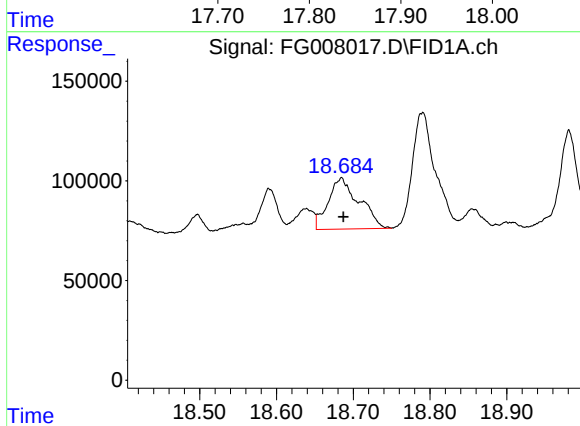

#14 N-DOTRIACONTANE

R.T.: 18.685 min
Delta R.T.: -0.002 min
Response: 716891
Conc: 5.25 ug/ml

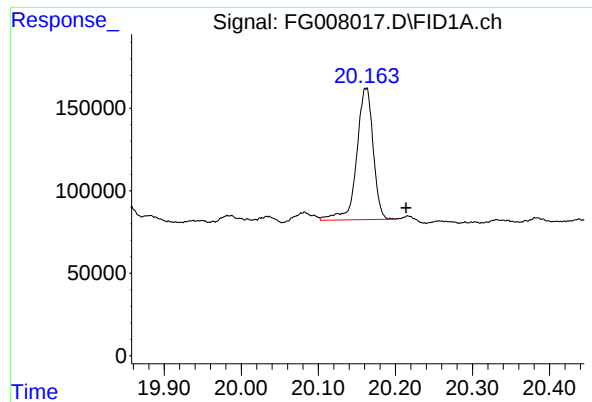

#16 N-HEXATRIACONTANE

R.T.: 20.162 min
Delta R.T.: -0.052 min
Response: 1182940
Conc: 10.11 ug/ml

Instrument :
FID_G
ClientSampleId :