

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050721\
Data File : FG008021.D
Signal(s) : FID1A.ch
Acq On : 07 May 2021 17:24
Operator : DD\AJ
Sample : PB136244BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB136244BL

Integration File: autoint1.e
Quant Time: May 07 23:09:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	2023319	15.198 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050721\
Data File : FG008021.D
Signal(s) : FID1A.ch
Acq On : 07 May 2021 17:24
Operator : DD\AJ
Sample : PB136244BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB136244BL

Integration File: autoint1.e
Quant Time: May 07 23:09:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

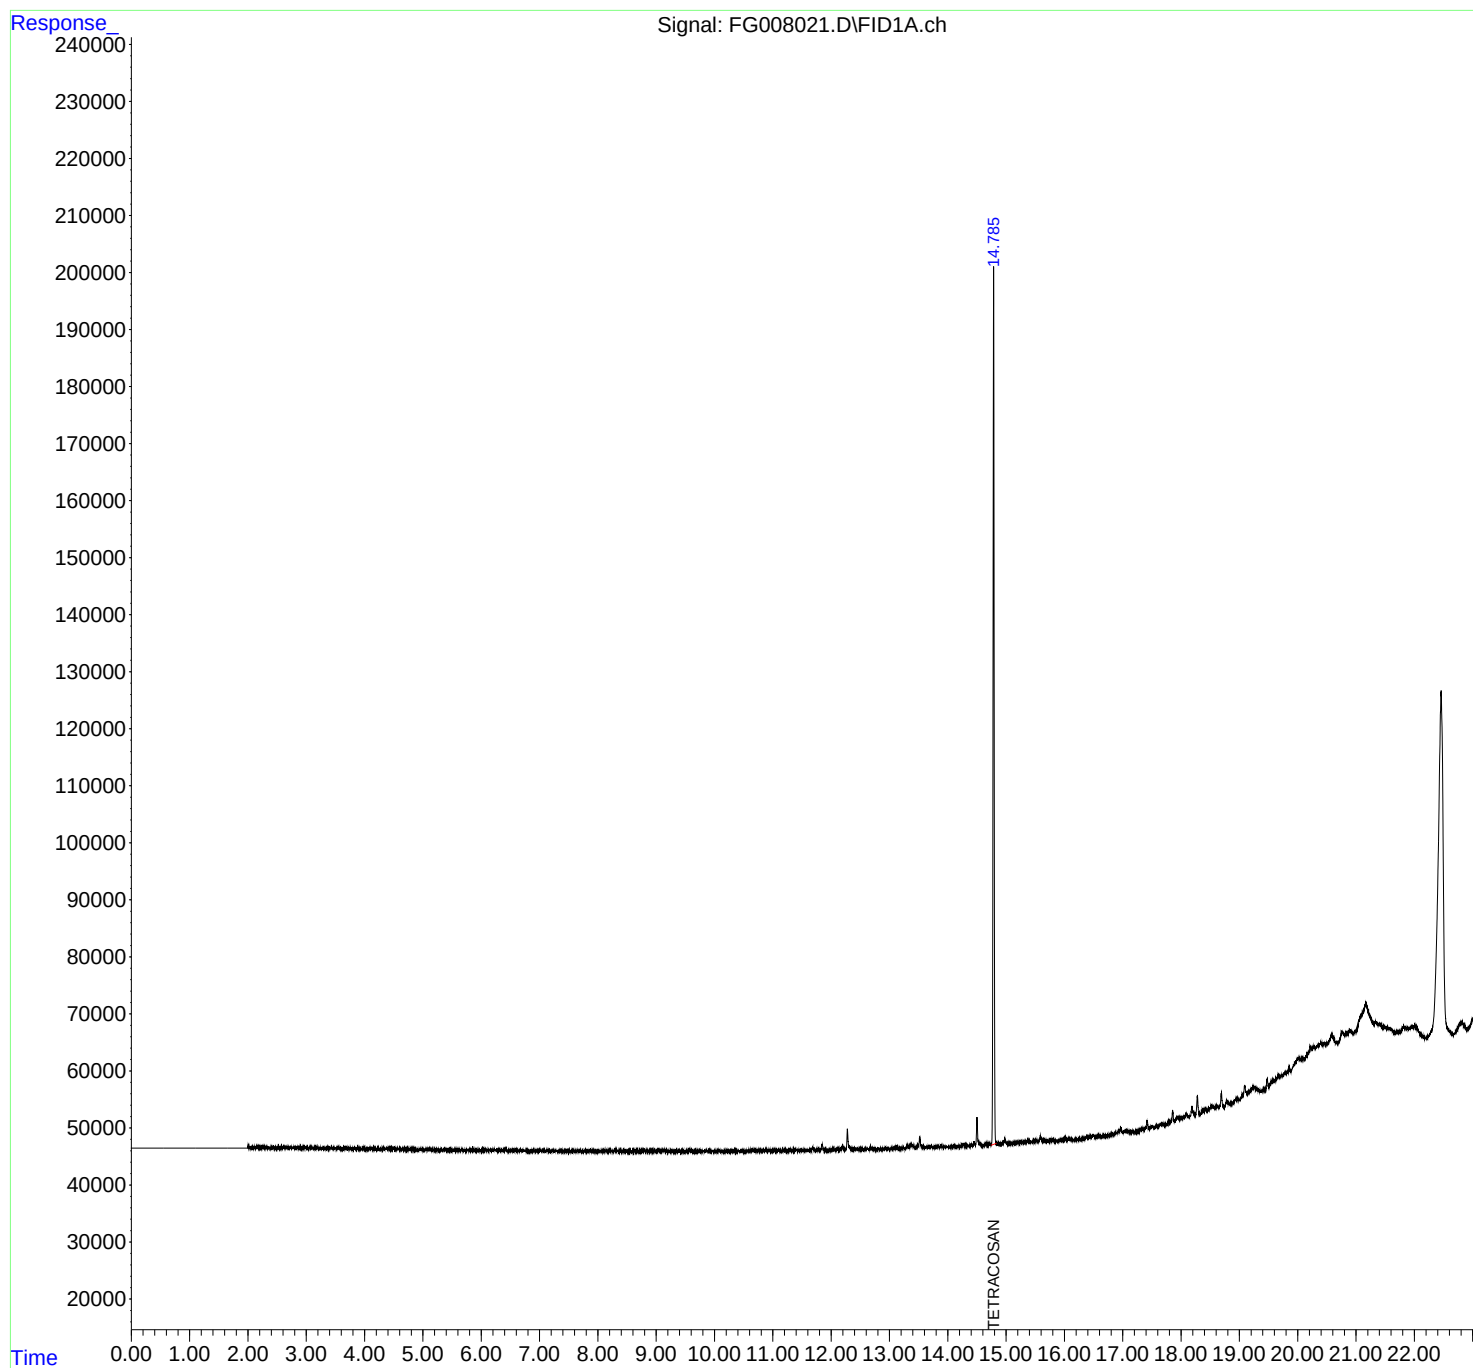

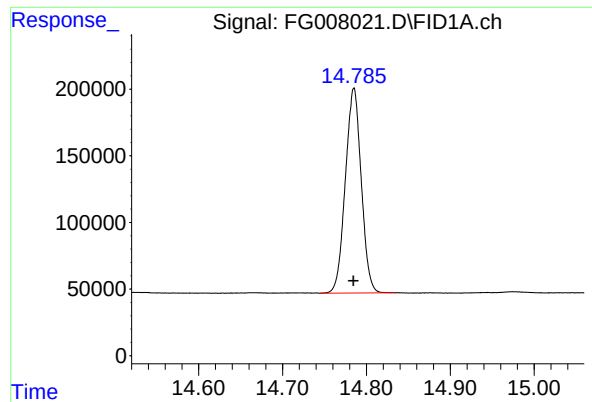

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 2023319
Conc: 15.20 ug/ml

Instrument :
FID_G
ClientSampleId :
PB136244BL