

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004902.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 11:38
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 14:01:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:01:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
12) N-OCTACOSANE	16.959	38781	0.309 ug/ml
13) N-TRIACONTANE	17.849	92511	0.755 ug/ml
14) N-DOTRIACONTANE	18.685	77762	0.664 ug/ml
15) N-TETRATRIACONTANE	19.470	47765	0.430 ug/ml
16) N-HEXATRIACONTANE	20.211	42833	0.405 ug/ml
17) N-OCTATRIACONTANE	20.977	25735	0.266 ug/ml
18) N-TETRACONTANE	21.992f	724219	7.450 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004902.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 11:38
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: May 09 14:01:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:01:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

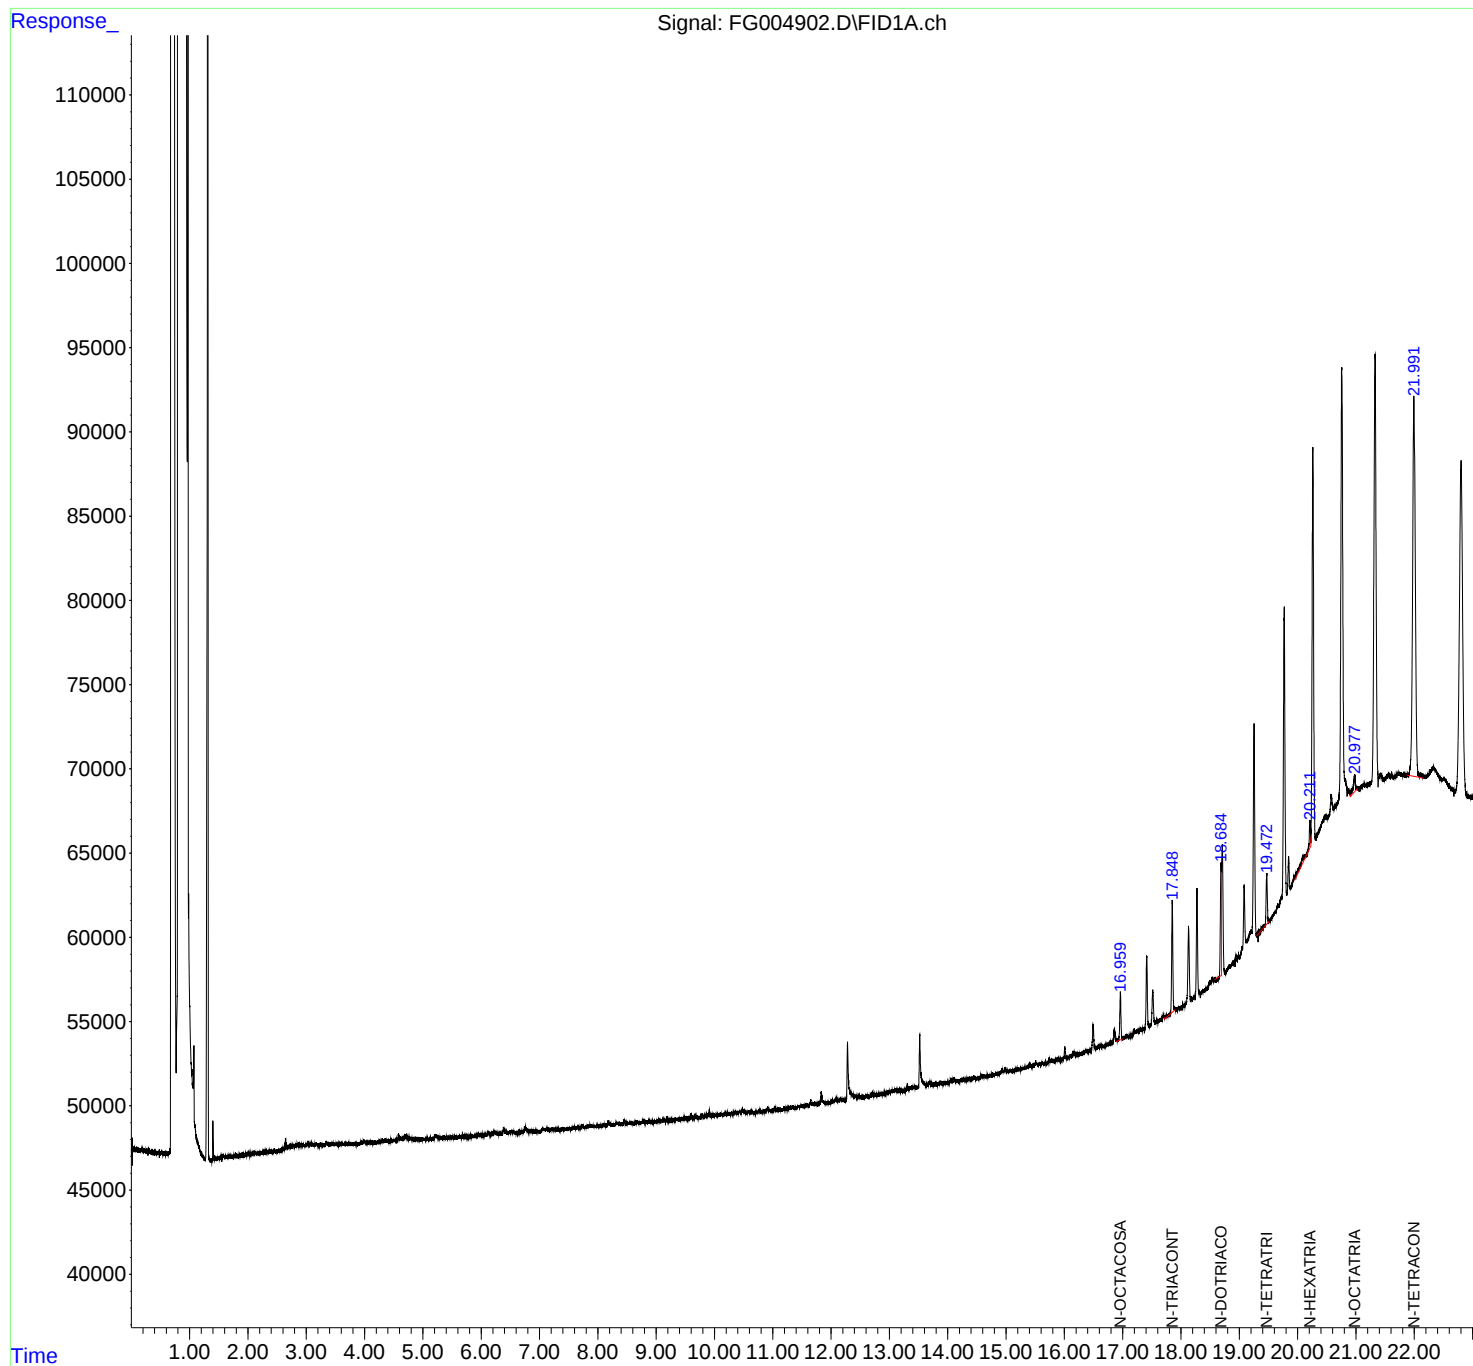


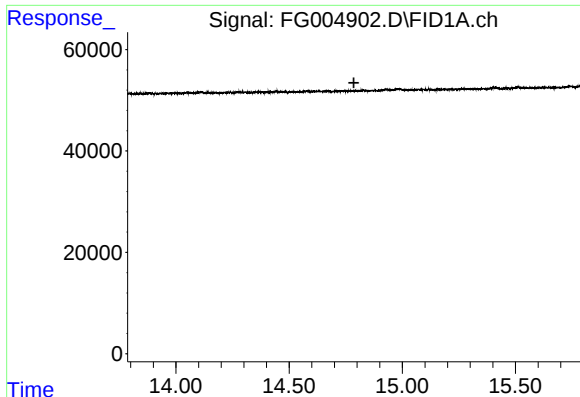

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.786 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

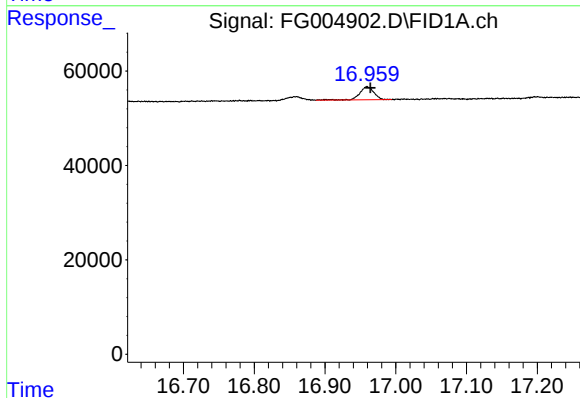


#12 N-OCTACOSANE

R.T.: 16.959 min
Delta R.T.: -0.005 min
Response: 38781
Conc: 0.31 ug/ml

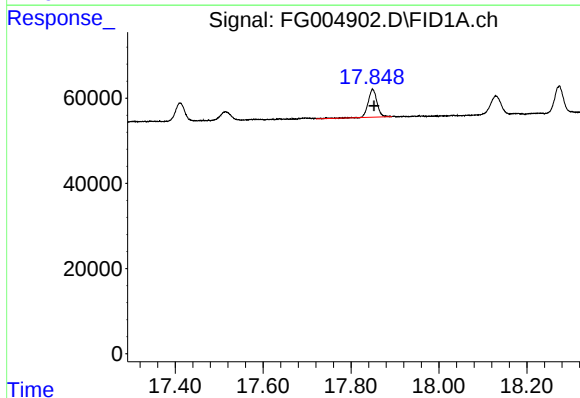


#13 N-TRIACONTANE

R.T.: 17.849 min
Delta R.T.: -0.004 min
Response: 92511
Conc: 0.76 ug/ml

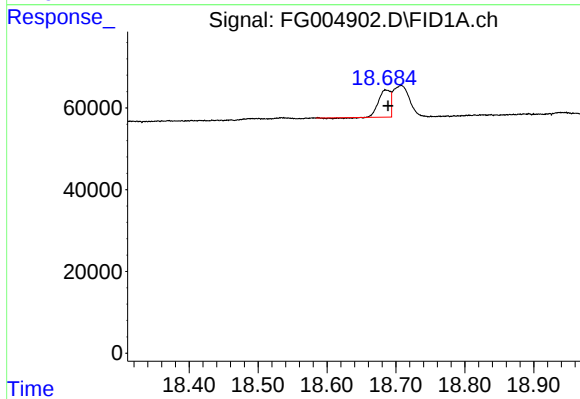

#14 N-DOTRIACONTANE


R.T.: 18.685 min
Delta R.T.: -0.004 min
Response: 77762
Conc: 0.66 ug/ml

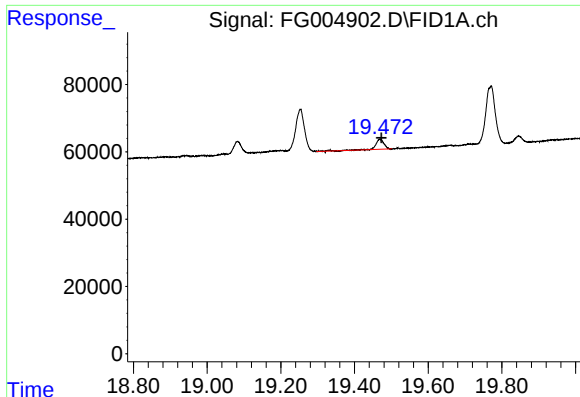

#15 N-TETRATRIACONTANE


R.T.: 19.470 min
Delta R.T.: -0.003 min
Response: 47765
Conc: 0.43 ug/ml

Instrument :
FID_G
ClientSampleId :

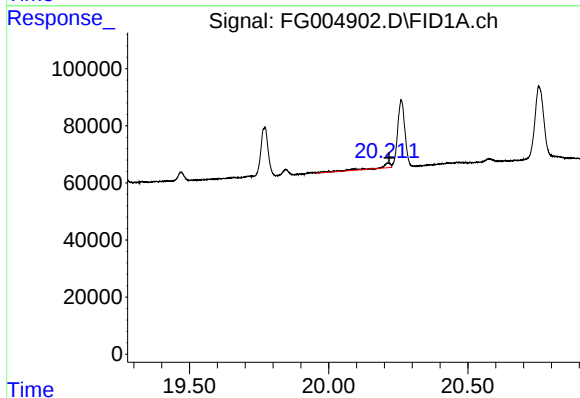


#16 N-HEXATRIACONTANE

R.T.: 20.211 min
Delta R.T.: -0.006 min
Response: 42833
Conc: 0.40 ug/ml

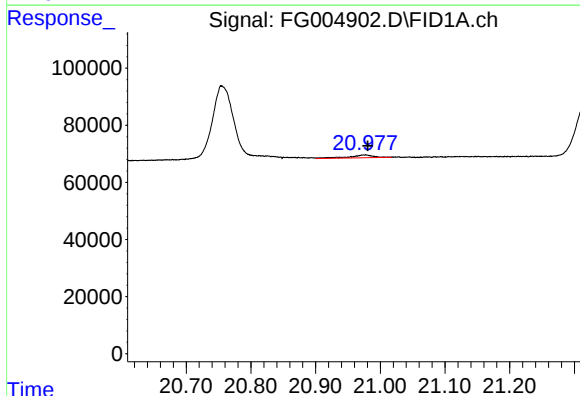

#17 N-OCTATRIACONTANE

R.T.: 20.977 min
Delta R.T.: -0.004 min
Response: 25735
Conc: 0.27 ug/ml

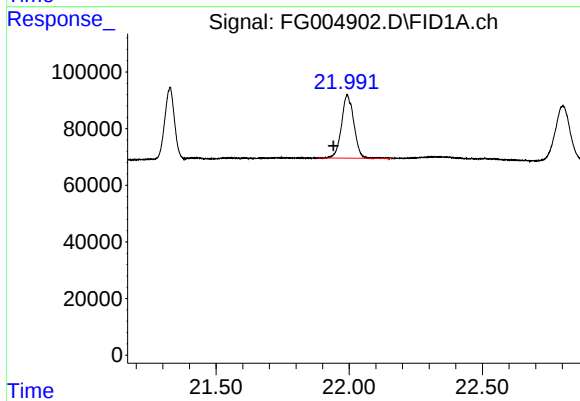

#18 N-TETRACONTANE

R.T.: 21.992 min
Delta R.T.: 0.051 min
Response: 724219
Conc: 7.45 ug/ml