

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG050919\  
Data File : FG004902.D  
Signal(s) : FID1A.ch  
Acq On : 09 May 2019 11:38  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
MECL2

Integration File: autoint1.e  
Quant Time: May 09 14:01:47 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG050919.M  
Quant Title :  
QLast Update : Thu May 09 14:01:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.    | Response | Conc Units  |
|-----------------------------|---------|----------|-------------|
| -----                       |         |          |             |
| System Monitoring Compounds |         |          |             |
| Target Compounds            |         |          |             |
| 12) N-OCTACOSANE            | 16.959  | 38781    | 0.309 ug/ml |
| 13) N-TRIACONTANE           | 17.849  | 92511    | 0.755 ug/ml |
| 14) N-DOTRIACONTANE         | 18.685  | 77762    | 0.664 ug/ml |
| 15) N-TETRATRIACONTANE      | 19.470  | 47765    | 0.430 ug/ml |
| 16) N-HEXATRIACONTANE       | 20.211  | 42833    | 0.405 ug/ml |
| 17) N-OCTATRIACONTANE       | 20.977  | 25735    | 0.266 ug/ml |
| 18) N-TETRACONTANE          | 21.992f | 724219   | 7.450 ug/ml |
| -----                       |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG050919\  
Data File : FG004902.D  
Signal(s) : FID1A.ch  
Acq On : 09 May 2019 11:38  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampled :  
MECL2

Integration File: autoint1.e  
Quant Time: May 09 14:01:47 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG050919.M  
Quant Title :  
QLast Update : Thu May 09 14:01:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

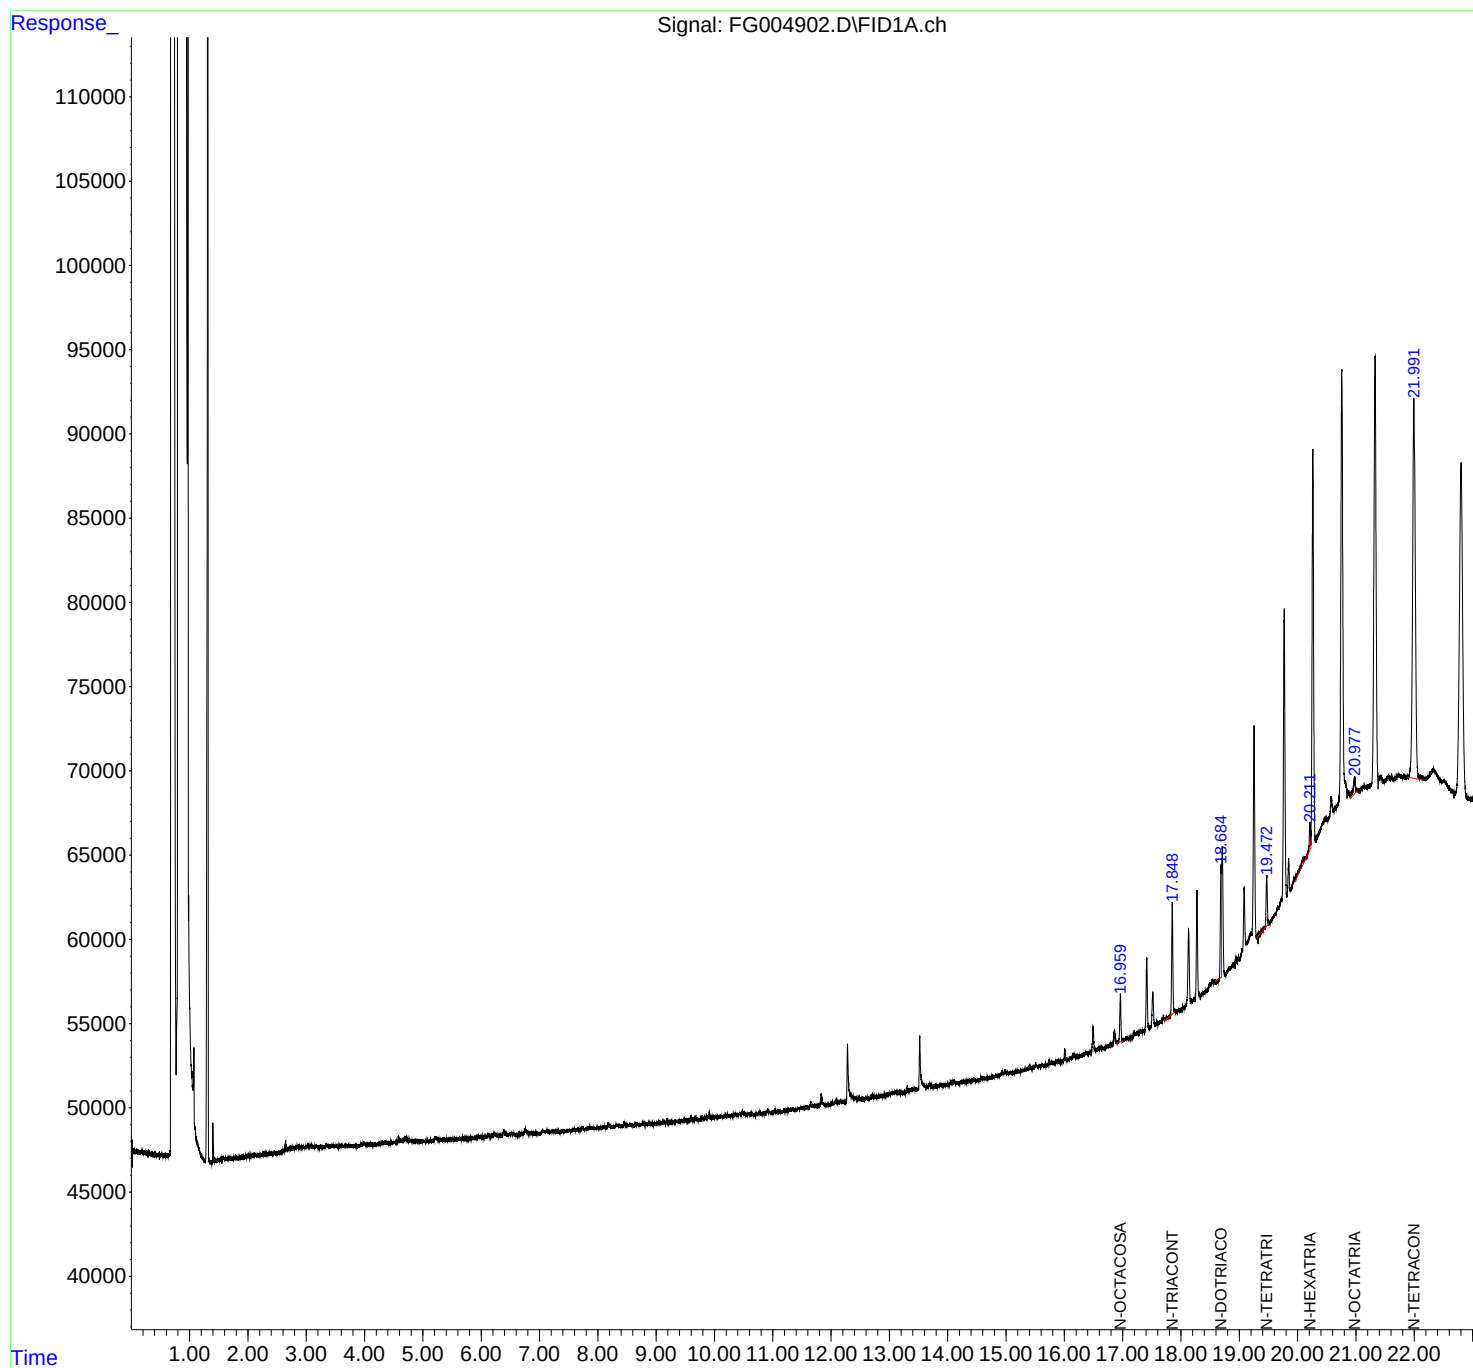


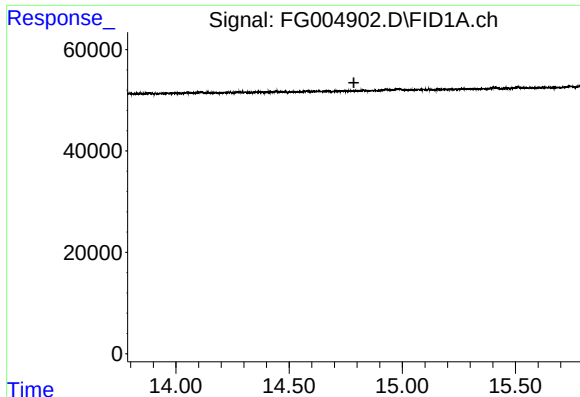

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 14.786 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_G  
ClientSampleId :  
MECL2

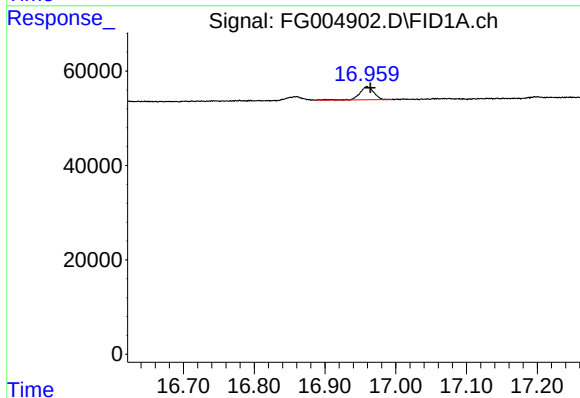


#12 N-OCTACOSANE

R.T.: 16.959 min  
Delta R.T.: -0.005 min  
Response: 38781  
Conc: 0.31 ug/ml

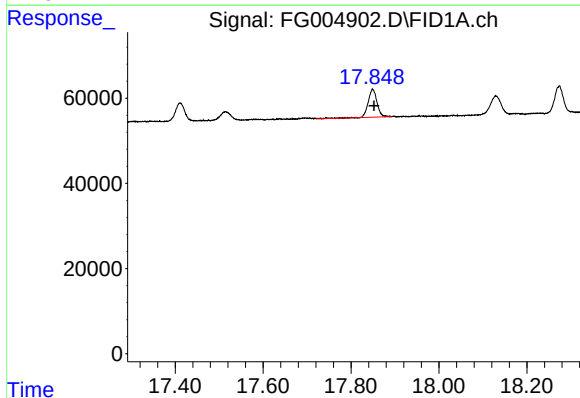


#13 N-TRIACONTANE

R.T.: 17.849 min  
Delta R.T.: -0.004 min  
Response: 92511  
Conc: 0.76 ug/ml

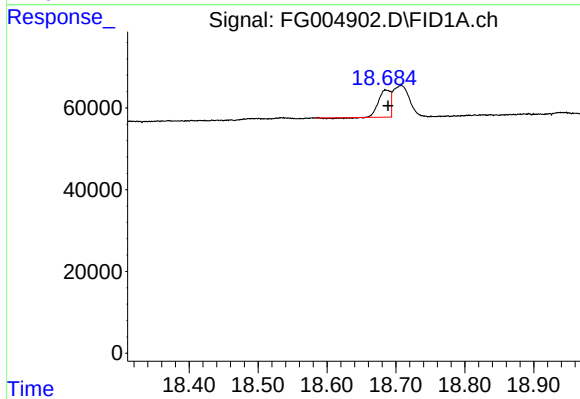

#14 N-DOTRIACONTANE


R.T.: 18.685 min  
Delta R.T.: -0.004 min  
Response: 77762  
Conc: 0.66 ug/ml

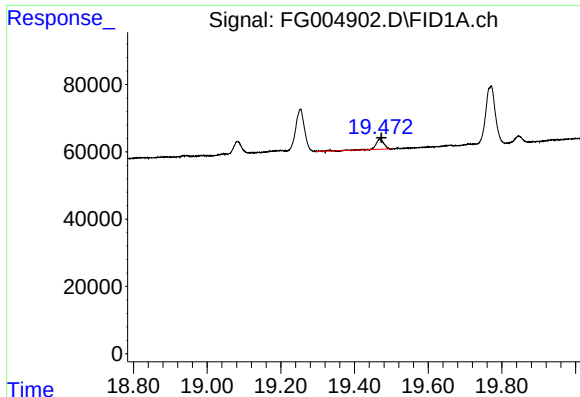

#15 N-TETRATRIACONTANE


R.T.: 19.470 min  
Delta R.T.: -0.003 min  
Response: 47765  
Conc: 0.43 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
MECL2

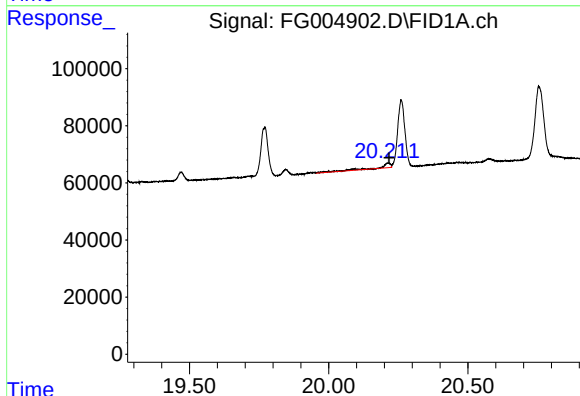


#16 N-HEXATRIACONTANE

R.T.: 20.211 min  
Delta R.T.: -0.006 min  
Response: 42833  
Conc: 0.40 ug/ml

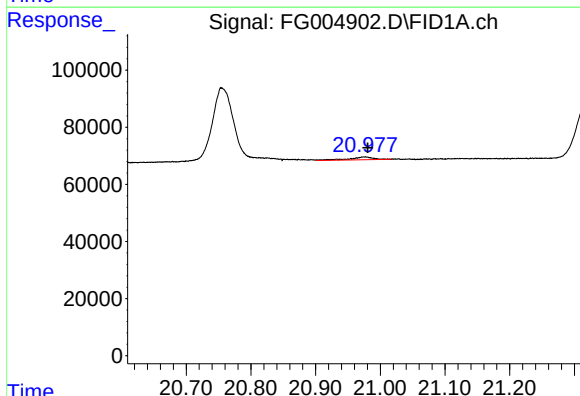

#17 N-OCTATRIACONTANE

R.T.: 20.977 min  
Delta R.T.: -0.004 min  
Response: 25735  
Conc: 0.27 ug/ml

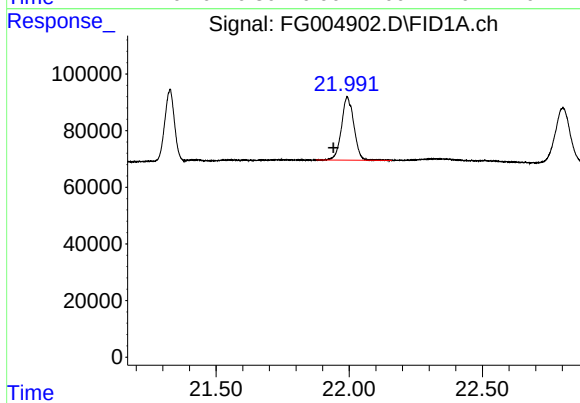

#18 N-TETRACONTANE

R.T.: 21.992 min  
Delta R.T.: 0.051 min  
Response: 724219  
Conc: 7.45 ug/ml