

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004903.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 12:07
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 14:01:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:01:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.782	2422527	20.332 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.848	51967	0.424 ug/ml
14) N-DOTRIACONTANE	18.683	46487	0.397 ug/ml
15) N-TETRATRIACONTANE	19.470	21084	0.190 ug/ml
16) N-HEXATRIACONTANE	20.213	38451	0.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004903.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 12:07
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 14:01:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:01:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

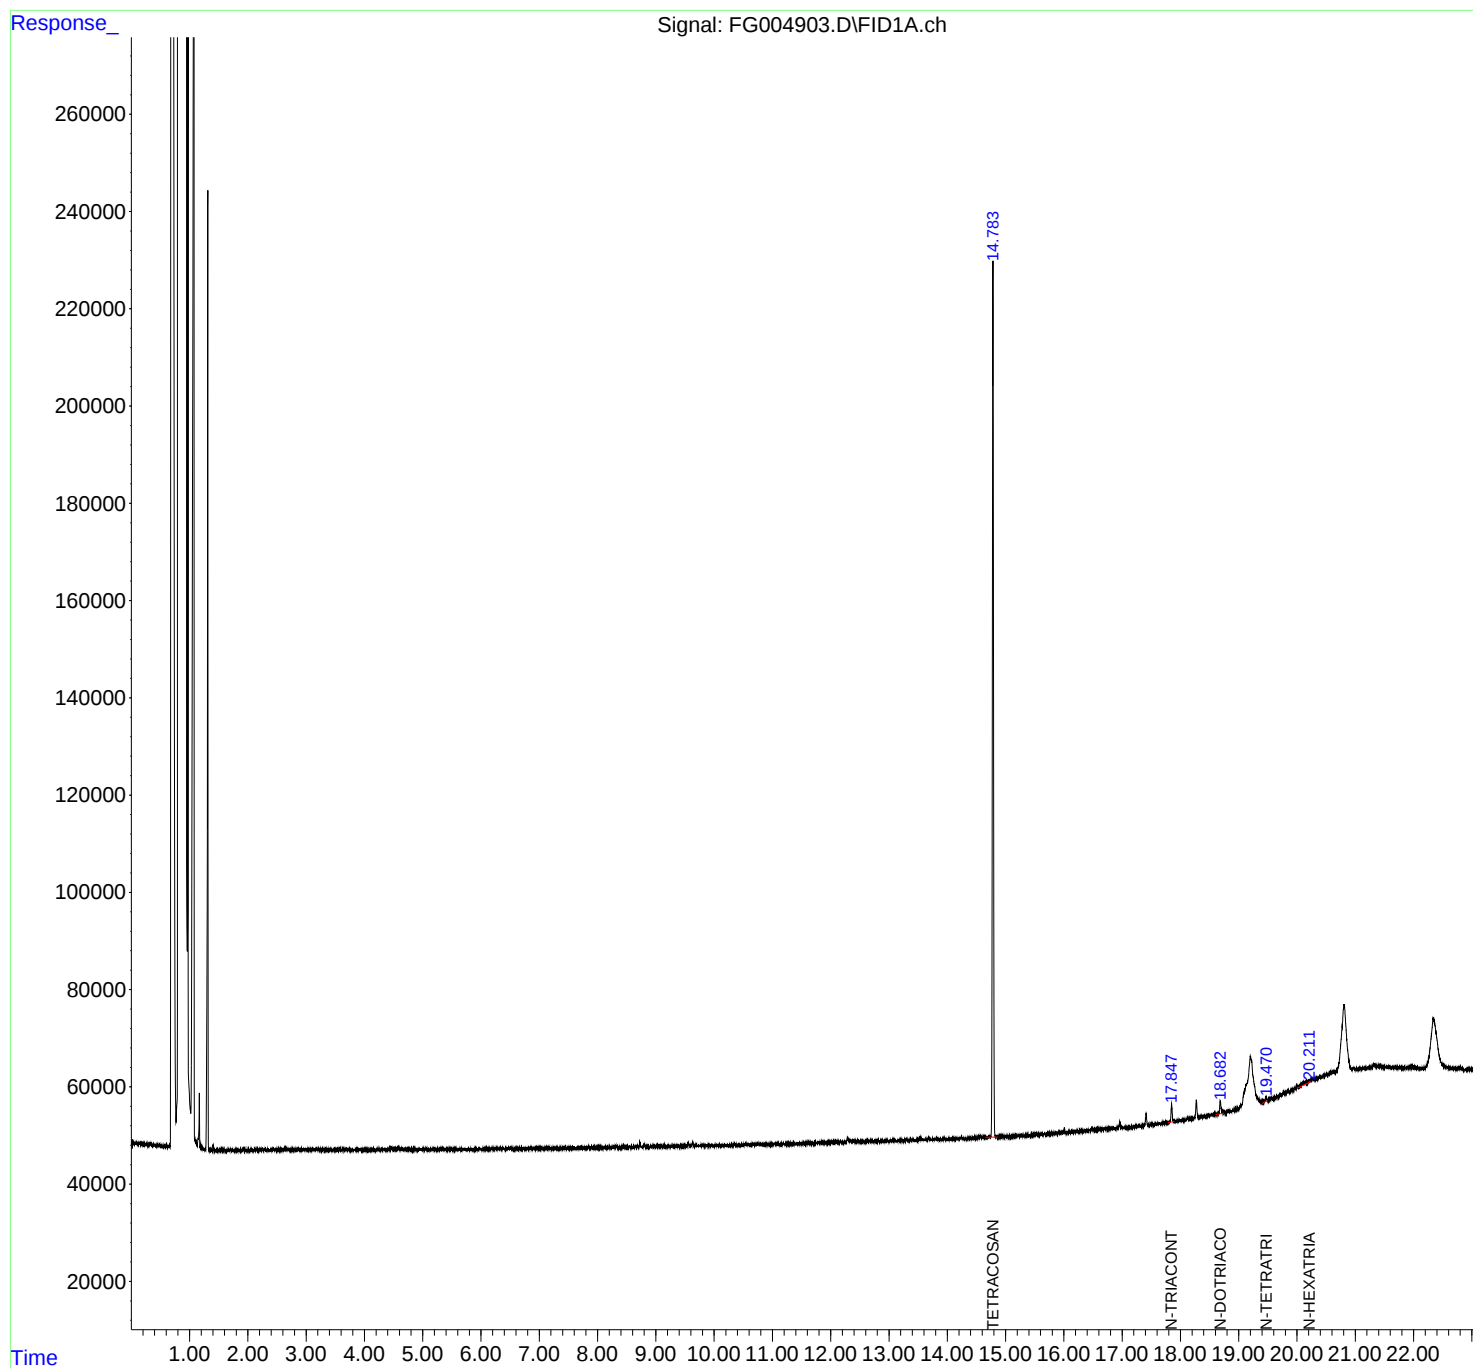


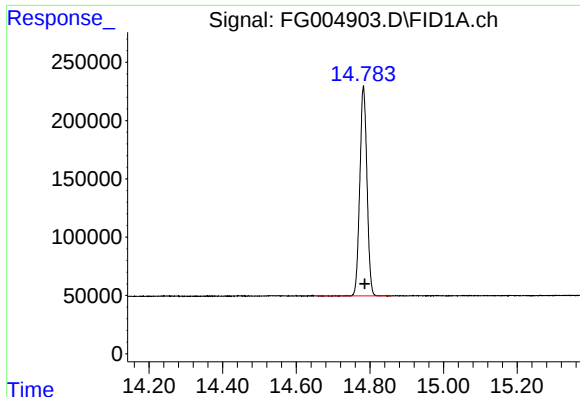

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.782 min
Delta R.T.: -0.004 min
Response: 2422527
Conc: 20.33 ug/ml

Instrument :
FID_G
ClientSampleId :

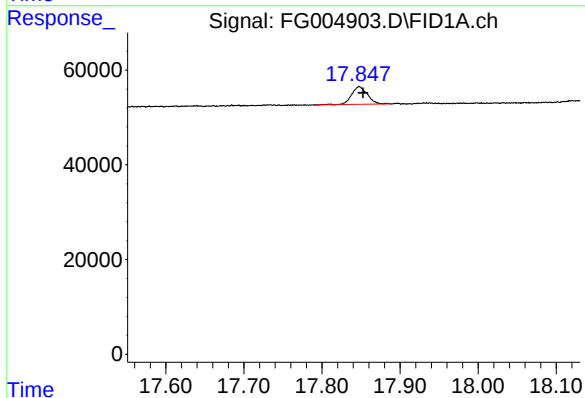


#13 N-TRIACONTANE

R.T.: 17.848 min
Delta R.T.: -0.005 min
Response: 51967
Conc: 0.42 ug/ml

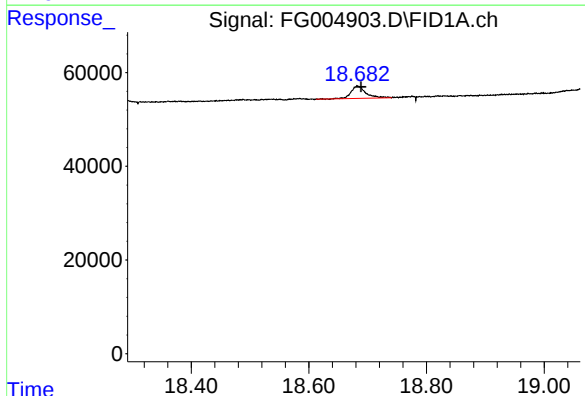


#14 N-DOTRIACONTANE

R.T.: 18.683 min
Delta R.T.: -0.006 min
Response: 46487
Conc: 0.40 ug/ml

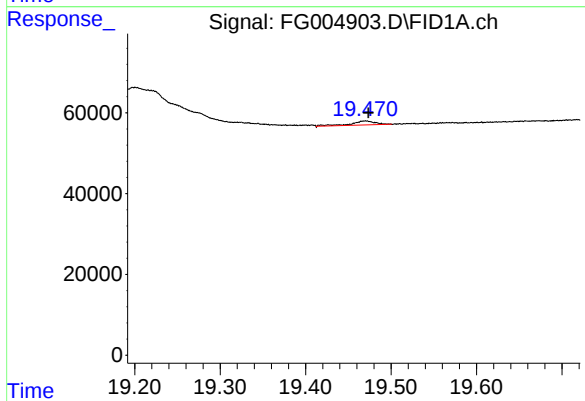

#15 N-TETRATRIACONTANE

R.T.: 19.470 min
Delta R.T.: -0.003 min
Response: 21084
Conc: 0.19 ug/ml

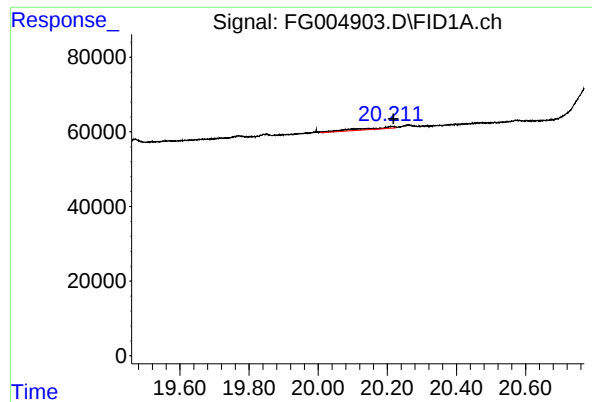

#16 N-HEXATRIACONTANE

R.T.: 20.213 min
Delta R.T.: -0.004 min
Response: 38451
Conc: 0.36 ug/ml

Instrument :
FID_G
ClientSampleId :