

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
 Data File : FG004910.D
 Signal(s) : FID1A.ch
 Acq On : 09 May 2019 15:35
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 10 00:44:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	2410480	20.086 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.852	63417	0.505 ug/ml
14) N-DOTRIACONTANE	18.687	59743	0.499 ug/ml
16) N-HEXATRIACONTANE	20.218	28782	0.271 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004910.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 15:35
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 00:44:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

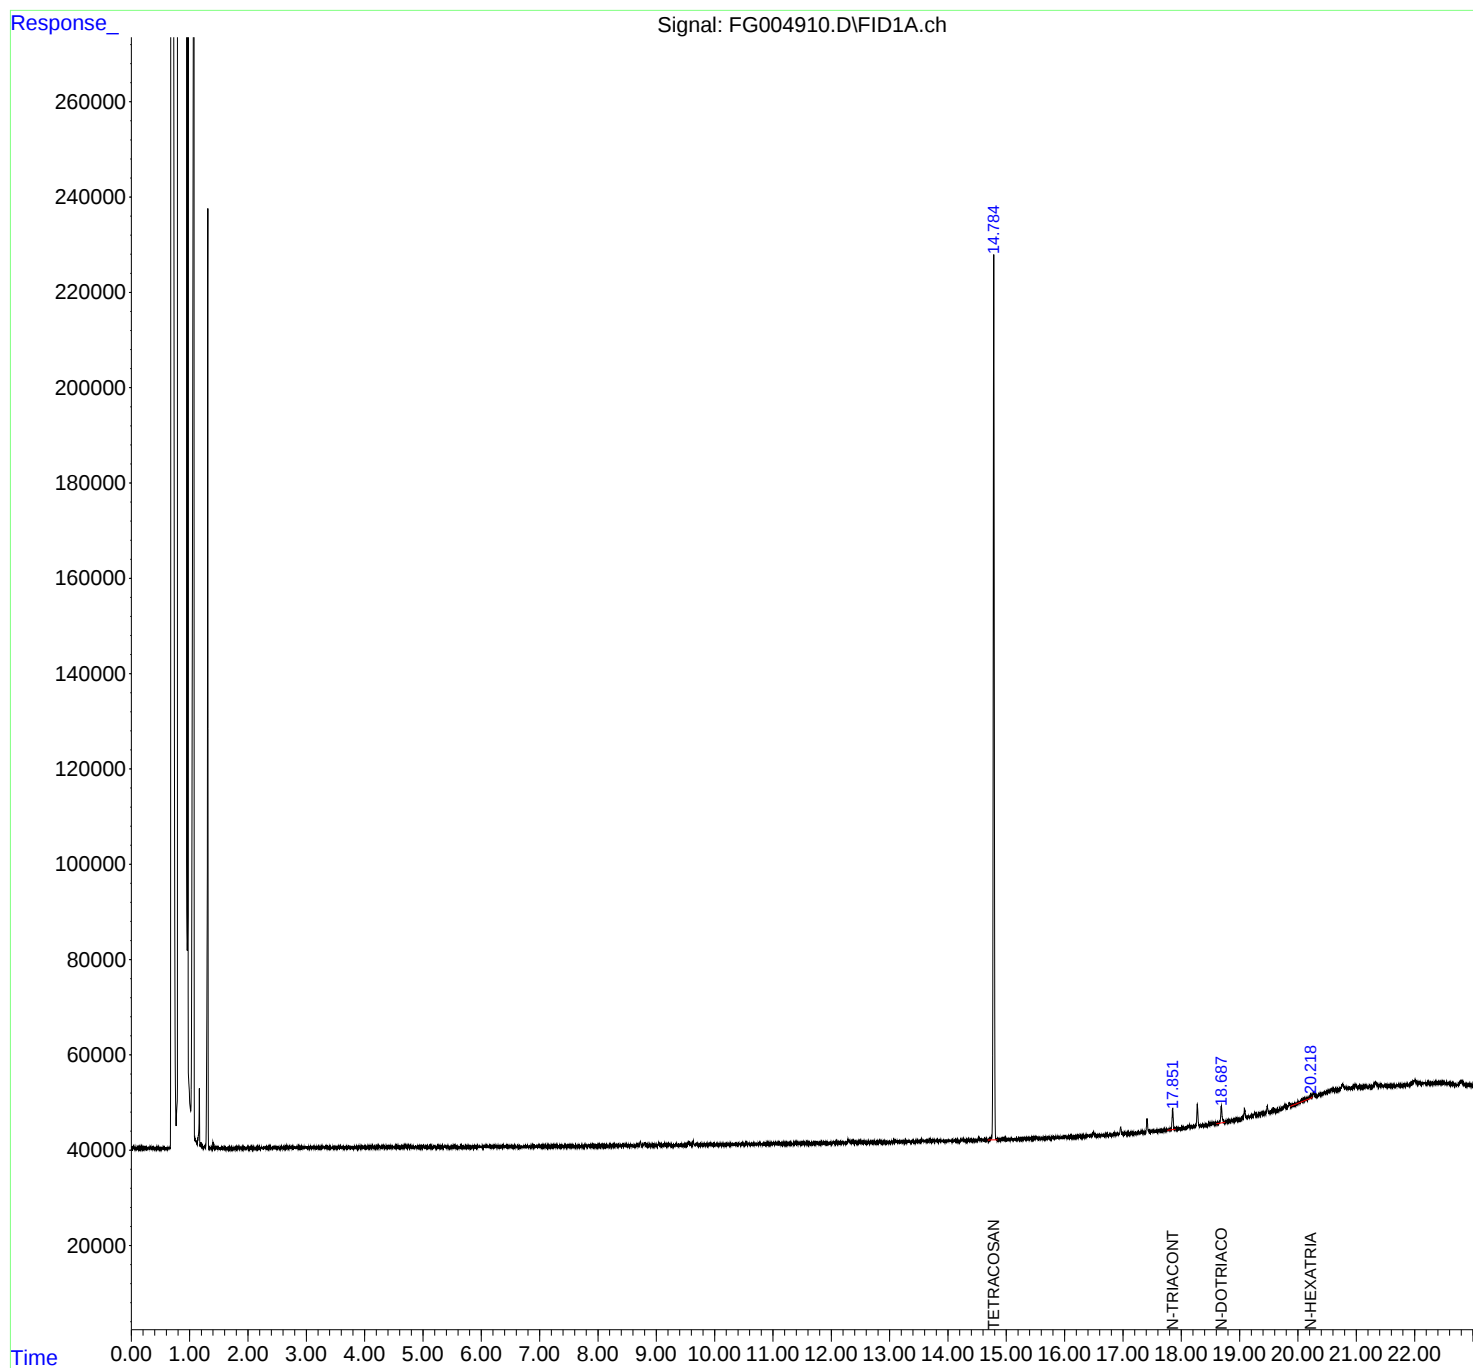


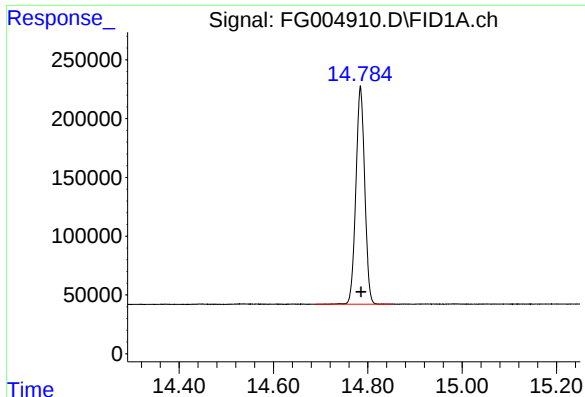

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.785 min
Delta R.T.: -0.002 min
Response: 2410480
Conc: 20.09 ug/ml

Instrument :
FID_G
ClientSampleId :

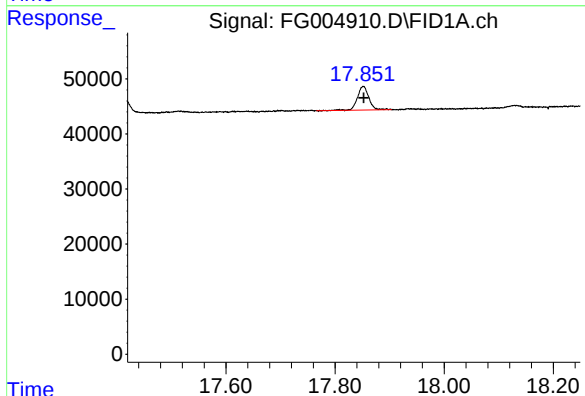


#13 N-TRIACONTANE

R.T.: 17.852 min
Delta R.T.: 0.000 min
Response: 63417
Conc: 0.50 ug/ml

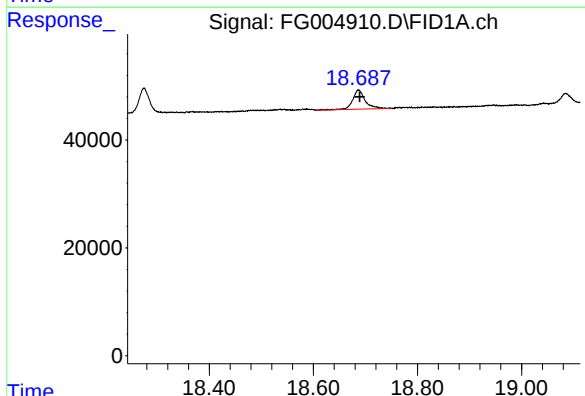

#14 N-DOTRIACONTANE

R.T.: 18.687 min
Delta R.T.: -0.002 min
Response: 59743
Conc: 0.50 ug/ml

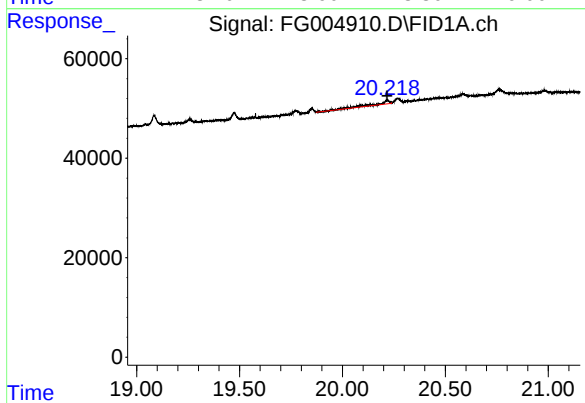

#16 N-HEXATRIACONTANE

R.T.: 20.218 min
Delta R.T.: 0.000 min
Response: 28782
Conc: 0.27 ug/ml