

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004912.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 16:33
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 10 00:44:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.514	3119002	21.740 ug/ml
12)	N-OCTACOSANE	16.963	2845692	22.386 ug/ml
13)	N-TRIACONTANE	17.850	97047	0.772 ug/ml
14)	N-DOTRIACONTANE	18.684	78005	0.651 ug/ml
15)	N-TETRATRIACONTANE	19.469	45818	0.407 ug/ml
16)	N-HEXATRIACONTANE	20.214	46108	0.435 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004912.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 16:33
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 10 00:44:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

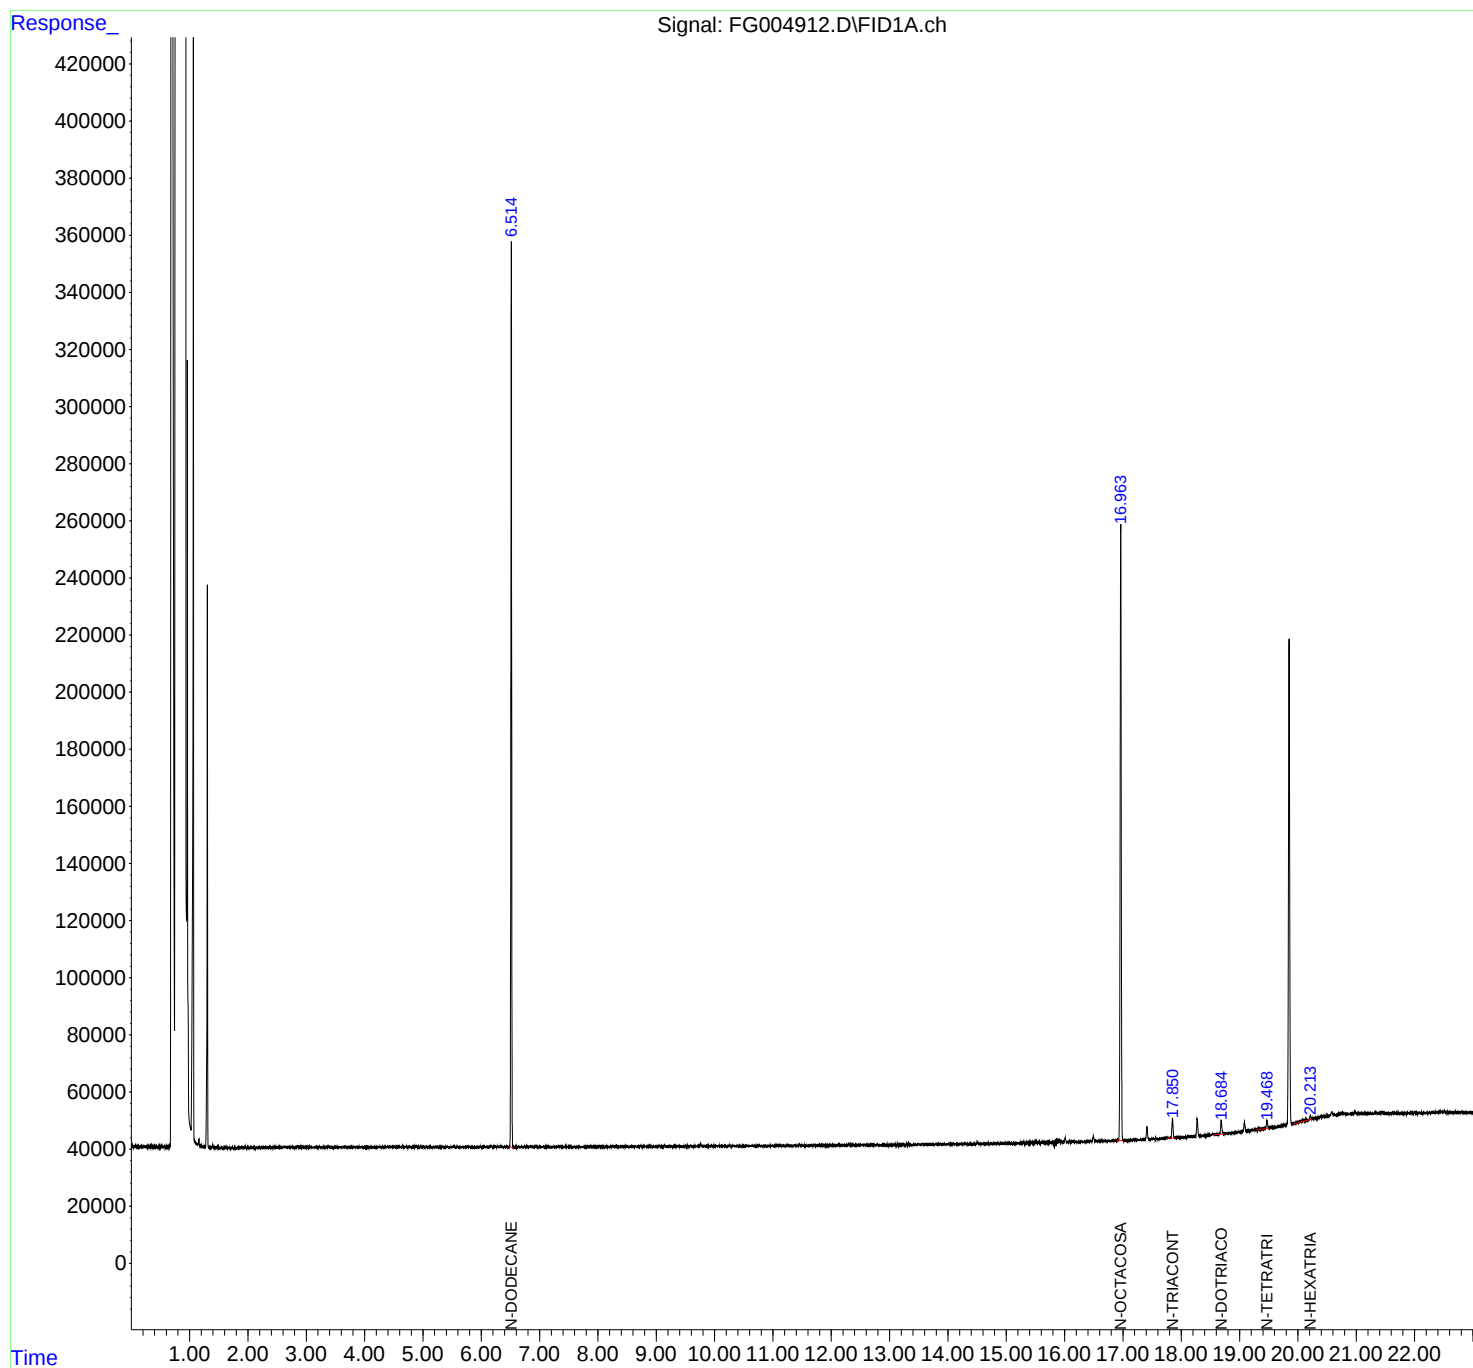


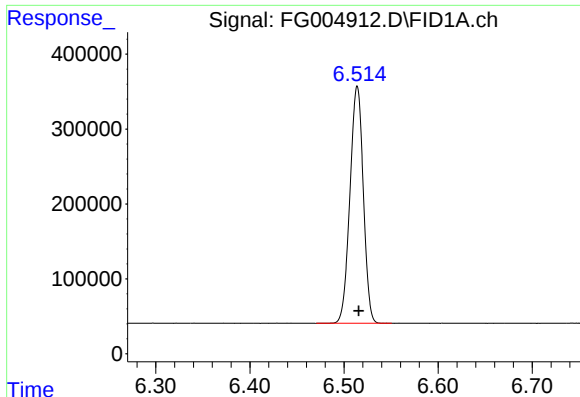

#3 N-DODECANE


R.T.: 6.514 min
Delta R.T.: -0.002 min
Response: 3119002
Conc: 21.74 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

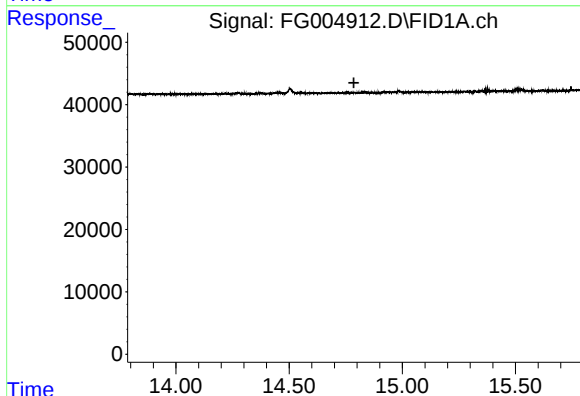


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

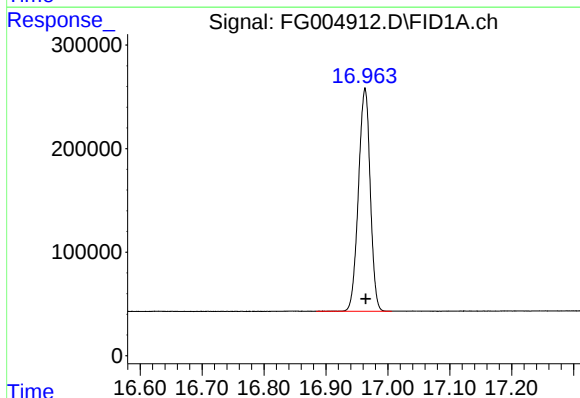


#12 N-OCTACOSANE

R.T.: 16.963 min
Delta R.T.: -0.001 min
Response: 2845692
Conc: 22.39 ug/ml

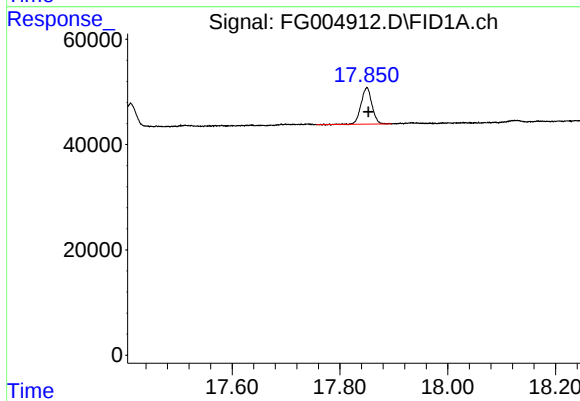

#13 N-TRIACONTANE


R.T.: 17.850 min
Delta R.T.: -0.003 min
Response: 97047
Conc: 0.77 ug/ml

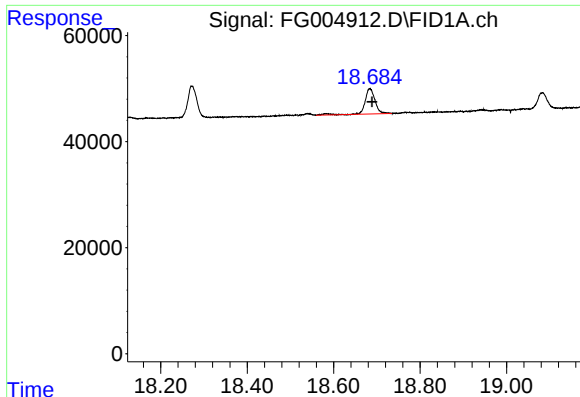

#14 N-DOTRIACONTANE


R.T.: 18.684 min
Delta R.T.: -0.005 min
Response: 78005
Conc: 0.65 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

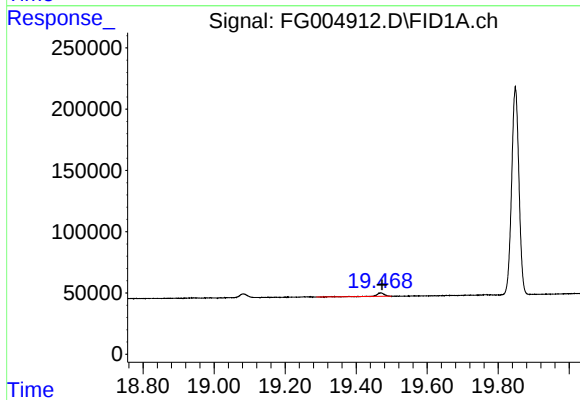

#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: -0.005 min
Response: 45818
Conc: 0.41 ug/ml

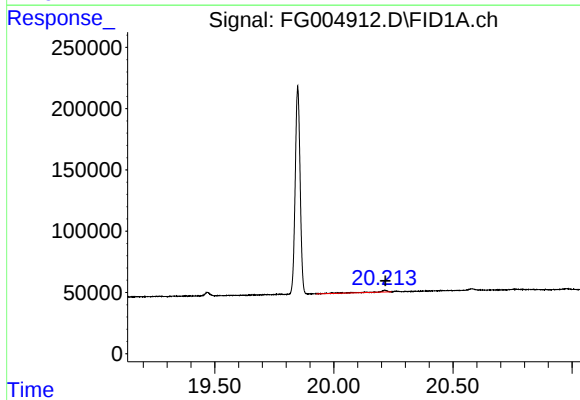

#16 N-HEXATRIACONTANE

R.T.: 20.214 min
Delta R.T.: -0.003 min
Response: 46108
Conc: 0.43 ug/ml