

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
 Data File : FG004921.D
 Signal(s) : FID1A.ch
 Acq On : 09 May 2019 20:54
 Operator : AJ\SJ
 Sample : K2754-03MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-3MS

Integration File: autoint1.e
 Quant Time: May 10 00:47:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	2371970	19.765 ug/ml
Target Compounds			
2) N-DECANE	4.484	2636203	18.651 ug/ml
3) N-DODECANE	6.514	2815178	19.623 ug/ml
4) N-TETRADECANE	8.317	2880655	20.074 ug/ml
5) N-HEXADECANE	9.923	2876787	19.916 ug/ml
6) N-OCTADECANE	11.369	2821301	19.788 ug/ml
7) N-EICOSANE	12.683	2731737	19.275 ug/ml
8) N-DOCOSANE	13.884	2642820	19.070 ug/ml
10) N-TETRACOSANE	14.989	2683294	19.807 ug/ml
11) N-HEXACOSANE	16.012	2578791	19.638 ug/ml
12) N-OCTACOSANE	16.964	2743793	21.584 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050919\
Data File : FG004921.D
Signal(s) : FID1A.ch
Acq On : 09 May 2019 20:54
Operator : AJ\SJ
Sample : K2754-03MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-3MS

Integration File: autoint1.e
Quant Time: May 10 00:47:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

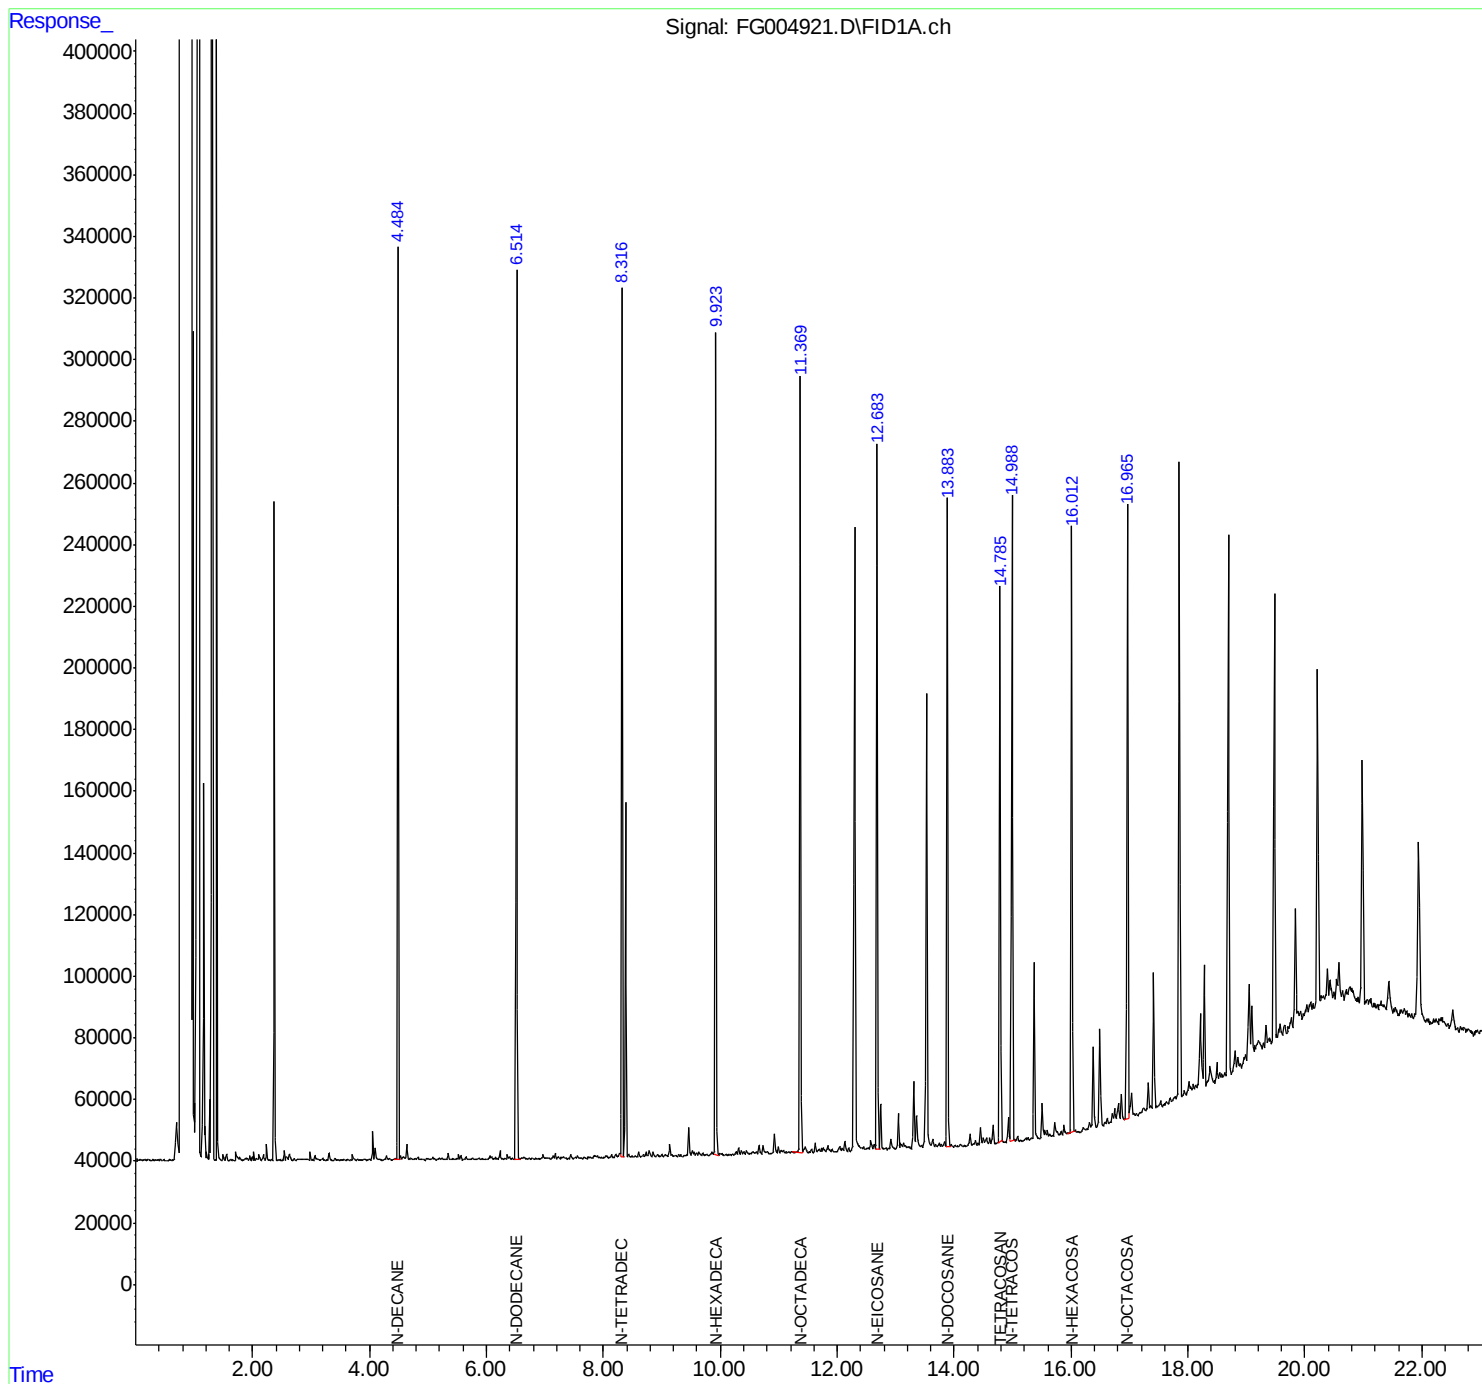


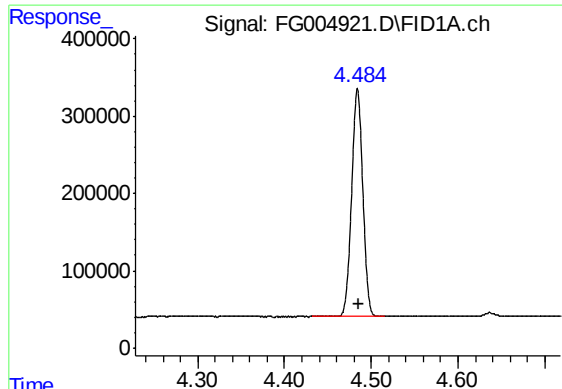

#2 N-DECANE


R.T.: 4.484 min
Delta R.T.: -0.001 min
Response: 2636203
Conc: 18.65 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3MS

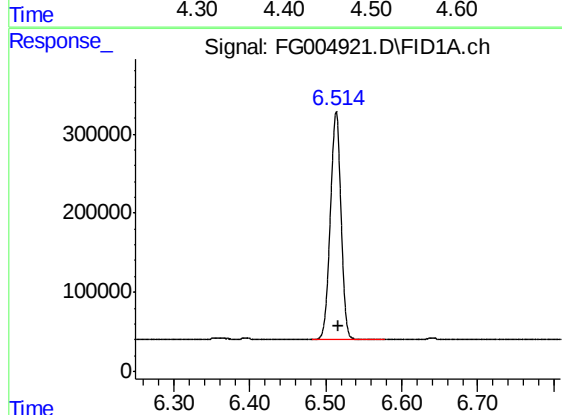


#3 N-DODECANE

R.T.: 6.514 min
Delta R.T.: -0.002 min
Response: 2815178
Conc: 19.62 ug/ml

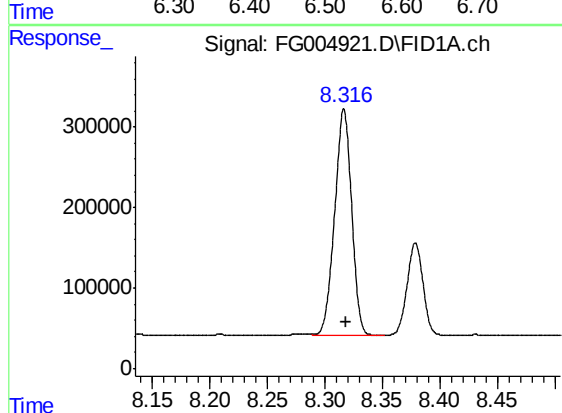


#4 N-TETRADECANE

R.T.: 8.317 min
Delta R.T.: -0.002 min
Response: 2880655
Conc: 20.07 ug/ml

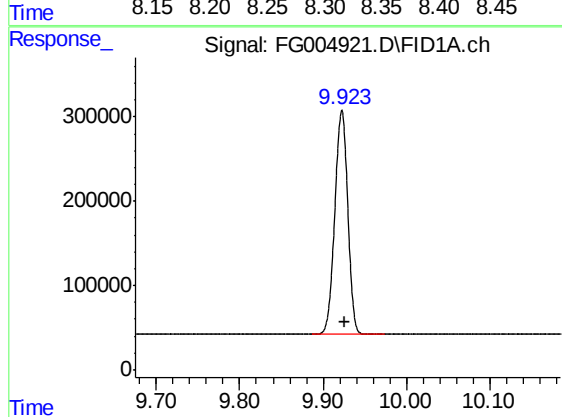

#5 N-HEXADECANE


R.T.: 9.923 min
Delta R.T.: -0.003 min
Response: 2876787
Conc: 19.92 ug/ml

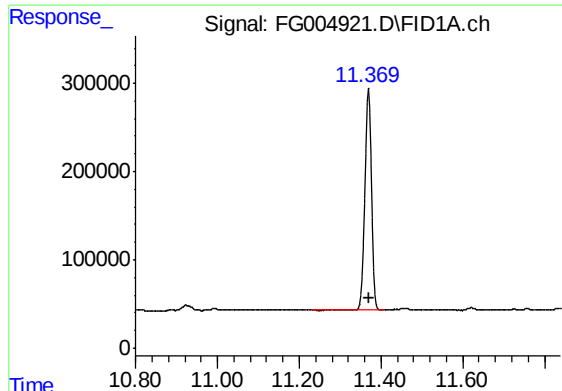

#6 N-OCTADECANE


R.T.: 11.369 min
Delta R.T.: -0.002 min
Response: 2821301
Conc: 19.79 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3MS

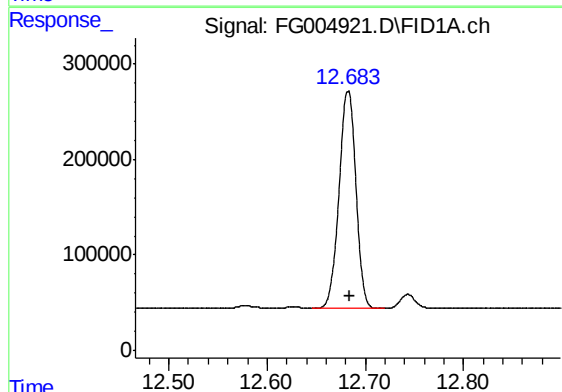


#7 N-EICOSANE

R.T.: 12.683 min
Delta R.T.: -0.002 min
Response: 2731737
Conc: 19.28 ug/ml

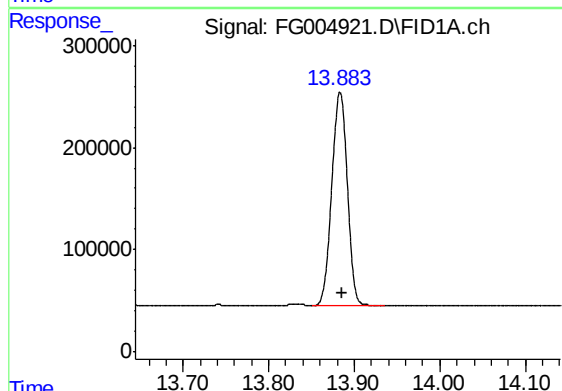


#8 N-DOCOSANE

R.T.: 13.884 min
Delta R.T.: -0.003 min
Response: 2642820
Conc: 19.07 ug/ml

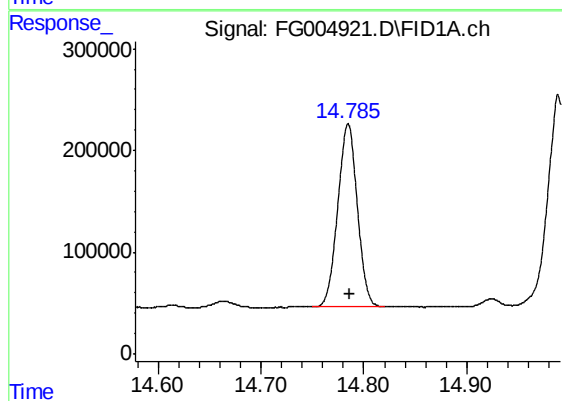

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.785 min
Delta R.T.: -0.001 min
Response: 2371970
Conc: 19.77 ug/ml

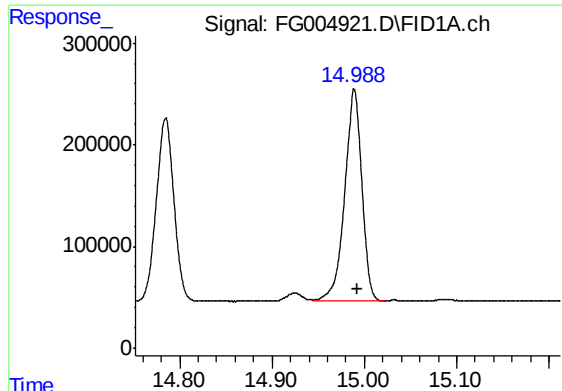

#10 N-TETRACOSANE


R.T.: 14.989 min
Delta R.T.: -0.003 min
Response: 2683294
Conc: 19.81 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3MS

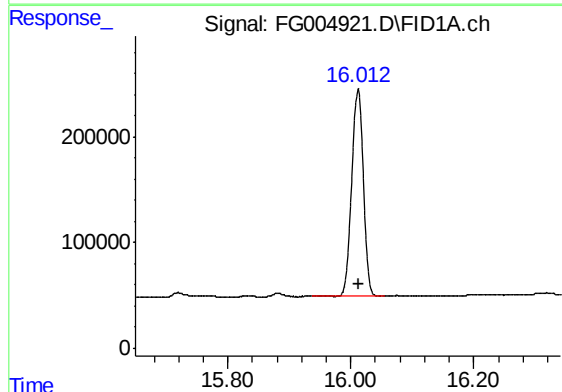

#11 N-HEXACOSANE

R.T.: 16.012 min
Delta R.T.: -0.001 min
Response: 2578791
Conc: 19.64 ug/ml

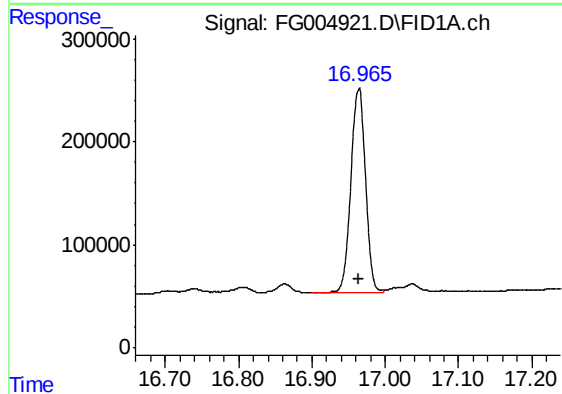

#12 N-OCTACOSANE

R.T.: 16.964 min
Delta R.T.: 0.000 min
Response: 2743793
Conc: 21.58 ug/ml