

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050924\
Data File : FG013769.D
Signal(s) : FID1A.ch
Acq On : 09 May 2024 16:19
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 04:11:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050924.M
Quant Title :
QLast Update : Thu May 09 14:35:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.753	2707603	21.014 ug/ml
12) N-OCTACOSANE	17.250	2764086	21.782 ug/ml
14) N-DOTRIACONTANE	18.983	272790	2.144 ug/ml
16) N-HEXATRIACONTANE	20.538	362204	3.287 ug/ml
18) N-TETRACONTANE	22.238	363824	3.684 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050924\
Data File : FG013769.D
Signal(s) : FID1A.ch
Acq On : 09 May 2024 16:19
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 04:11:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050924.M
Quant Title :
QLast Update : Thu May 09 14:35:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

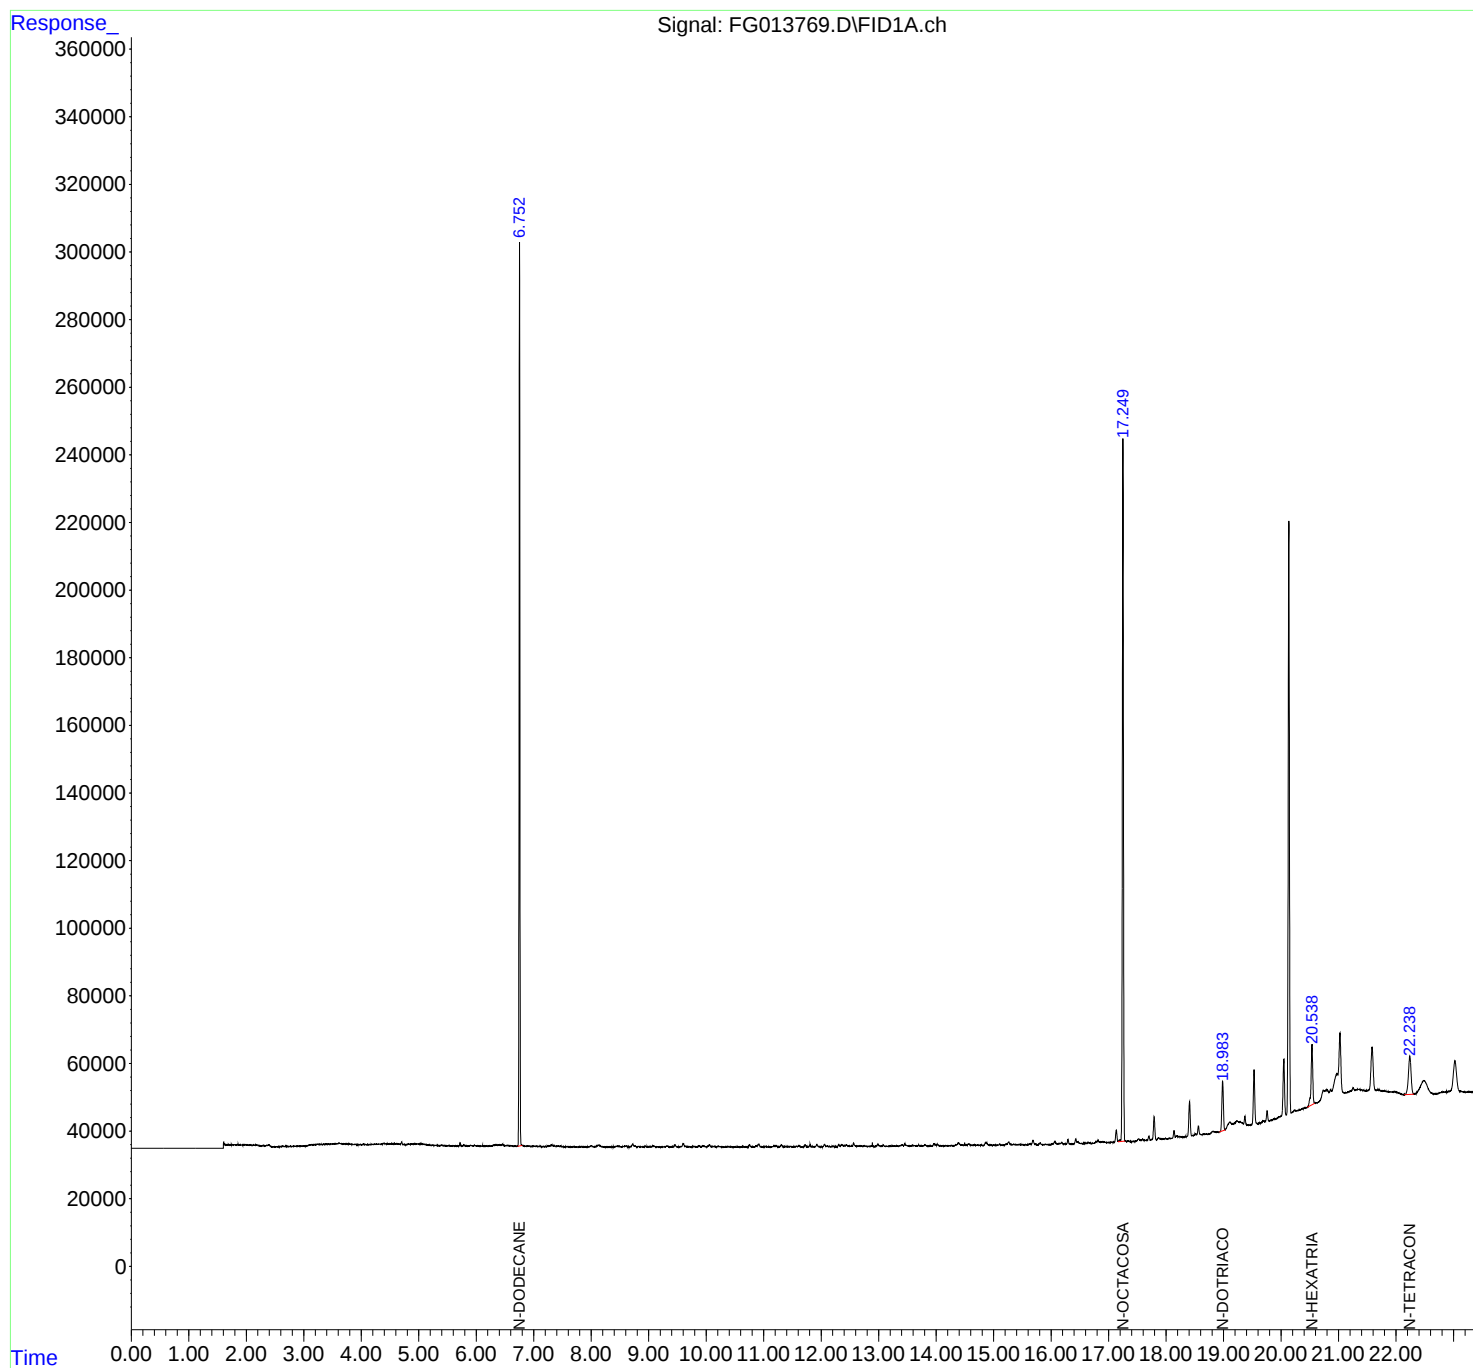


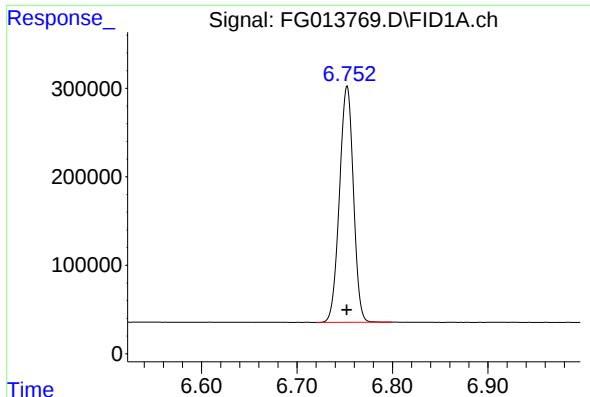

#3 N-DODECANE


R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 2707603
Conc: 21.01 ug/ml

Instrument :
FID_G
ClientSampleId :

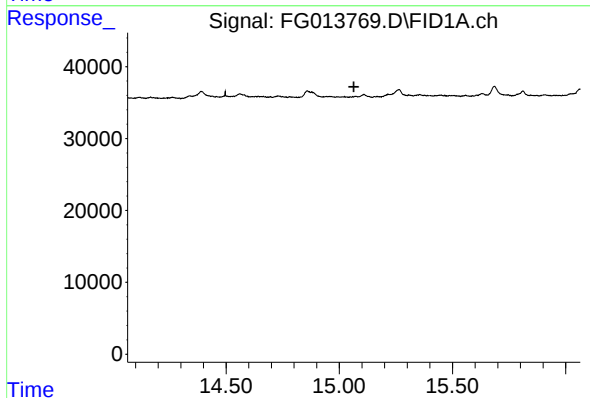


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.065 min
Response: 0
Conc: N.D.

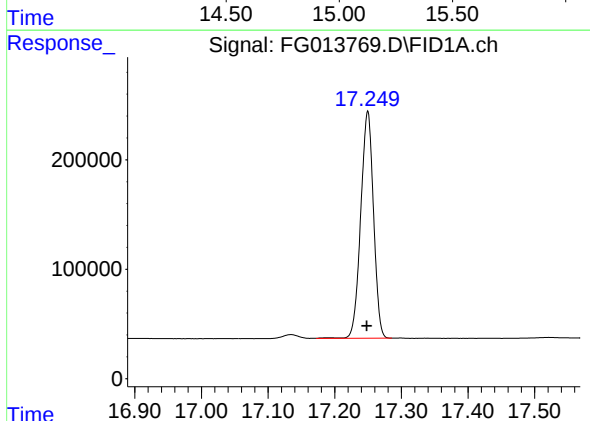


#12 N-OCTACOSANE

R.T.: 17.250 min
Delta R.T.: 0.002 min
Response: 2764086
Conc: 21.78 ug/ml

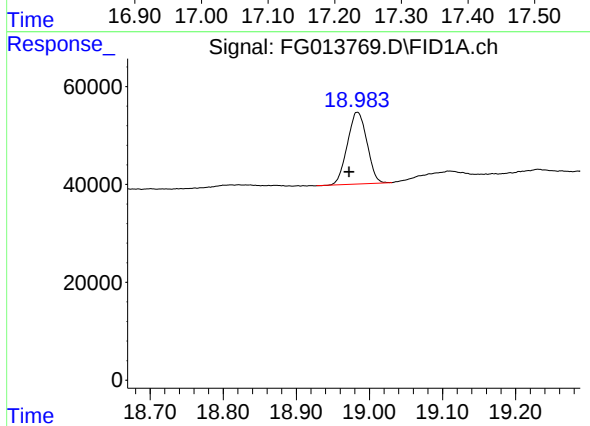

#14 N-DOTRIACONTANE


R.T.: 18.983 min
Delta R.T.: 0.011 min
Response: 272790
Conc: 2.14 ug/ml

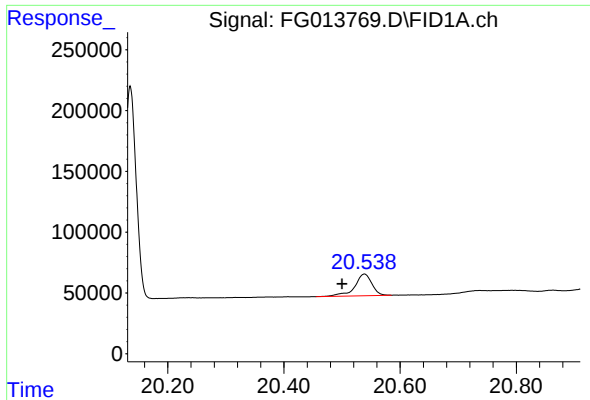

#16 N-HEXATRIACONTANE

R.T.: 20.538 min
Delta R.T.: 0.038 min
Response: 362204
Conc: 3.29 ug/ml

Instrument :
FID_G
ClientSampleId :

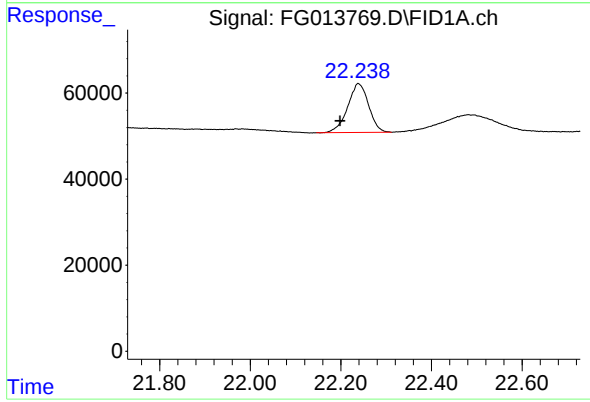

#18 N-TETRACONTANE

R.T.: 22.238 min
Delta R.T.: 0.040 min
Response: 363824
Conc: 3.68 ug/ml