

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050924\
 Data File : FG013788.D
 Signal(s) : FID1A.ch
 Acq On : 10 May 2024 02:12
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: May 10 04:14:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050924.M
 Quant Title :
 QLast Update : Thu May 09 14:35:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.068	5647758	48.478 ug/ml
Target Compounds			
2) N-DECANE	4.581	6354735	50.158 ug/ml
3) N-DODECANE	6.753	6443055	50.005 ug/ml
4) N-TETRADECANE	8.586	6479444	49.263 ug/ml
5) N-HEXADECANE	10.199	6515531	48.877 ug/ml
6) N-OCTADECANE	11.648	6610103	48.531 ug/ml
7) N-EICOSANE	12.963	6654630	48.310 ug/ml
8) N-DOCOSANE	14.165	6404829	48.294 ug/ml
10) N-TETRACOSANE	15.273	6347495	48.093 ug/ml
11) N-HEXACOSANE	16.297	6285761	48.408 ug/ml
12) N-OCTACOSANE	17.250	6176260	48.671 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050924\
Data File : FG013788.D
Signal(s) : FID1A.ch
Acq On : 10 May 2024 02:12
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: May 10 04:14:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050924.M
Quant Title :
QLast Update : Thu May 09 14:35:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

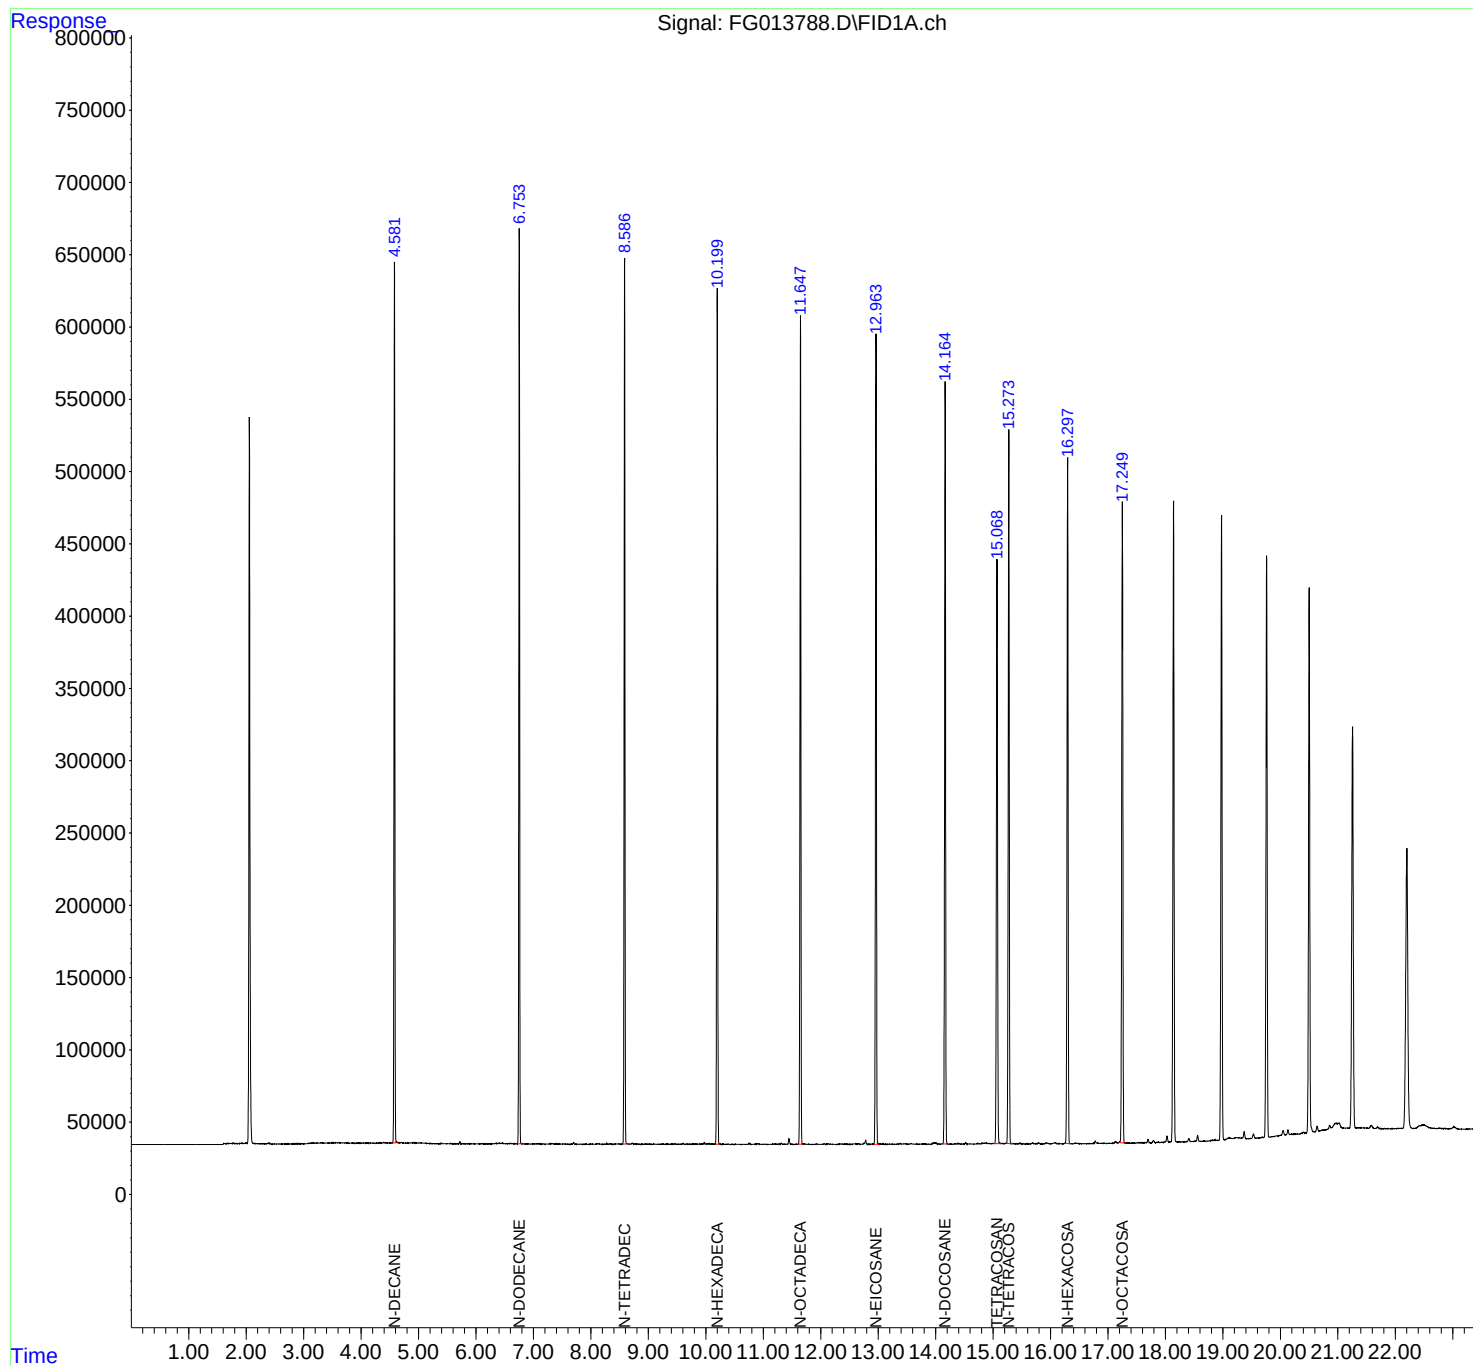


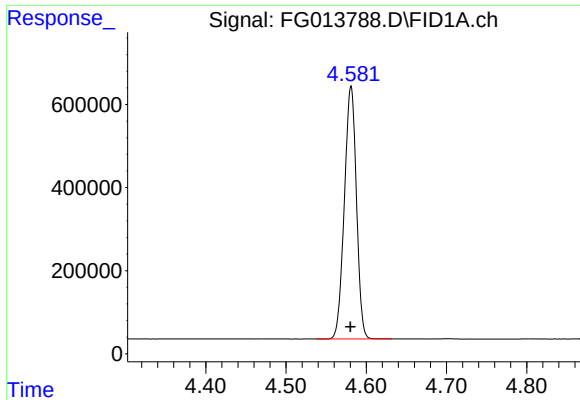

#2 N-DECANE


R.T.: 4.581 min
Delta R.T.: 0.000 min
Response: 6354735
Conc: 50.16 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

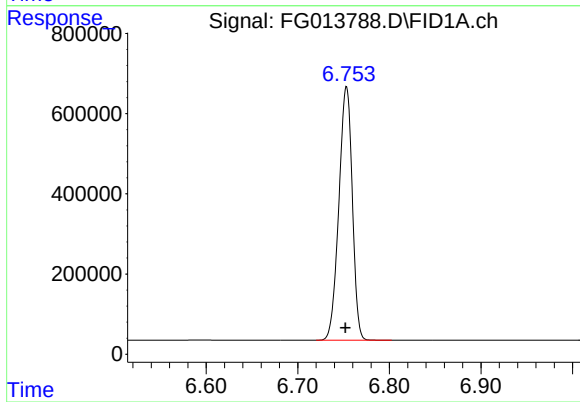


#3 N-DODECANE

R.T.: 6.753 min
Delta R.T.: 0.001 min
Response: 6443055
Conc: 50.00 ug/ml

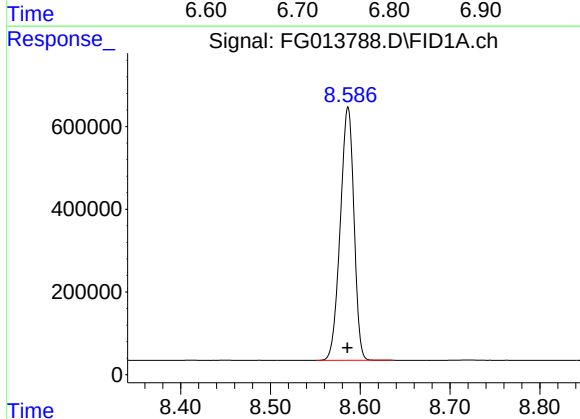


#4 N-TETRADECANE

R.T.: 8.586 min
Delta R.T.: 0.000 min
Response: 6479444
Conc: 49.26 ug/ml

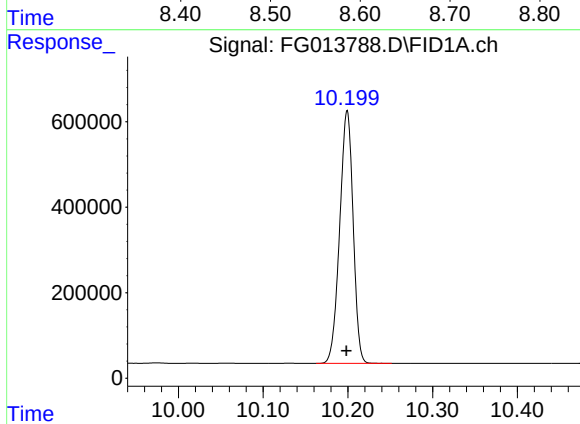

#5 N-HEXADECANE


R.T.: 10.199 min
Delta R.T.: 0.001 min
Response: 6515531
Conc: 48.88 ug/ml

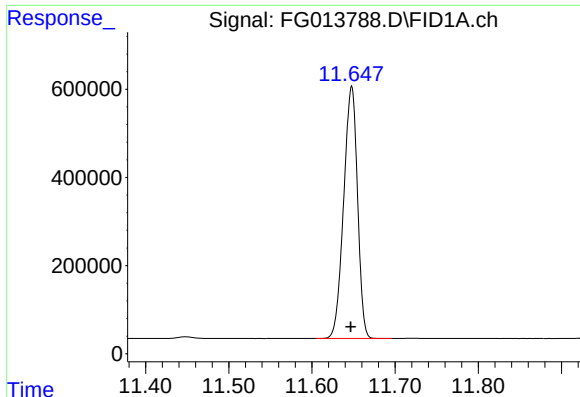

#6 N-OCTADECANE


R.T.: 11.648 min
Delta R.T.: 0.001 min
Response: 6610103
Conc: 48.53 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

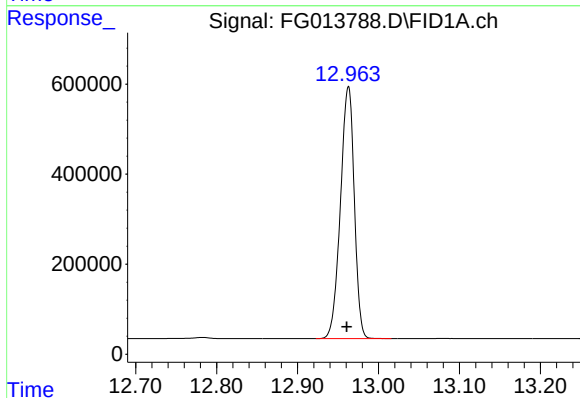


#7 N-EICOSANE

R.T.: 12.963 min
Delta R.T.: 0.002 min
Response: 6654630
Conc: 48.31 ug/ml

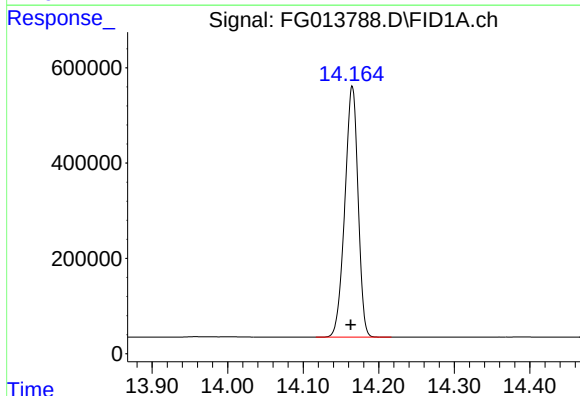


#8 N-DOCOSANE

R.T.: 14.165 min
Delta R.T.: 0.002 min
Response: 6404829
Conc: 48.29 ug/ml

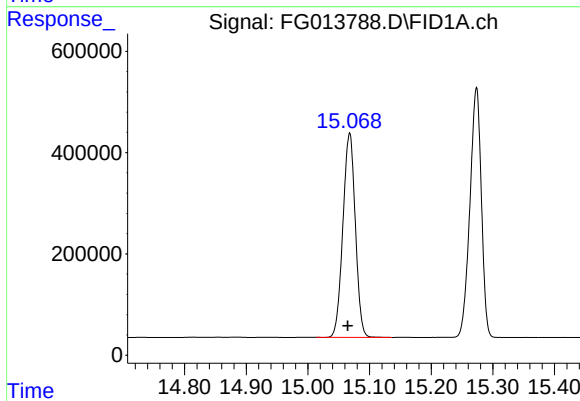

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.068 min
Delta R.T.: 0.003 min
Response: 5647758
Conc: 48.48 ug/ml

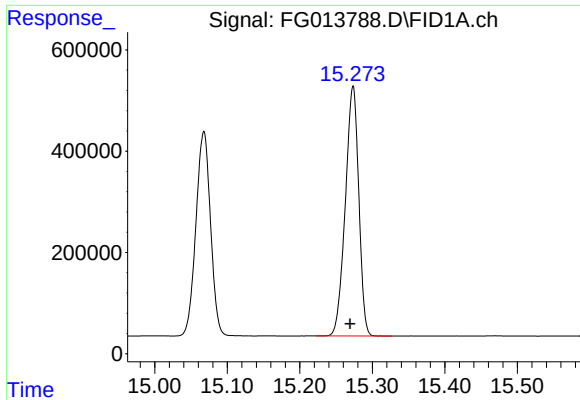

#10 N-TETRACOSANE


R.T.: 15.273 min
Delta R.T.: 0.004 min
Response: 6347495
Conc: 48.09 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

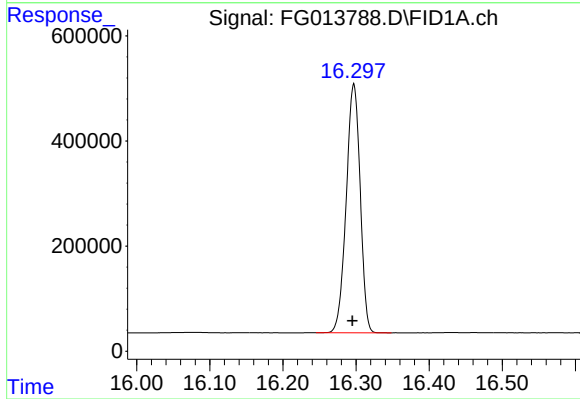

#11 N-HEXACOSANE

R.T.: 16.297 min
Delta R.T.: 0.002 min
Response: 6285761
Conc: 48.41 ug/ml

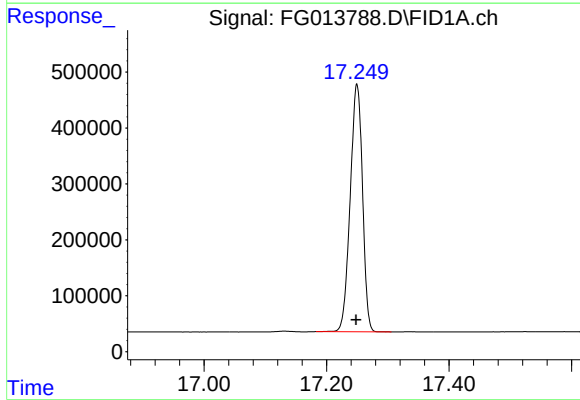

#12 N-OCTACOSANE

R.T.: 17.250 min
Delta R.T.: 0.002 min
Response: 6176260
Conc: 48.67 ug/ml