

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051021\
Data File : FG008041.D
Signal(s) : FID1A.ch
Acq On : 10 May 2021 19:15
Operator : DD\AJ
Sample : PB136185BL
Misc : MDL-BL-WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB136185BL

Integration File: autoint1.e
Quant Time: May 11 02:58:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2139363	16.070 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051021\
Data File : FG008041.D
Signal(s) : FID1A.ch
Acq On : 10 May 2021 19:15
Operator : DD\AJ
Sample : PB136185BL
Misc : MDL-BL-WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB136185BL

Integration File: autoint1.e
Quant Time: May 11 02:58:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

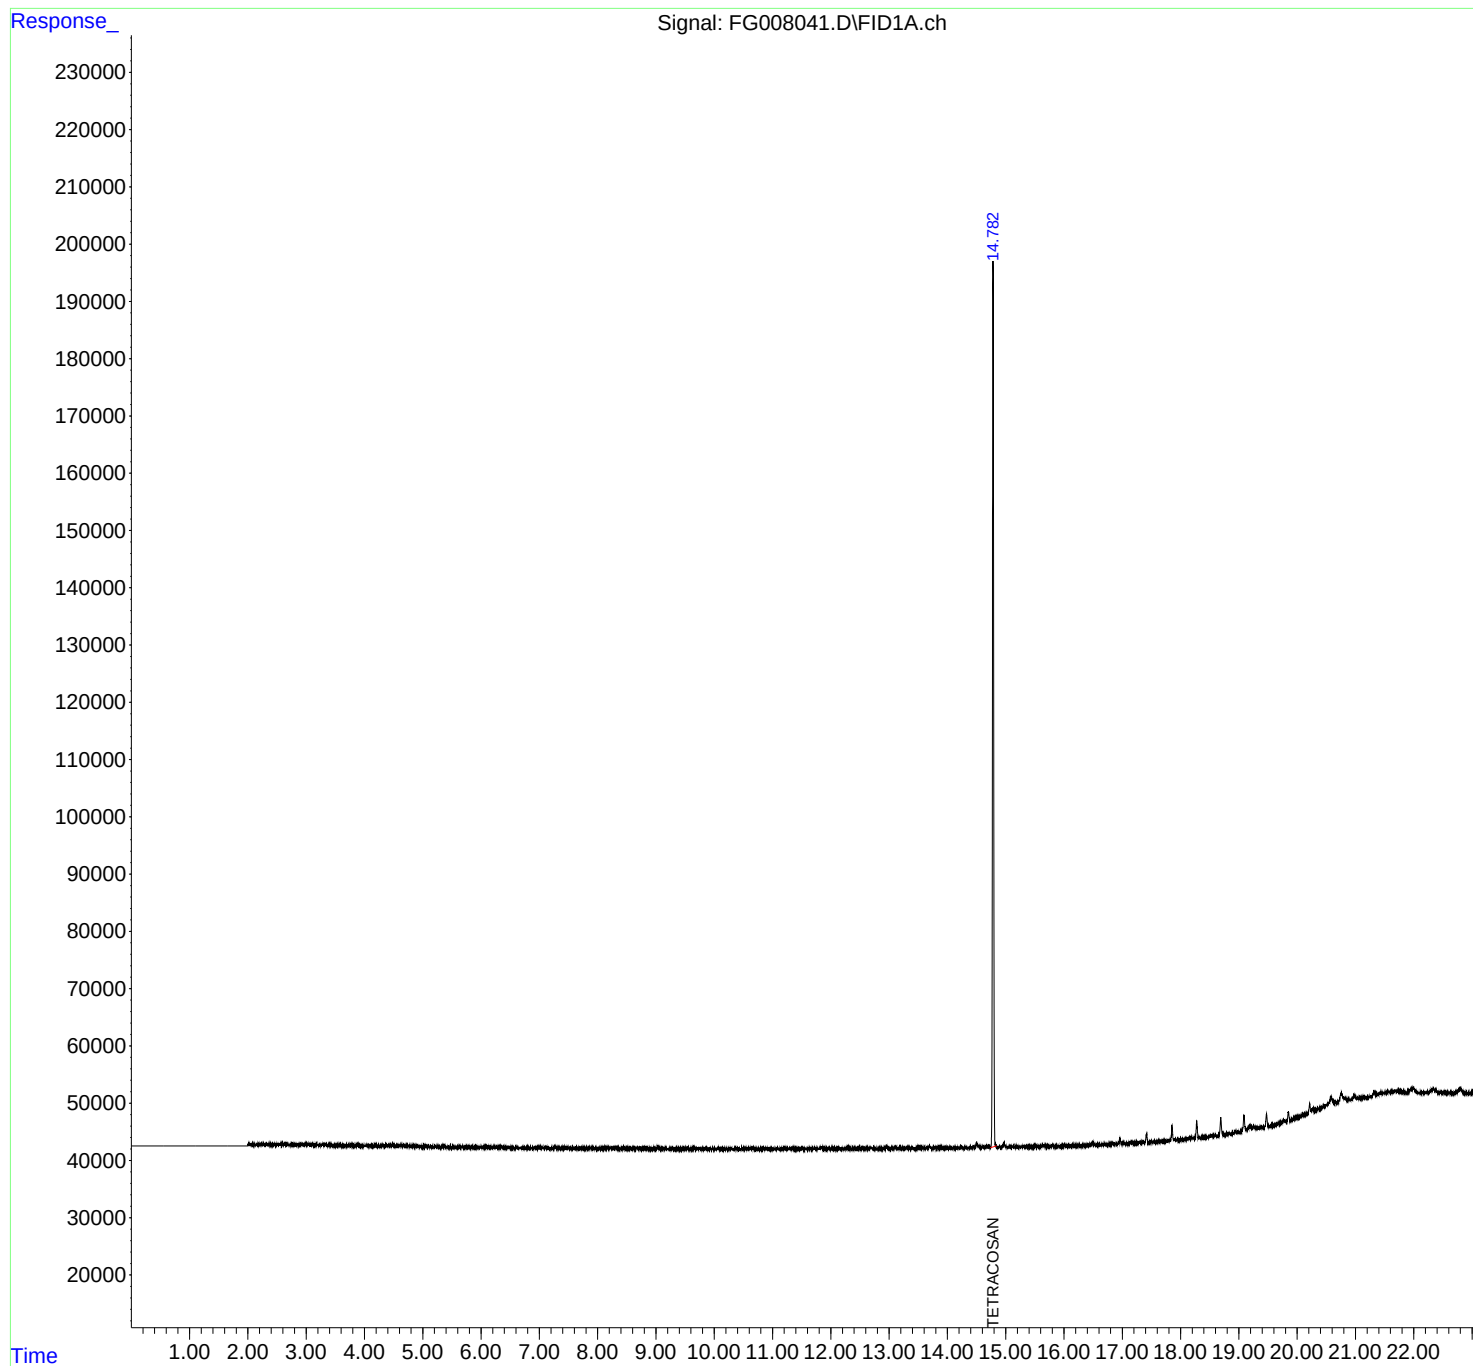

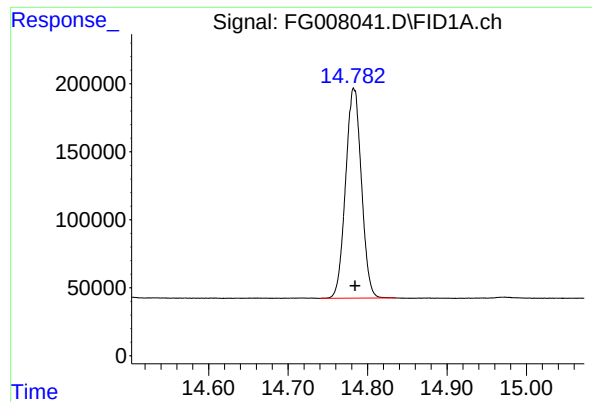

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.001 min
Response: 2139363
Conc: 16.07 ug/ml

Instrument :
FID_G
ClientSampleId :
PB136185BL