

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051024\
 Data File : FG013791.D
 Signal(s) : FID1A.ch
 Acq On : 10 May 2024 09:07
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: May 11 01:17:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050924.M
 Quant Title :
 QLast Update : Thu May 09 14:35:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.067	6487726	55.687 ug/ml
Target Compounds			
2) N-DECANE	4.580	6681878	52.740 ug/ml
3) N-DODECANE	6.752	6876930	53.372 ug/ml
4) N-TETRADECANE	8.586	7059713	53.675 ug/ml
5) N-HEXADECANE	10.199	7194400	53.970 ug/ml
6) N-OCTADECANE	11.648	7398784	54.321 ug/ml
7) N-EICOSANE	12.963	7515603	54.560 ug/ml
8) N-DOCOSANE	14.164	7301874	55.057 ug/ml
10) N-TETRACOSANE	15.272	7318954	55.453 ug/ml
11) N-HEXACOSANE	16.297	7262508	55.930 ug/ml
12) N-OCTACOSANE	17.250	7190075	56.660 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051024\
Data File : FG013791.D
Signal(s) : FID1A.ch
Acq On : 10 May 2024 09:07
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: May 11 01:17:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050924.M
Quant Title :
QLast Update : Thu May 09 14:35:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

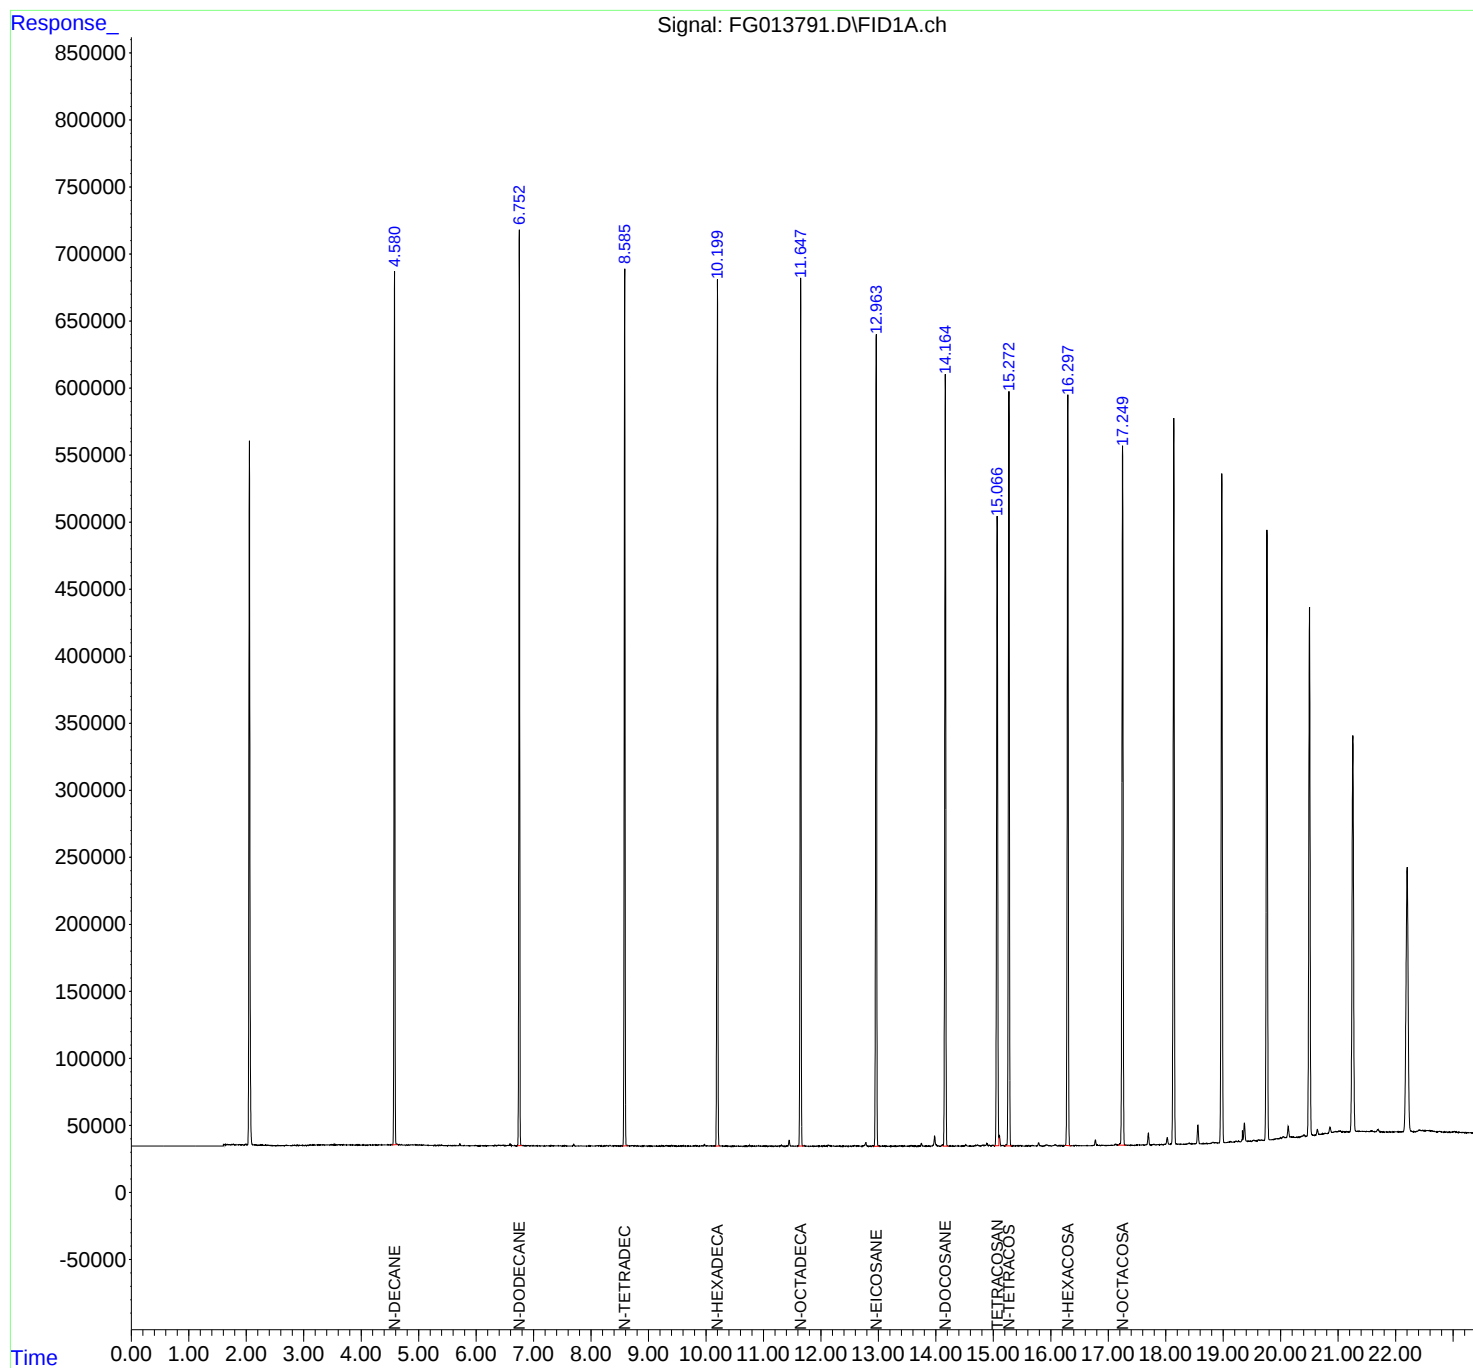


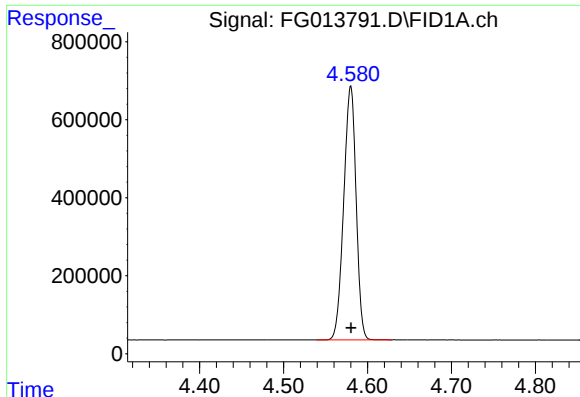

#2 N-DECANE


R.T.: 4.580 min
Delta R.T.: 0.000 min
Response: 6681878
Conc: 52.74 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

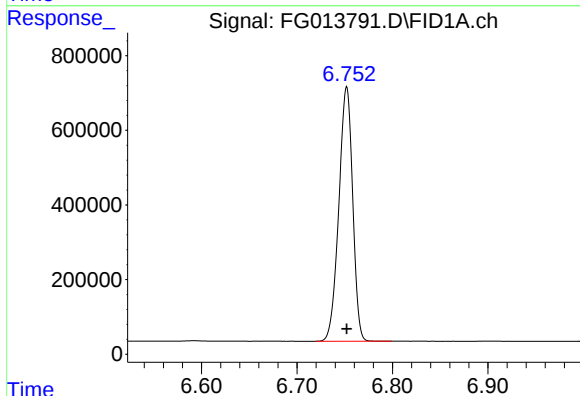


#3 N-DODECANE

R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 6876930
Conc: 53.37 ug/ml

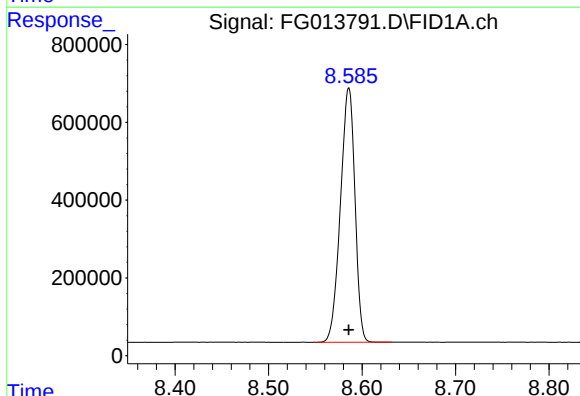


#4 N-TETRADECANE

R.T.: 8.586 min
Delta R.T.: 0.000 min
Response: 7059713
Conc: 53.67 ug/ml

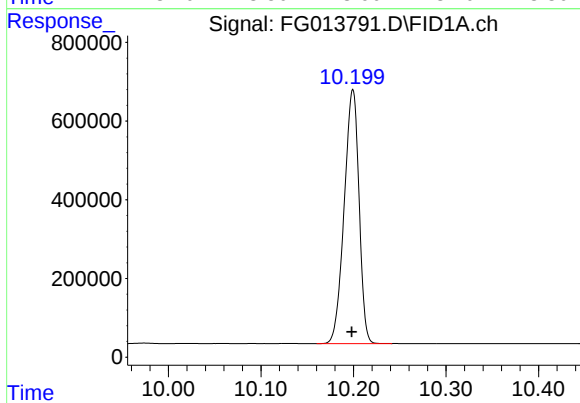

#5 N-HEXADECANE


R.T.: 10.199 min
Delta R.T.: 0.001 min
Response: 7194400
Conc: 53.97 ug/ml

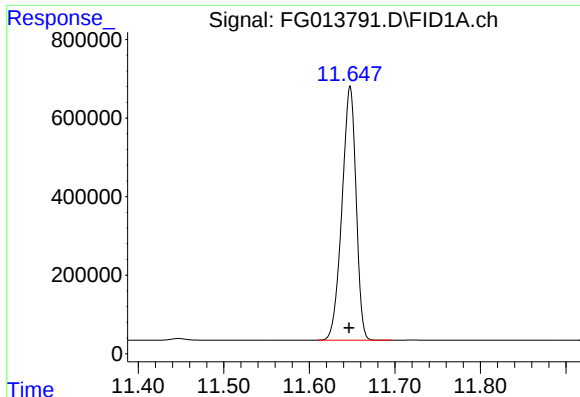

#6 N-OCTADECANE


R.T.: 11.648 min
Delta R.T.: 0.001 min
Response: 7398784
Conc: 54.32 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

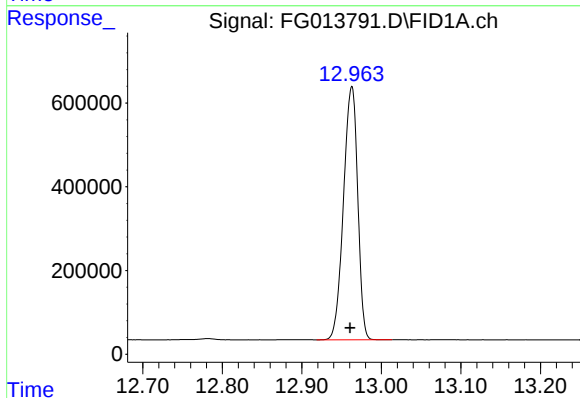


#7 N-EICOSANE

R.T.: 12.963 min
Delta R.T.: 0.002 min
Response: 7515603
Conc: 54.56 ug/ml

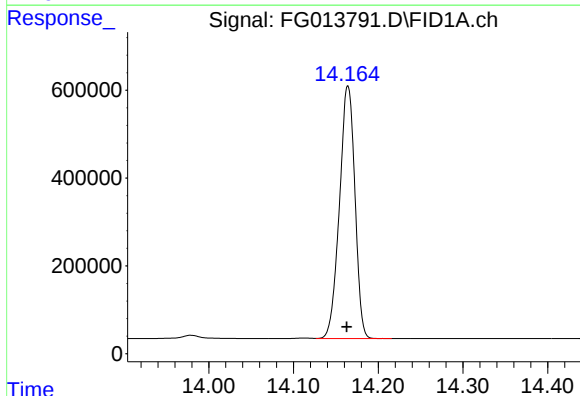


#8 N-DOCOSANE

R.T.: 14.164 min
Delta R.T.: 0.001 min
Response: 7301874
Conc: 55.06 ug/ml

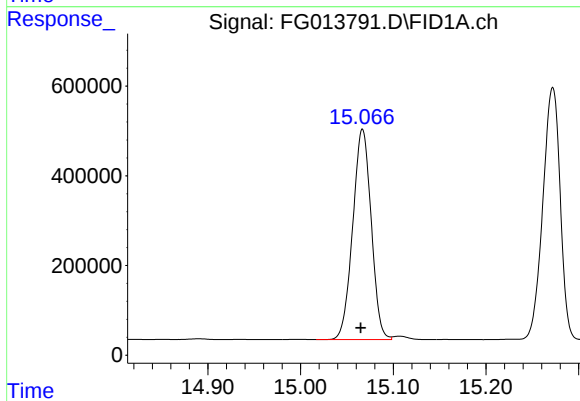

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.067 min
Delta R.T.: 0.002 min
Response: 6487726
Conc: 55.69 ug/ml

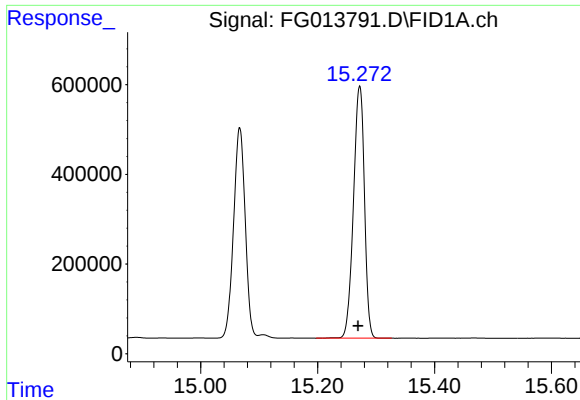

#10 N-TETRACOSANE


R.T.: 15.272 min
Delta R.T.: 0.003 min
Response: 7318954
Conc: 55.45 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

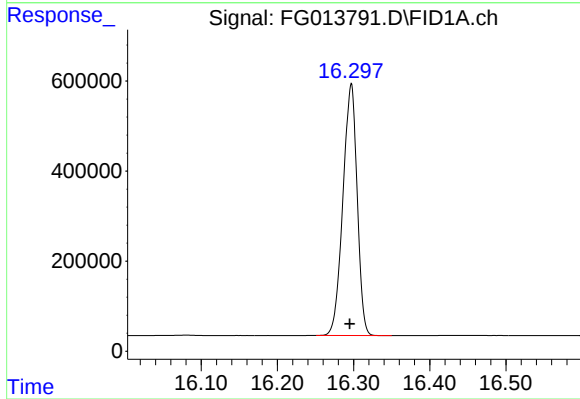

#11 N-HEXACOSANE

R.T.: 16.297 min
Delta R.T.: 0.002 min
Response: 7262508
Conc: 55.93 ug/ml

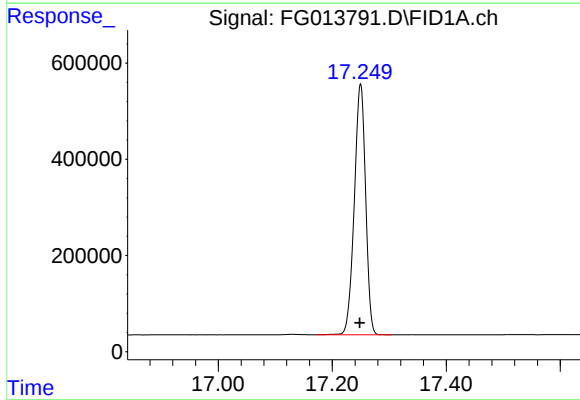

#12 N-OCTACOSANE

R.T.: 17.250 min
Delta R.T.: 0.002 min
Response: 7190075
Conc: 56.66 ug/ml