

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051024AL\
Data File : FG013806.D
Signal(s) : FID1A.ch
Acq On : 10 May 2024 17:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 05:14:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 051024.M
Quant Title : GC Extractables
QLast Update : Fri May 10 16:04:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.982	267787	2.044 ug/ml
20) T	n-Hexatriacontane (C36)	20.537	270298	2.343 ug/ml
22) T	n-Tetracontane (C40)	22.236	249726	2.401 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051024AL\
Data File : FG013806.D
Signal(s) : FID1A.ch
Acq On : 10 May 2024 17:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 05:14:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 051024.M
Quant Title : GC Extractables
QLast Update : Fri May 10 16:04:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

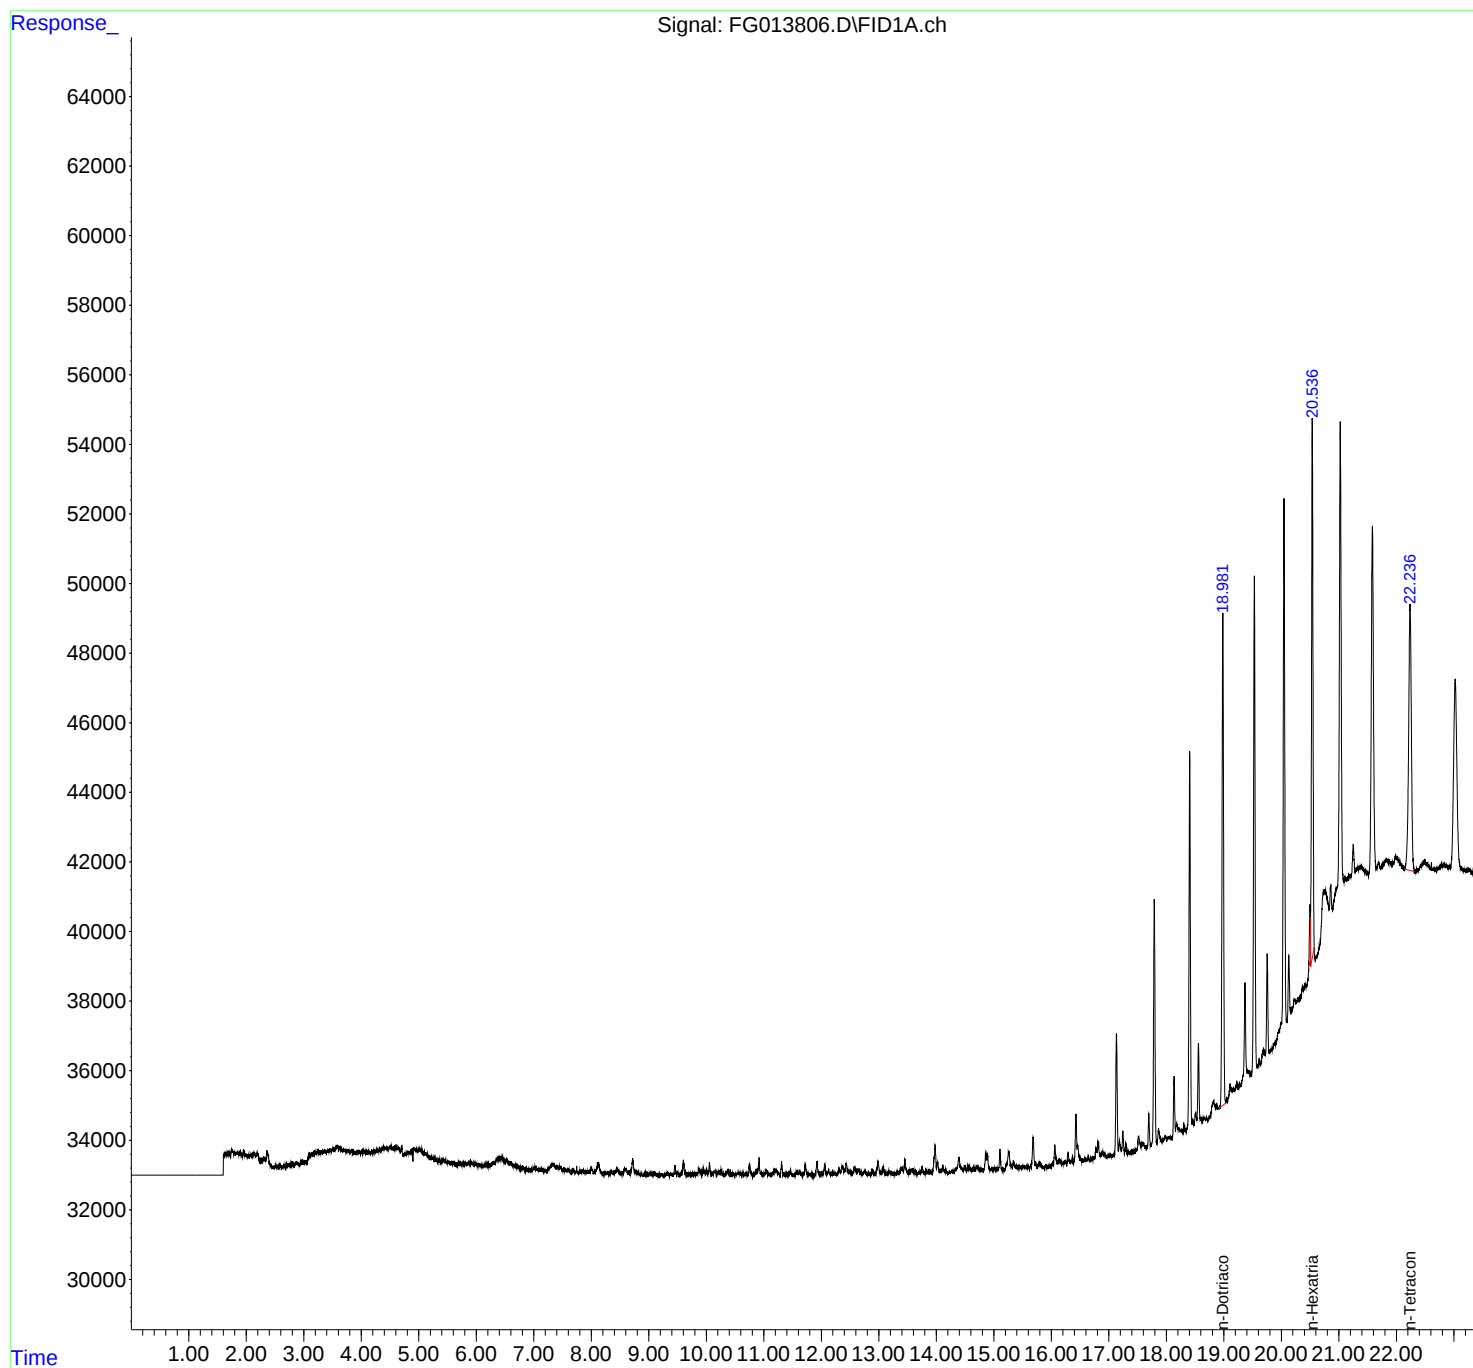


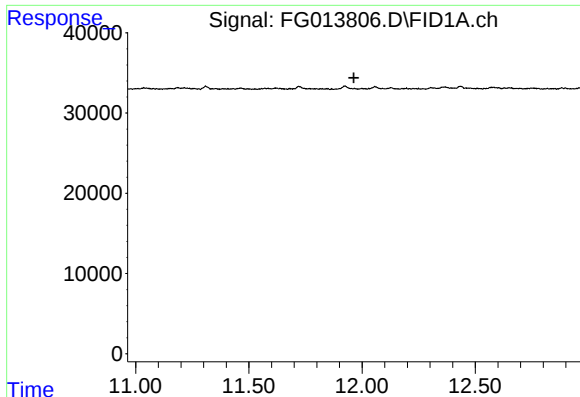

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.963 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

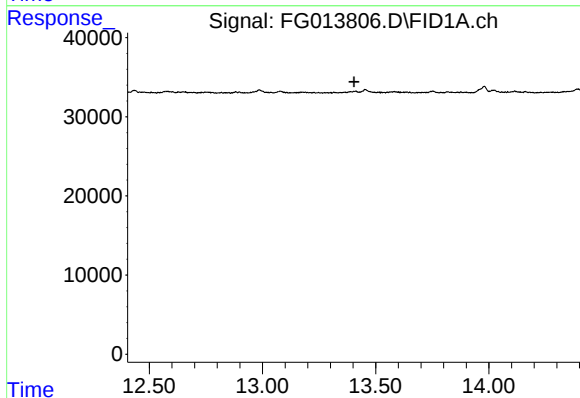


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.404 min
Response: 0
Conc: N.D.

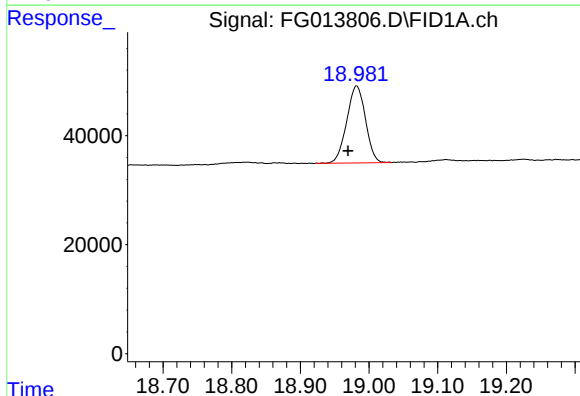


#18 n-Dotriacontane (C32)

R.T.: 18.982 min
Delta R.T.: 0.012 min
Response: 267787
Conc: 2.04 ug/ml

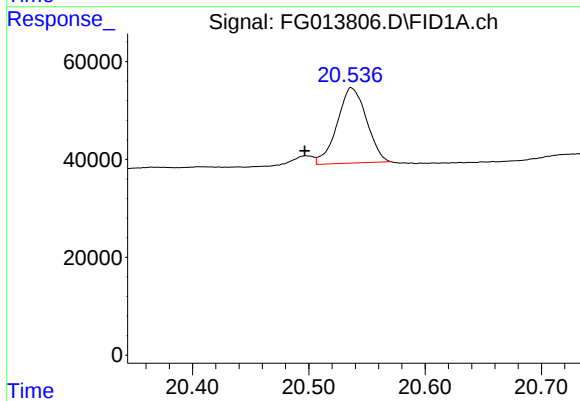

#20 n-Hexatriacontane (C36)

R.T.: 20.537 min
Delta R.T.: 0.040 min
Response: 270298
Conc: 2.34 ug/ml

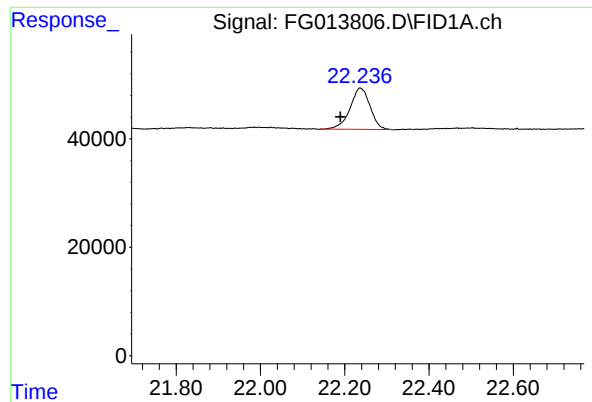

#22 n-Tetracontane (C40)

R.T.: 22.236 min
Delta R.T.: 0.046 min
Response: 249726
Conc: 2.40 ug/ml

Instrument :
FID_G
ClientSampleId :