

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG051325\  
 Data File : FG015816.D  
 Signal(s) : FID1A.ch  
 Acq On : 13 May 2025 10:42  
 Operator : YP\AJ  
 Sample : MECL2  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: May 14 03:54:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG042425.M  
 Quant Title :  
 QLast Update : Thu Apr 24 12:54:09 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units  |
|-------------------------------|--------|----------|-------------|
| -----                         |        |          |             |
| System Monitoring Compounds   |        |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 15.045 | 30377    | 0.258 ug/ml |
| Target Compounds              |        |          |             |
| 13) N-TRIACONTANE             | 18.068 | 36289    | 0.272 ug/ml |
| 14) N-DOTRIACONTANE           | 18.904 | 83934    | 0.637 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.688 | 33000    | 0.273 ug/ml |
| 16) N-HEXATRIACONTANE         | 20.429 | 20053    | 0.187 ug/ml |
| -----                         |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG051325\  
Data File : FG015816.D  
Signal(s) : FID1A.ch  
Acq On : 13 May 2025 10:42  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: May 14 03:54:06 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG042425.M  
Quant Title :  
QLast Update : Thu Apr 24 12:54:09 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

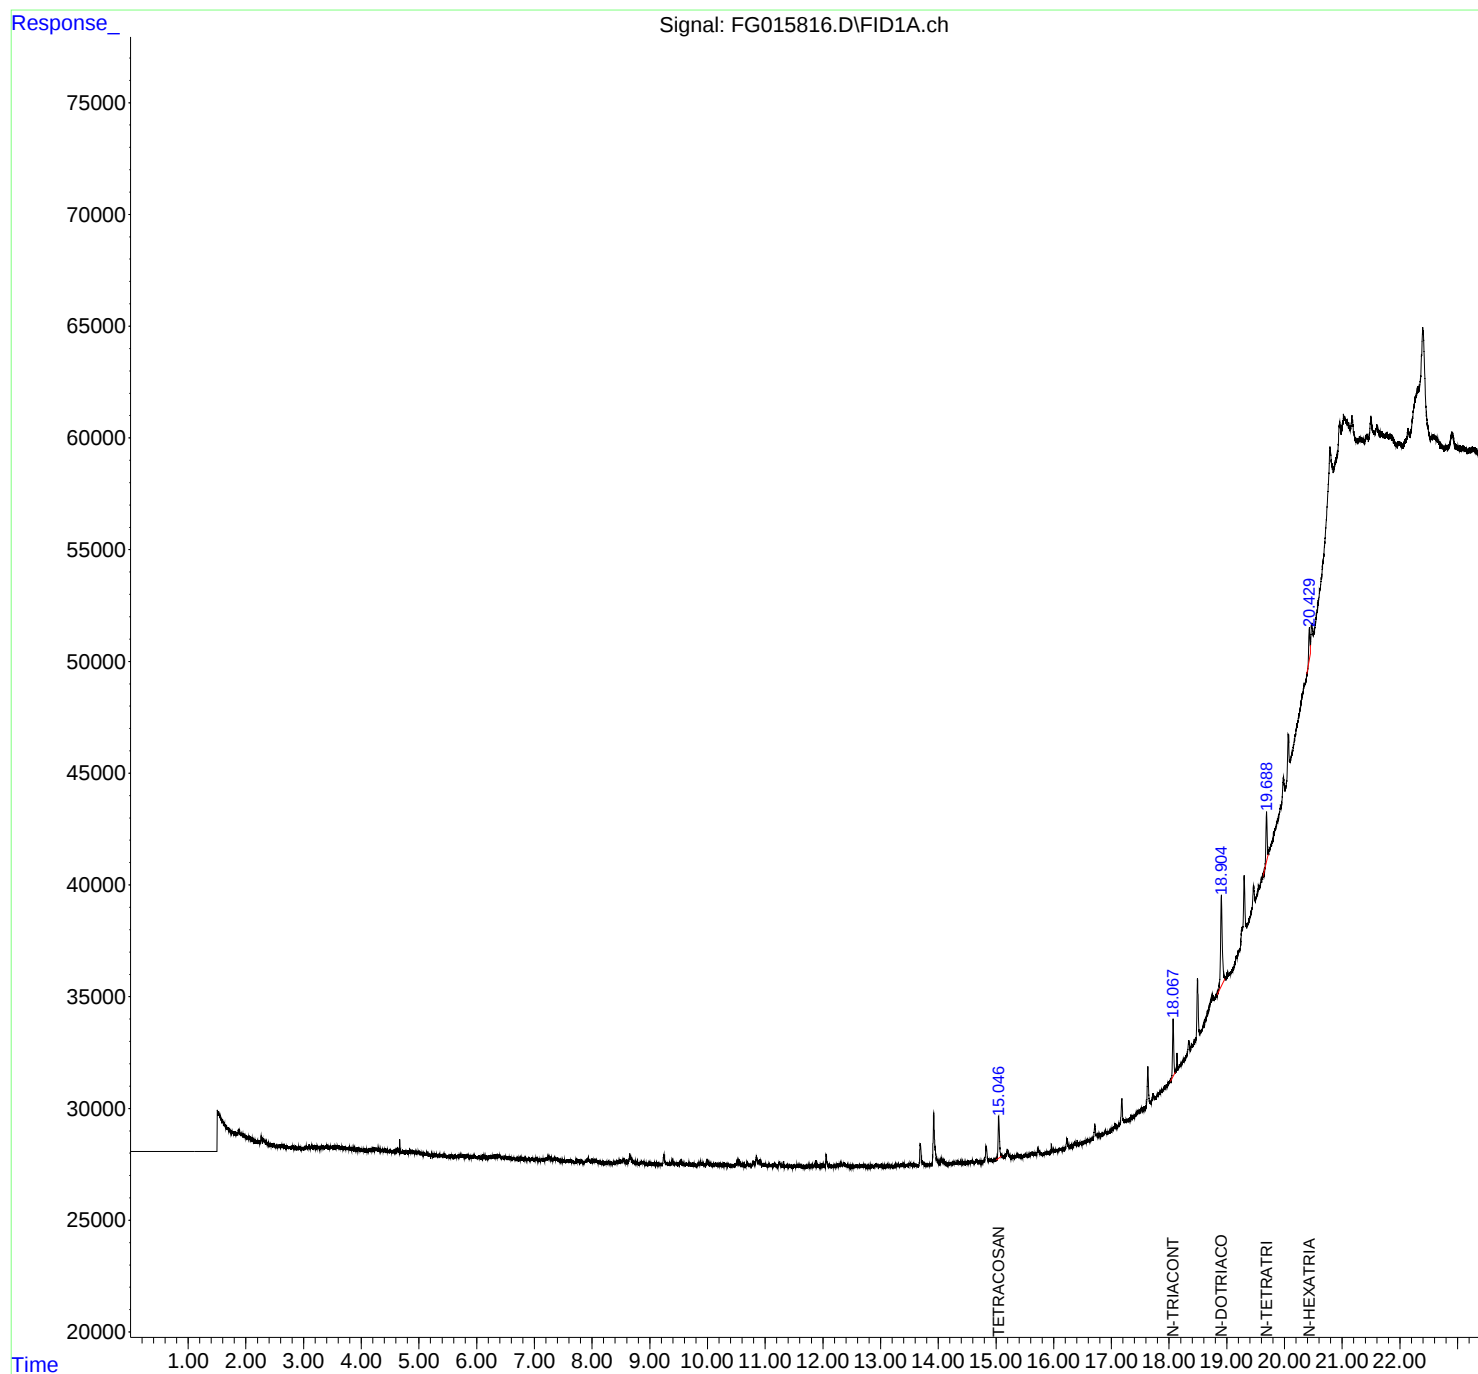


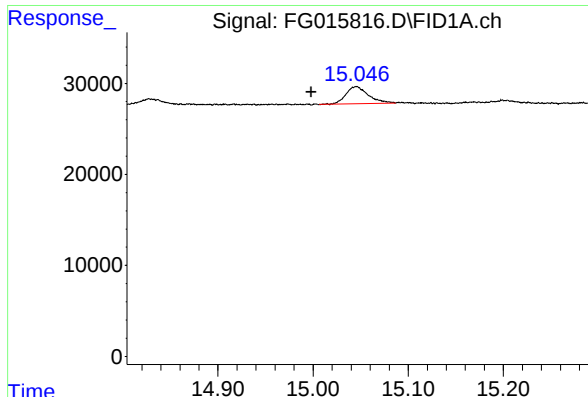

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.045 min  
Delta R.T.: 0.047 min  
Response: 30377  
Conc: 0.26 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

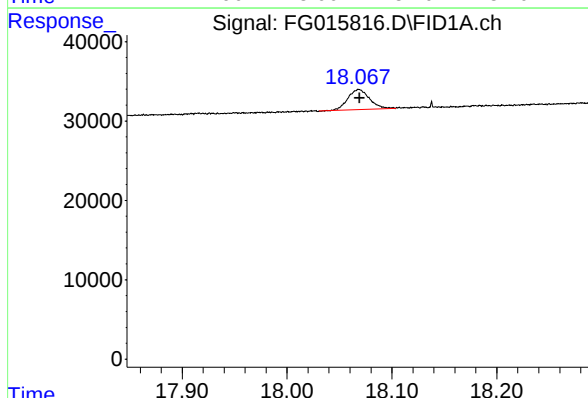


#13 N-TRIACONTANE

R.T.: 18.068 min  
Delta R.T.: 0.000 min  
Response: 36289  
Conc: 0.27 ug/ml

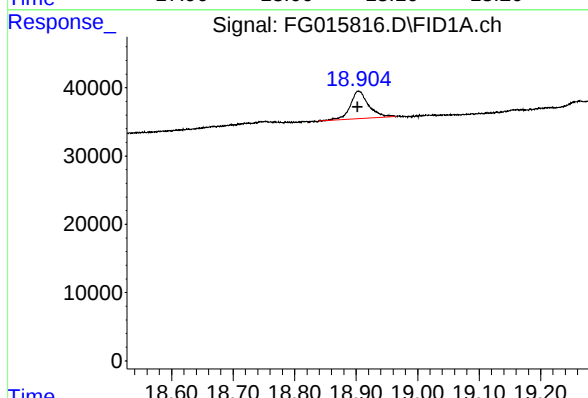


#14 N-DOTRIACONTANE

R.T.: 18.904 min  
Delta R.T.: 0.002 min  
Response: 83934  
Conc: 0.64 ug/ml

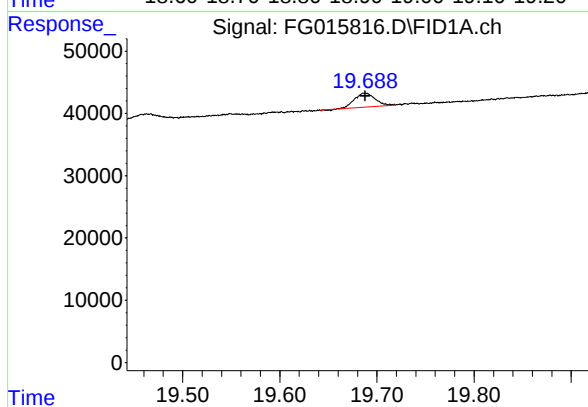

#15 N-TETRATRIACONTANE

R.T.: 19.688 min  
Delta R.T.: 0.000 min  
Response: 33000  
Conc: 0.27 ug/ml

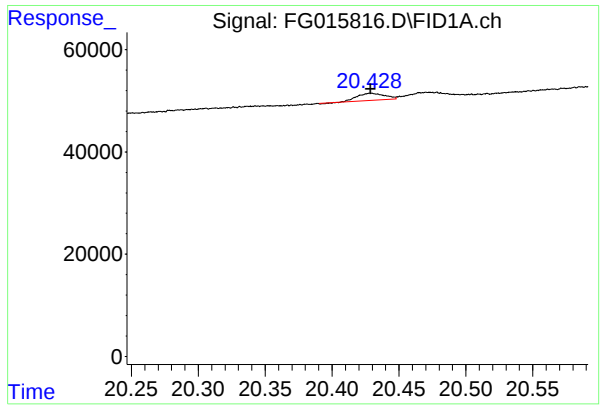

#16 N-HEXATRIACONTANE

R.T.: 20.429 min  
Delta R.T.: 0.000 min  
Response: 20053  
Conc: 0.19 ug/ml

Instrument :

FID\_G

ClientSampleId :