

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051421\
 Data File : FG008078.D
 Signal(s) : FID1A.ch
 Acq On : 14 May 2021 08:15
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 14 23:53:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
 Quant Title :
 QLast Update : Thu Apr 22 01:54:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	6921915	51.994 ug/ml
Target Compounds			
2) N-DECANE	4.483	9039367	59.798 ug/ml
3) N-DODECANE	6.512	8955622	58.536 ug/ml
4) N-TETRADECANE	8.314	8841856	56.647 ug/ml
5) N-HEXADECANE	9.921	8523029	55.009 ug/ml
6) N-OCTADECANE	11.367	8442930	53.696 ug/ml
7) N-EICOSANE	12.681	8148397	52.584 ug/ml
8) N-DOCOSANE	13.882	7941167	51.678 ug/ml
10) N-TETRACOSANE	14.991	7756640	50.977 ug/ml
11) N-HEXACOSANE	16.014	7579986	50.889 ug/ml
12) N-OCTACOSANE	16.967	7534229	51.448 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051421\
Data File : FG008078.D
Signal(s) : FID1A.ch
Acq On : 14 May 2021 08:15
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 14 23:53:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

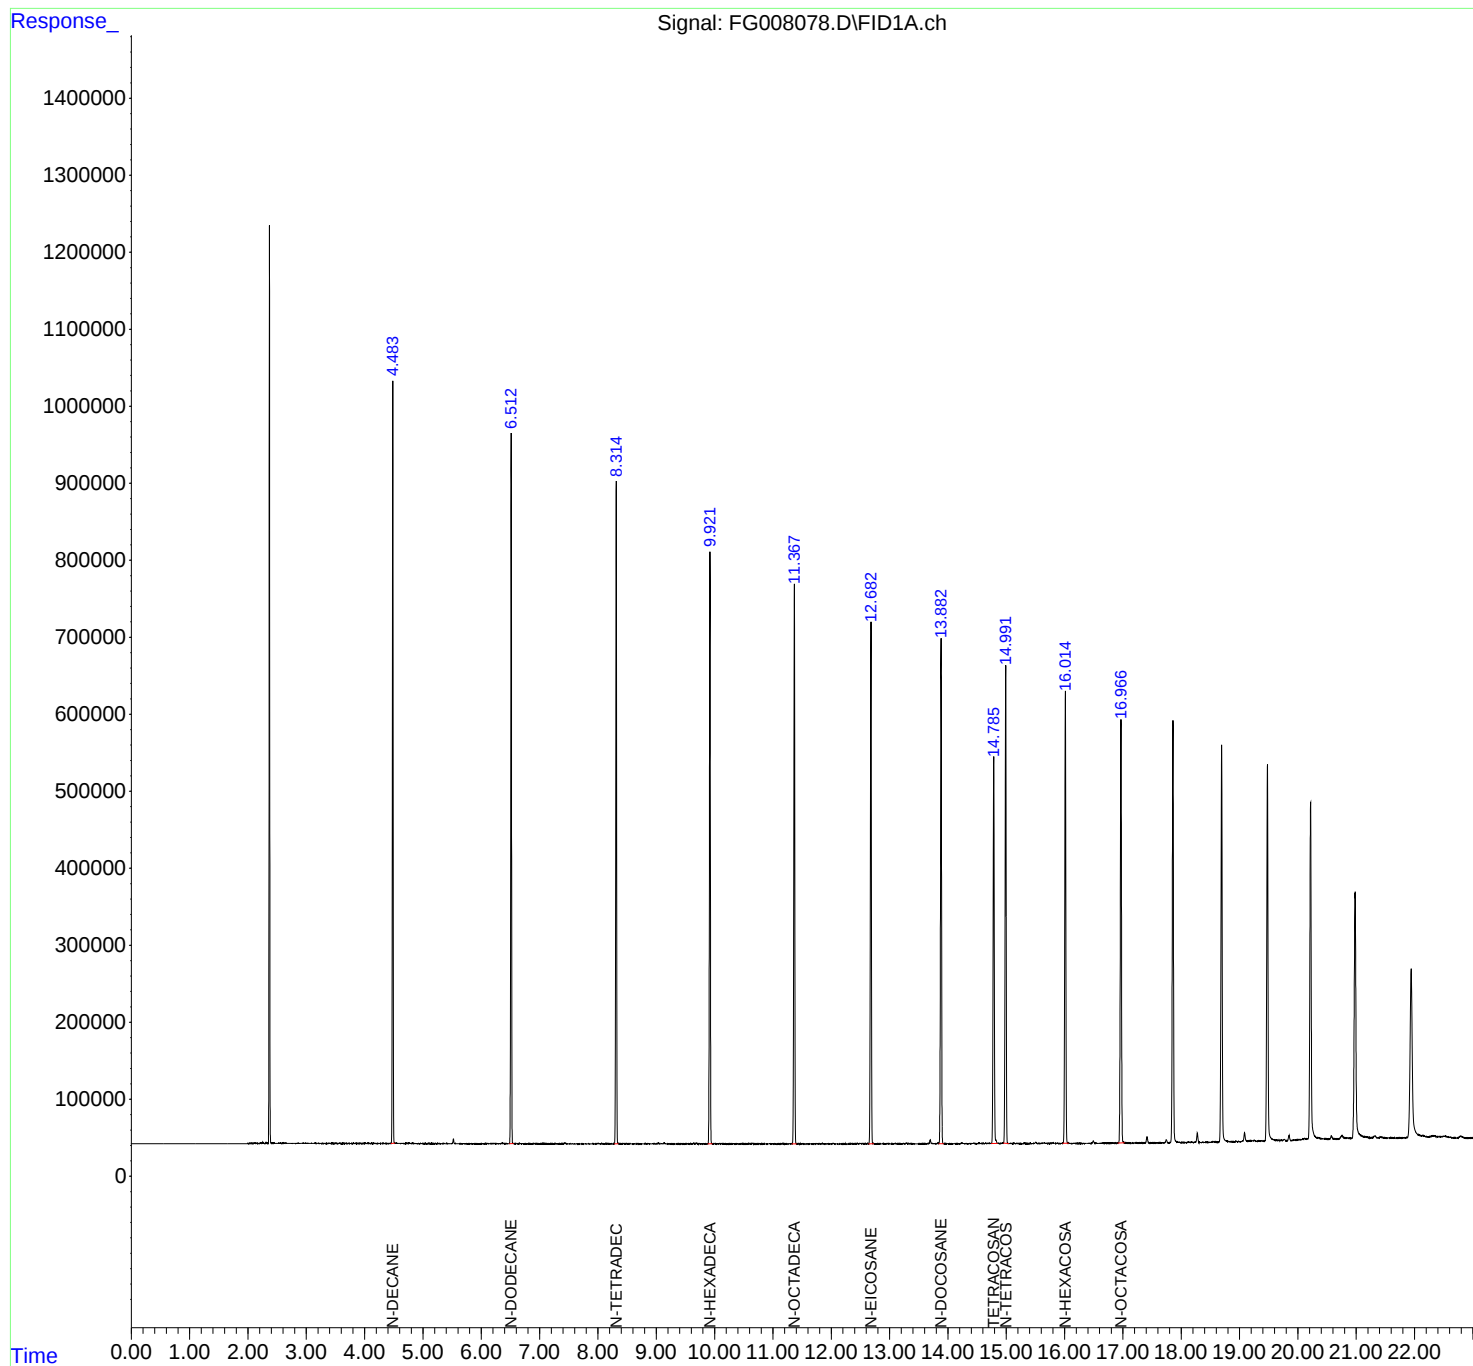

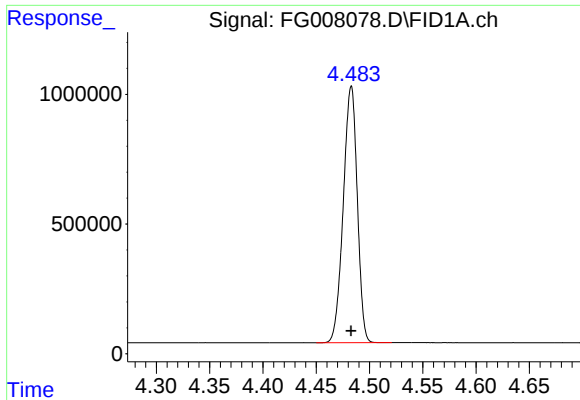


#2 N-DECANE

R.T.: 4.483 min
Delta R.T.: 0.000 min
Response: 9039367
Conc: 59.80 ug/ml

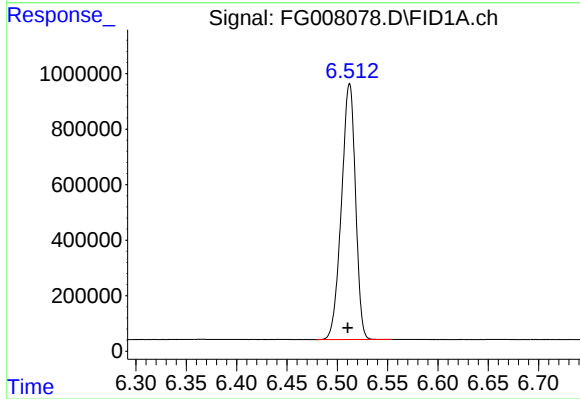


#3 N-DODECANE

R.T.: 6.512 min
Delta R.T.: 0.002 min
Response: 8955622
Conc: 58.54 ug/ml

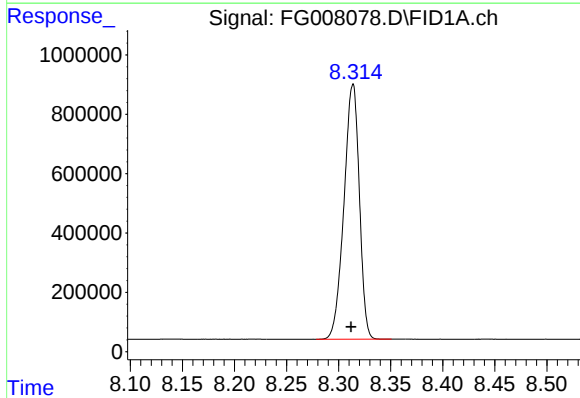


#4 N-TETRADECANE

R.T.: 8.314 min
Delta R.T.: 0.002 min
Response: 8841856
Conc: 56.65 ug/ml

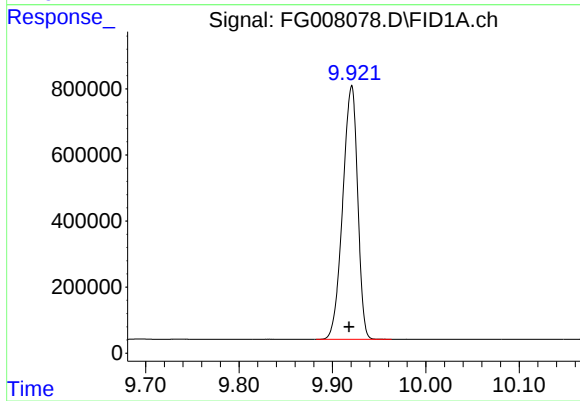


#5 N-HEXADECANE

R.T.: 9.921 min
Delta R.T.: 0.003 min
Response: 8523029
Conc: 55.01 ug/ml

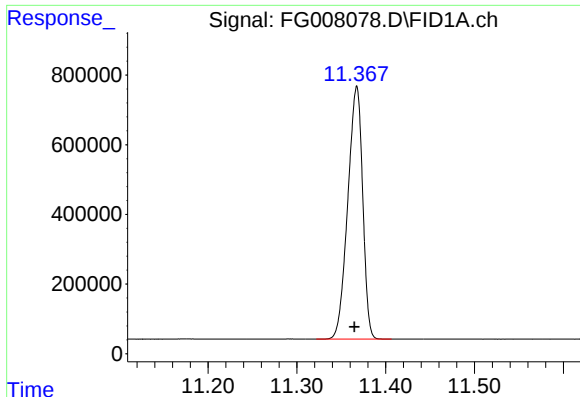


#6 N-OCTADECANE

R.T.: 11.367 min
Delta R.T.: 0.003 min
Response: 8442930
Conc: 53.70 ug/ml

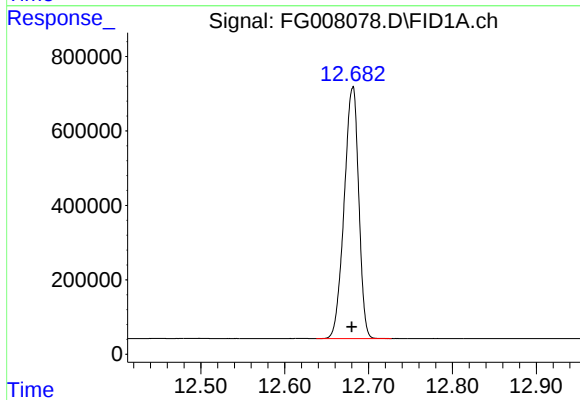


#7 N-EICOSANE

R.T.: 12.681 min
Delta R.T.: 0.002 min
Response: 8148397
Conc: 52.58 ug/ml

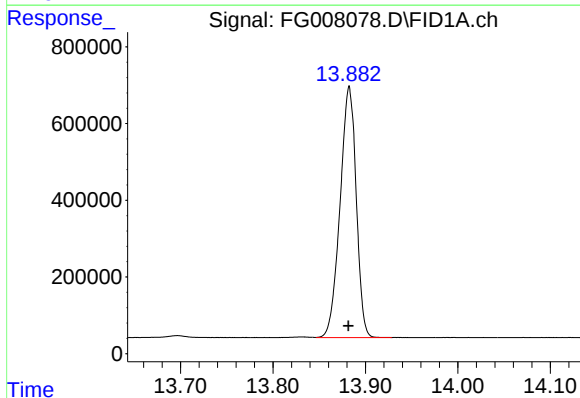


#8 N-DOCOSANE

R.T.: 13.882 min
Delta R.T.: 0.001 min
Response: 7941167
Conc: 51.68 ug/ml

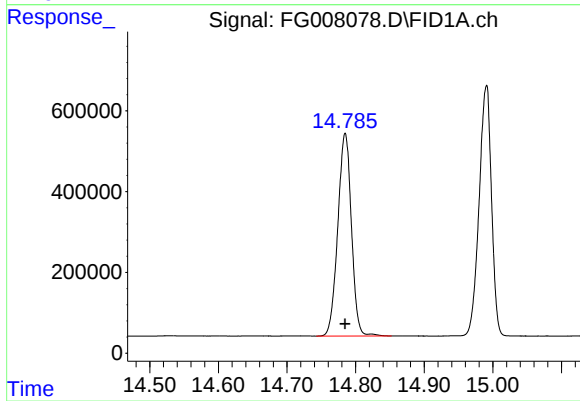


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 6921915
Conc: 51.99 ug/ml

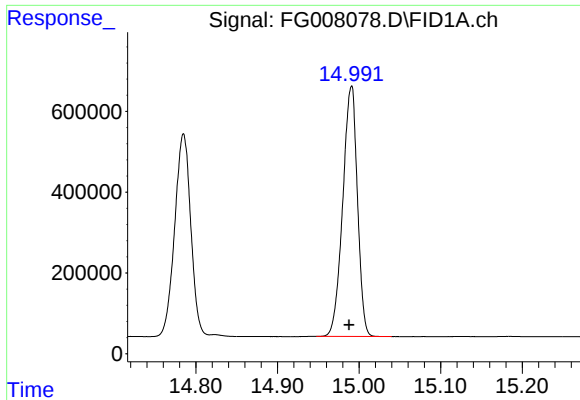


#10 N-TETRACOSANE

R.T.: 14.991 min
Delta R.T.: 0.003 min
Response: 7756640
Conc: 50.98 ug/ml

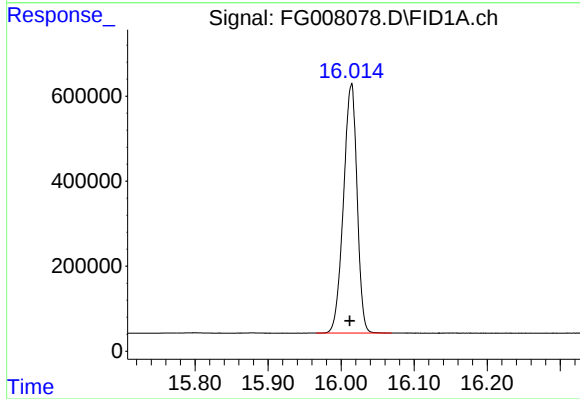

#11 N-HEXACOSANE

R.T.: 16.014 min
Delta R.T.: 0.002 min
Response: 7579986
Conc: 50.89 ug/ml

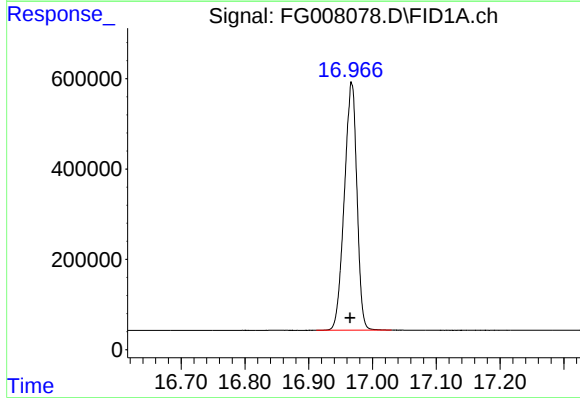

#12 N-OCTACOSANE

R.T.: 16.967 min
Delta R.T.: 0.003 min
Response: 7534229
Conc: 51.45 ug/ml