

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051519\
 Data File : FG004950.D
 Signal(s) : FID1A.ch
 Acq On : 15 May 2019 17:53
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 16 01:26:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.789	6036147	50.298 ug/ml
Target Compounds			
2) N-DECANE	4.485	7484258	52.951 ug/ml
3) N-DODECANE	6.516	7533745	52.512 ug/ml
4) N-TETRADECANE	8.319	7450126	51.915 ug/ml
5) N-HEXADECANE	9.925	7429849	51.436 ug/ml
6) N-OCTADECANE	11.372	7282882	51.082 ug/ml
7) N-EICOSANE	12.686	7198552	50.793 ug/ml
8) N-DOCOSANE	13.888	6999200	50.504 ug/ml
10) N-TETRACOSANE	14.994	6783885	50.075 ug/ml
11) N-HEXACOSANE	16.015	6508980	49.567 ug/ml
12) N-OCTACOSANE	16.966	6212560	48.871 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051519\
Data File : FG004950.D
Signal(s) : FID1A.ch
Acq On : 15 May 2019 17:53
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 16 01:26:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

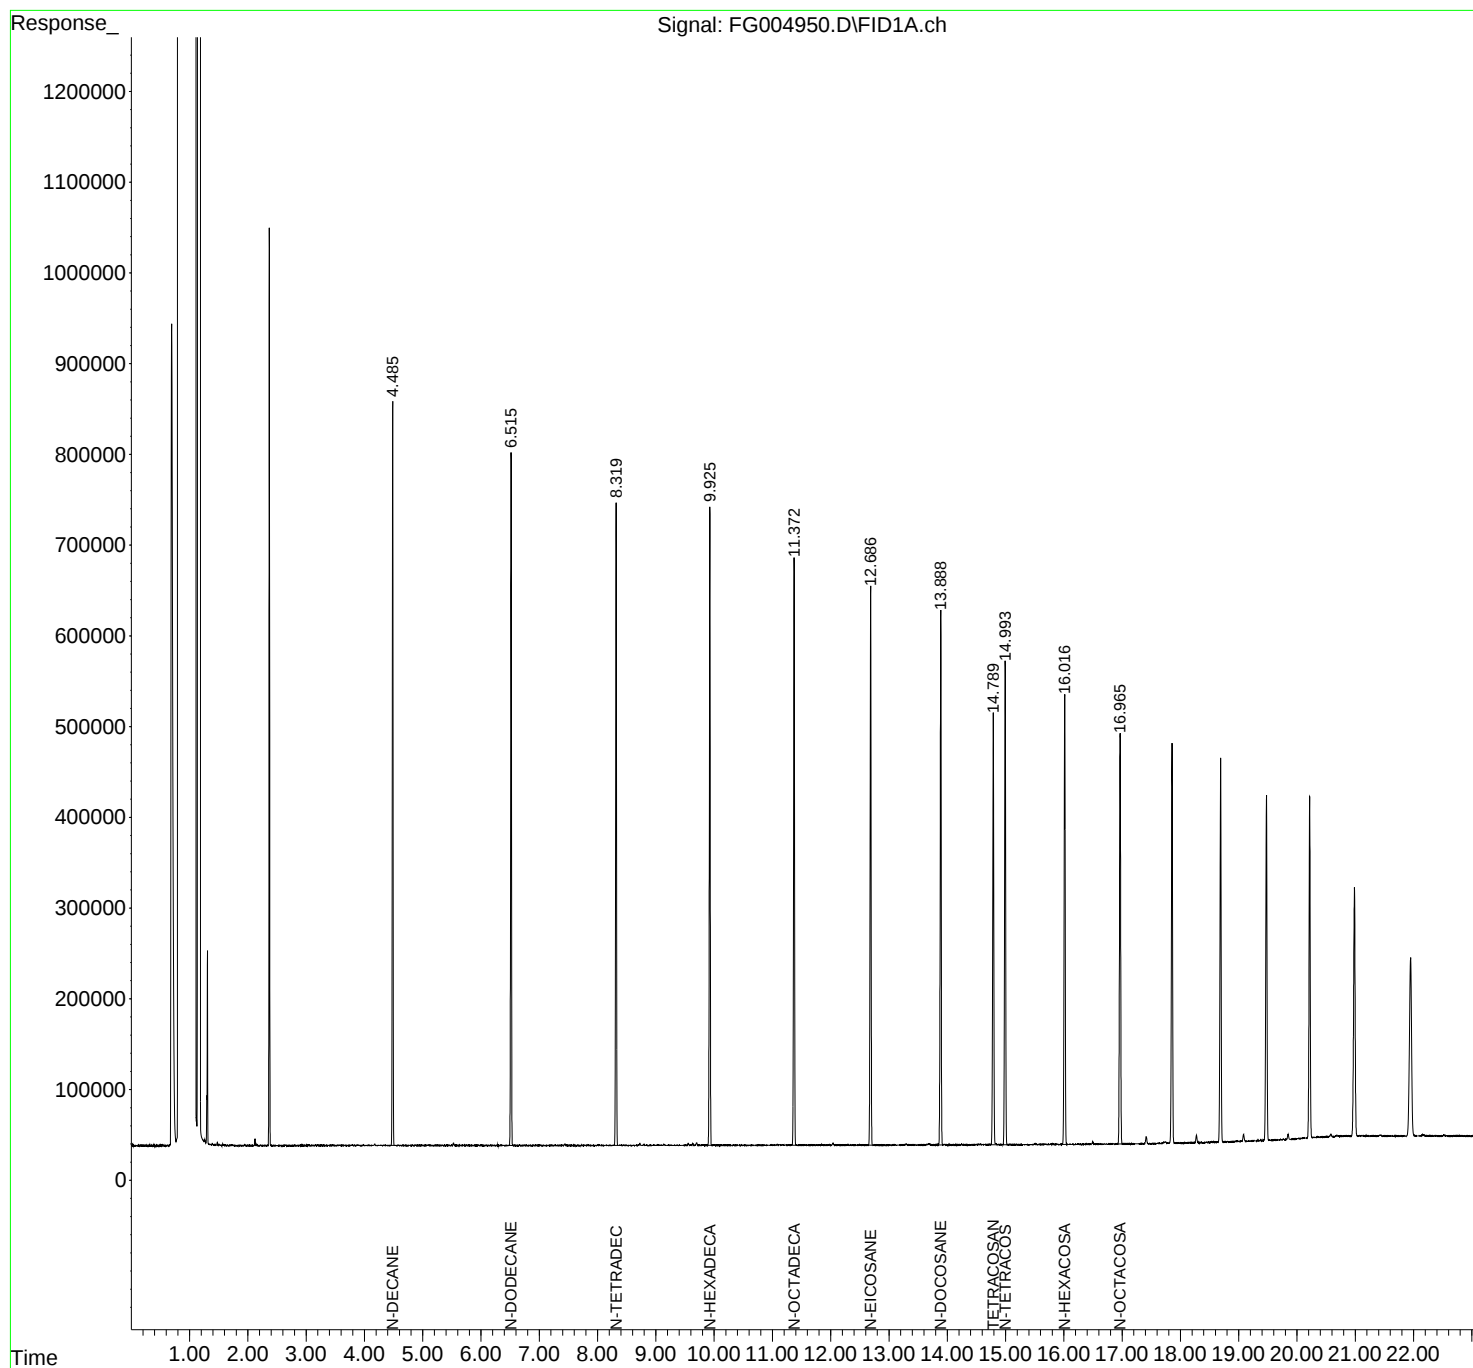

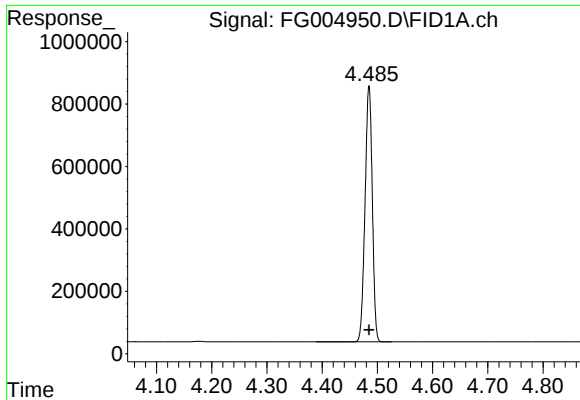


#2 N-DECANE

R.T.: 4.485 min
Delta R.T.: 0.000 min
Response: 7484258
Conc: 52.95 ug/ml

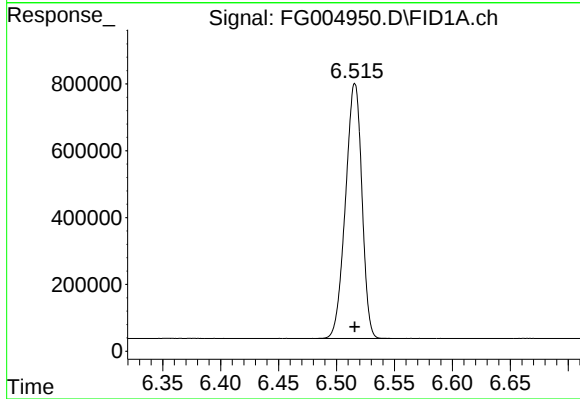


#3 N-DODECANE

R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 7533745
Conc: 52.51 ug/ml

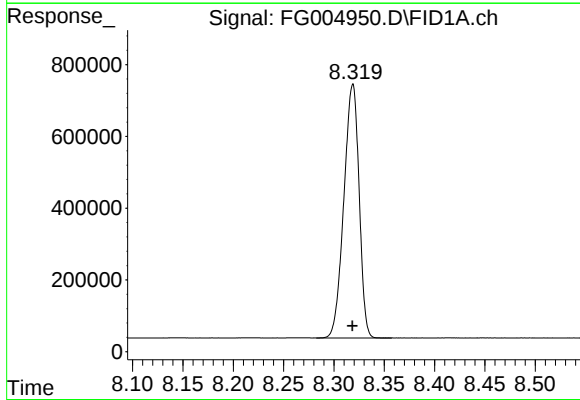


#4 N-TETRADECANE

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 7450126
Conc: 51.92 ug/ml

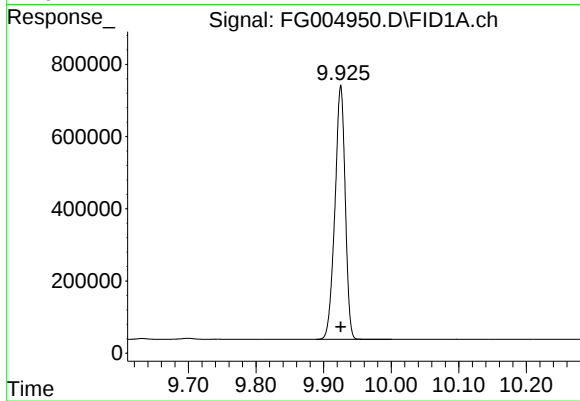


#5 N-HEXADECANE

R.T.: 9.925 min
Delta R.T.: 0.000 min
Response: 7429849
Conc: 51.44 ug/ml

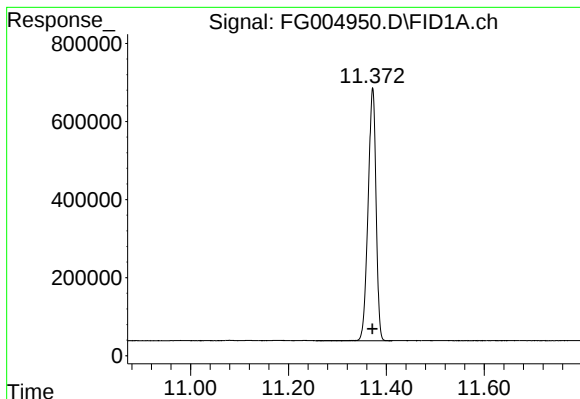


#6 N-OCTADECANE

R.T.: 11.372 min
Delta R.T.: 0.000 min
Response: 7282882
Conc: 51.08 ug/ml

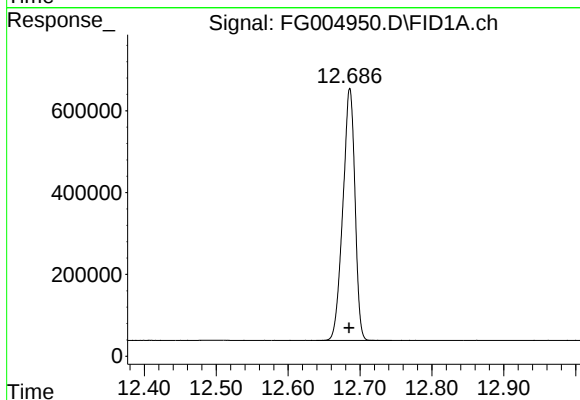


#7 N-EICOSANE

R.T.: 12.686 min
Delta R.T.: 0.001 min
Response: 7198552
Conc: 50.79 ug/ml

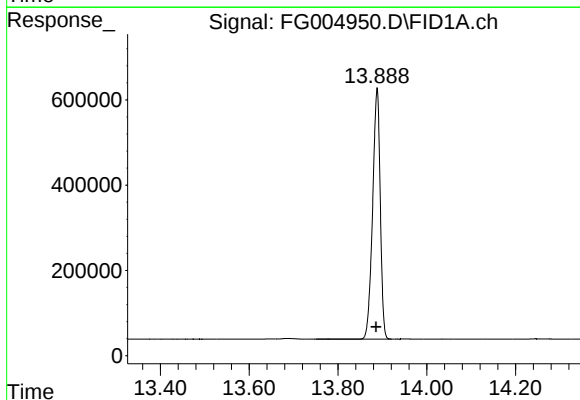


#8 N-DOCOSANE

R.T.: 13.888 min
Delta R.T.: 0.002 min
Response: 6999200
Conc: 50.50 ug/ml

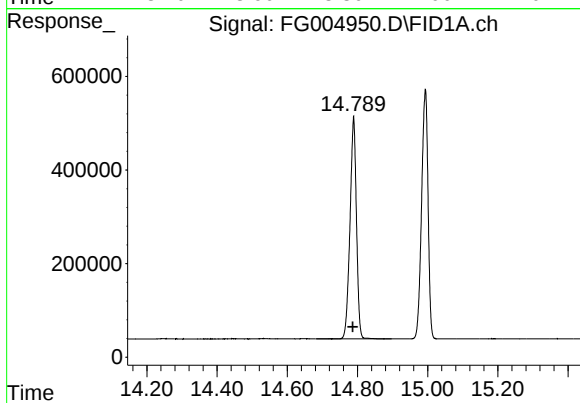


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.789 min
Delta R.T.: 0.003 min
Response: 6036147
Conc: 50.30 ug/ml

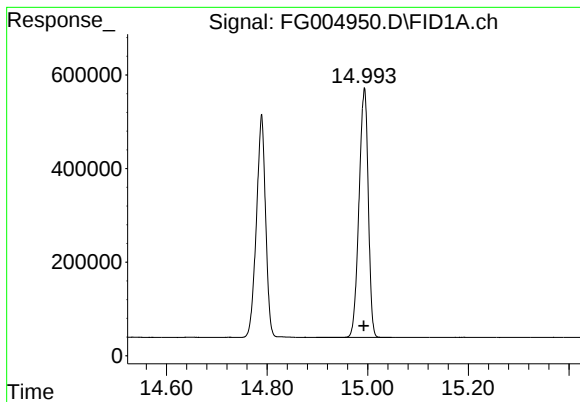


#10 N-TETRACOSANE

R.T.: 14.994 min
Delta R.T.: 0.001 min
Response: 6783885
Conc: 50.08 ug/ml

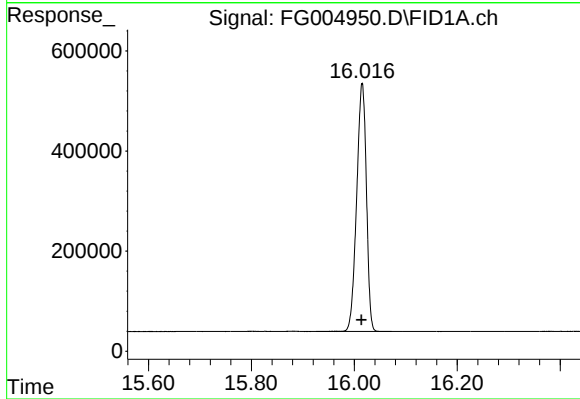

#11 N-HEXACOSANE

R.T.: 16.015 min
Delta R.T.: 0.002 min
Response: 6508980
Conc: 49.57 ug/ml

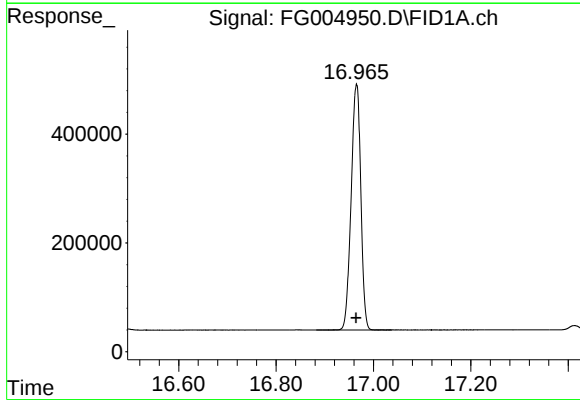

#12 N-OCTACOSANE

R.T.: 16.966 min
Delta R.T.: 0.001 min
Response: 6212560
Conc: 48.87 ug/ml