

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
 Data File : FG004971.D
 Signal(s) : FID1A.ch
 Acq On : 17 May 2019 15:55
 Operator : AJ\SJ
 Sample : K2884-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 MW-00-20190515

Integration File: autoint1.e
 Quant Time: May 18 04:50:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2261123	18.842 ug/ml
Target Compounds			
2) N-DECANE	4.455	25954	0.184 ug/ml
4) N-TETRADECANE	8.343	28779	0.201 ug/ml
5) N-HEXADECANE	9.887	43313	0.300 ug/ml
12) N-OCTACOSANE	16.962	43093	0.339 ug/ml
13) N-TRIACONTANE	17.852	54653	0.435 ug/ml
14) N-DOTRIACONTANE	18.688	43175	0.360 ug/ml
15) N-TETRATRIACONTANE	19.474	11502	0.102 ug/ml
16) N-HEXATRIACONTANE	20.216	16674	0.157 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
Data File : FG004971.D
Signal(s) : FID1A.ch
Acq On : 17 May 2019 15:55
Operator : AJ\SJ
Sample : K2884-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-00-20190515

Integration File: autoint1.e
Quant Time: May 18 04:50:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

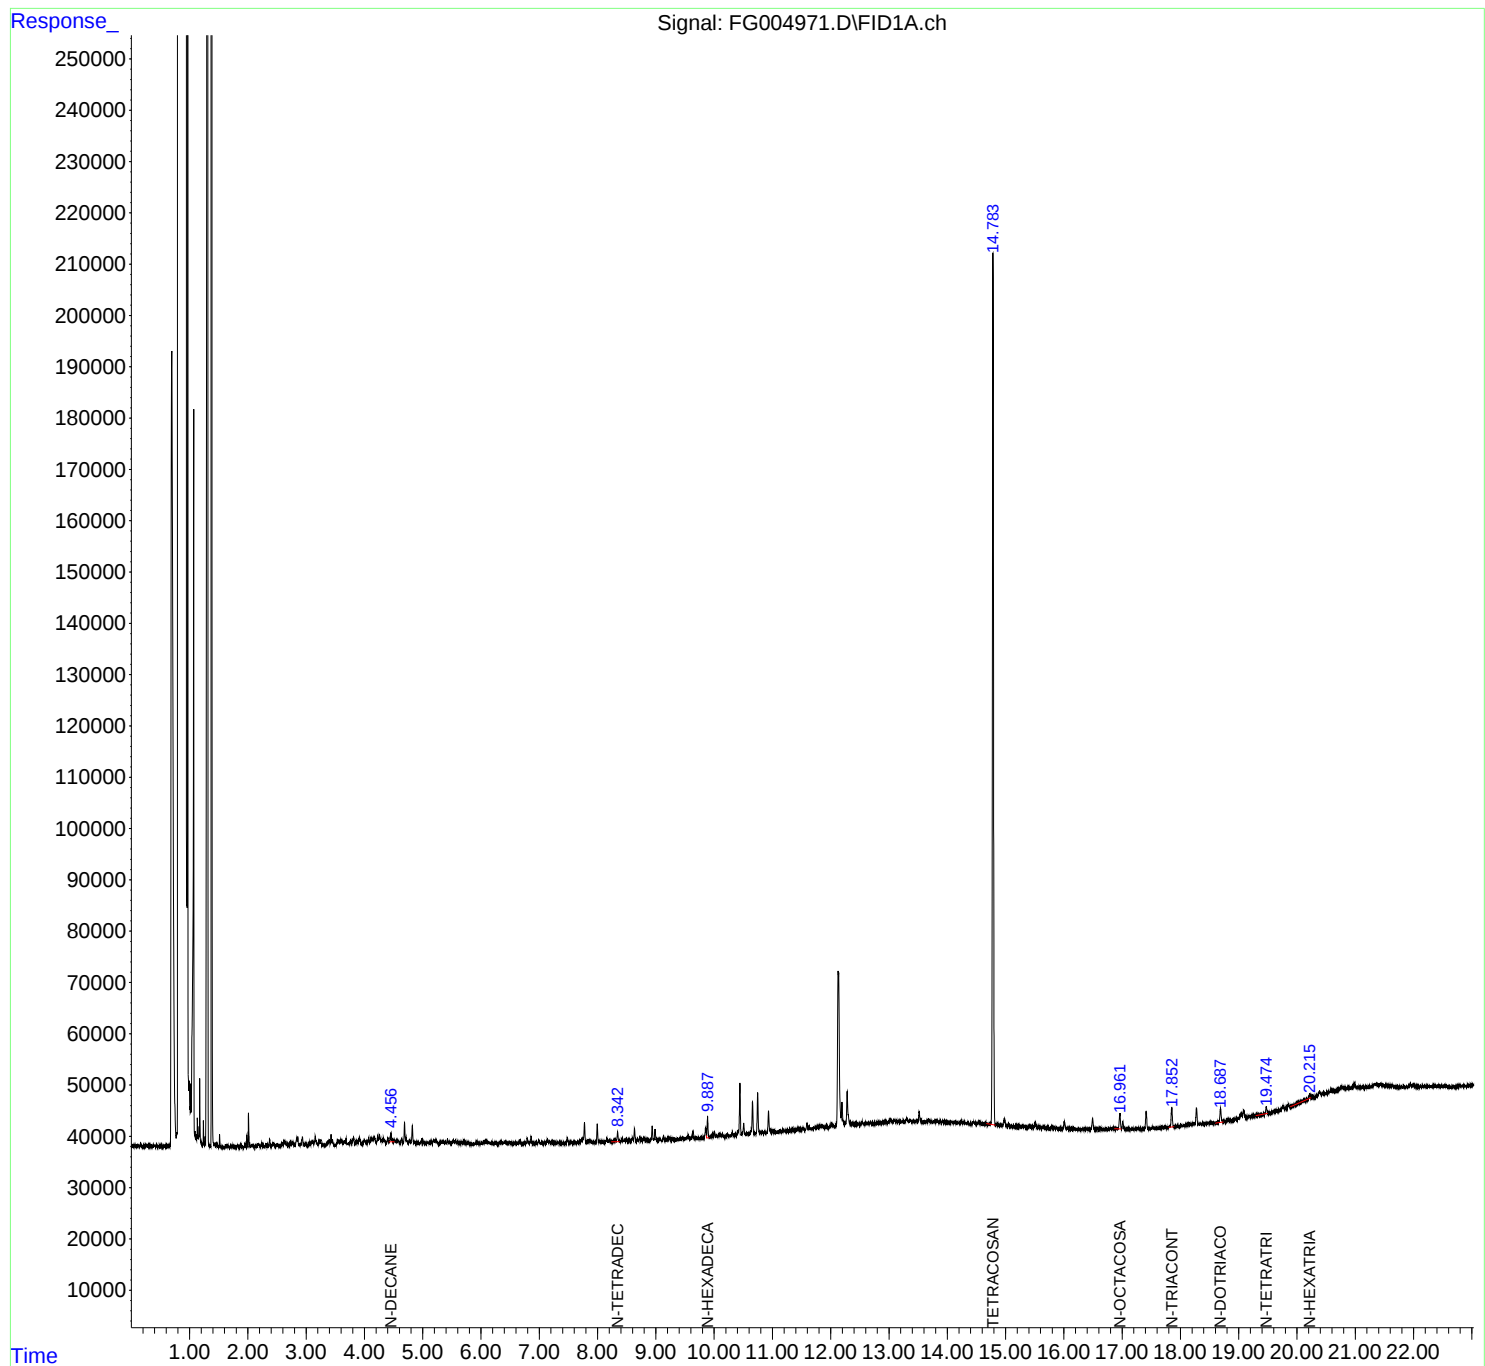


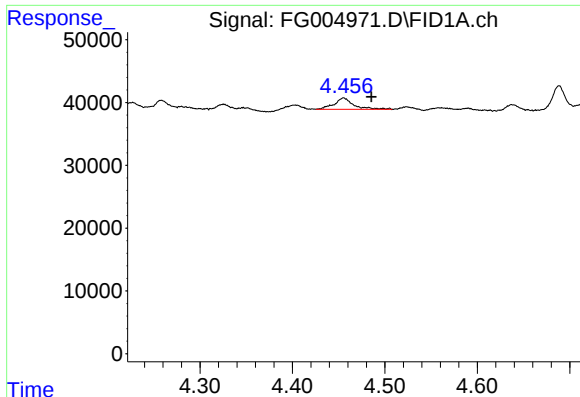

#2 N-DECANE


R.T.: 4.455 min
Delta R.T.: -0.030 min
Response: 25954
Conc: 0.18 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-00-20190515

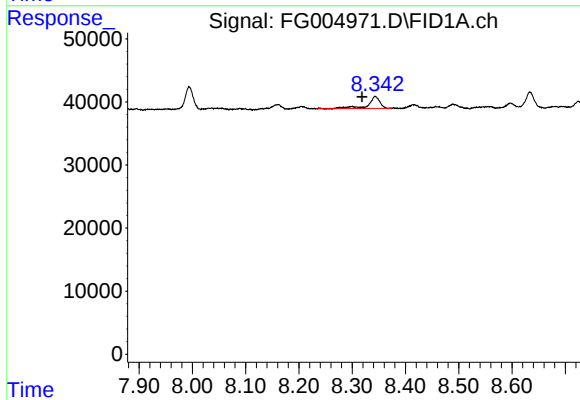


#4 N-TETRADECANE

R.T.: 8.343 min
Delta R.T.: 0.025 min
Response: 28779
Conc: 0.20 ug/ml

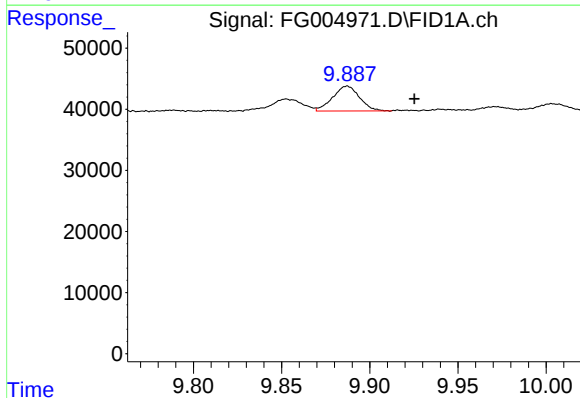


#5 N-HEXADECANE

R.T.: 9.887 min
Delta R.T.: -0.038 min
Response: 43313
Conc: 0.30 ug/ml

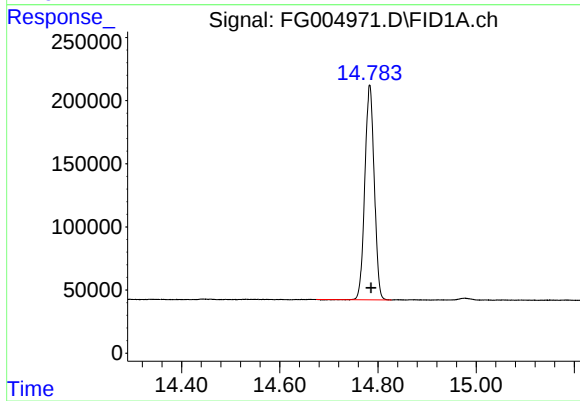

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.783 min
Delta R.T.: -0.003 min
Response: 2261123
Conc: 18.84 ug/ml

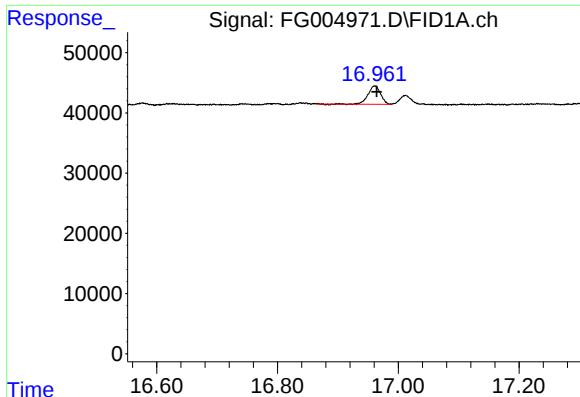

#12 N-OCTACOSANE


R.T.: 16.962 min
Delta R.T.: -0.003 min
Response: 43093
Conc: 0.34 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-00-20190515

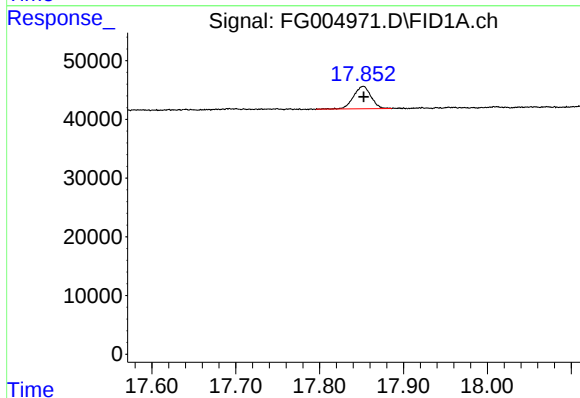


#13 N-TRIACONTANE

R.T.: 17.852 min
Delta R.T.: 0.000 min
Response: 54653
Conc: 0.43 ug/ml

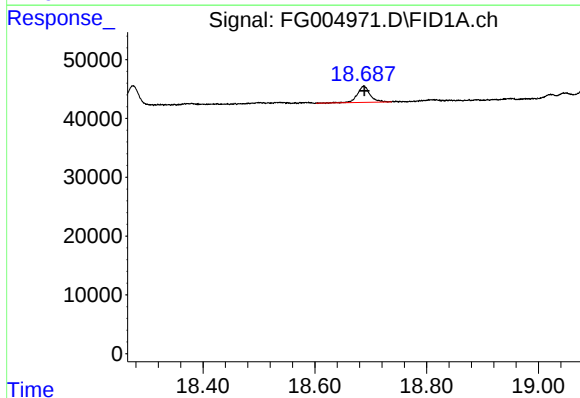


#14 N-DOTRIACONTANE

R.T.: 18.688 min
Delta R.T.: -0.001 min
Response: 43175
Conc: 0.36 ug/ml

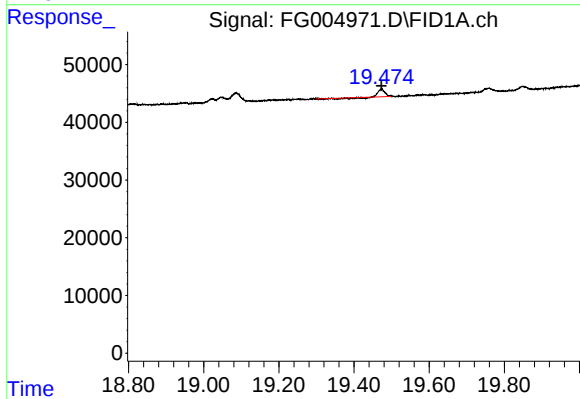

#15 N-TETRATRIACONTANE

R.T.: 19.474 min
Delta R.T.: 0.000 min
Response: 11502
Conc: 0.10 ug/ml

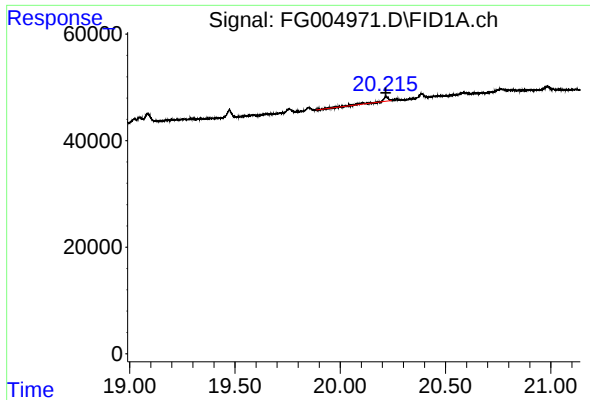

#16 N-HEXATRIACONTANE

R.T.: 20.216 min
Delta R.T.: 0.000 min
Response: 16674
Conc: 0.16 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-00-20190515