

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
 Data File : FG004974.D
 Signal(s) : FID1A.ch
 Acq On : 17 May 2019 17:23
 Operator : AJ\SJ
 Sample : K2884-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 MW-00-20190515-A

Integration File: autoint1.e
 Quant Time: May 18 04:51:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2019027	16.824 ug/ml
Target Compounds			
2) N-DECANE	4.456	15475	0.109 ug/ml
5) N-HEXADECANE	9.887	40098	0.278 ug/ml
12) N-OCTACOSANE	16.960	40950	0.322 ug/ml
13) N-TRIACONTANE	17.849	45048	0.358 ug/ml
14) N-DOTRIACONTANE	18.684	37428	0.312 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
Data File : FG004974.D
Signal(s) : FID1A.ch
Acq On : 17 May 2019 17:23
Operator : AJ\SJ
Sample : K2884-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-00-20190515-A

Integration File: autoint1.e
Quant Time: May 18 04:51:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

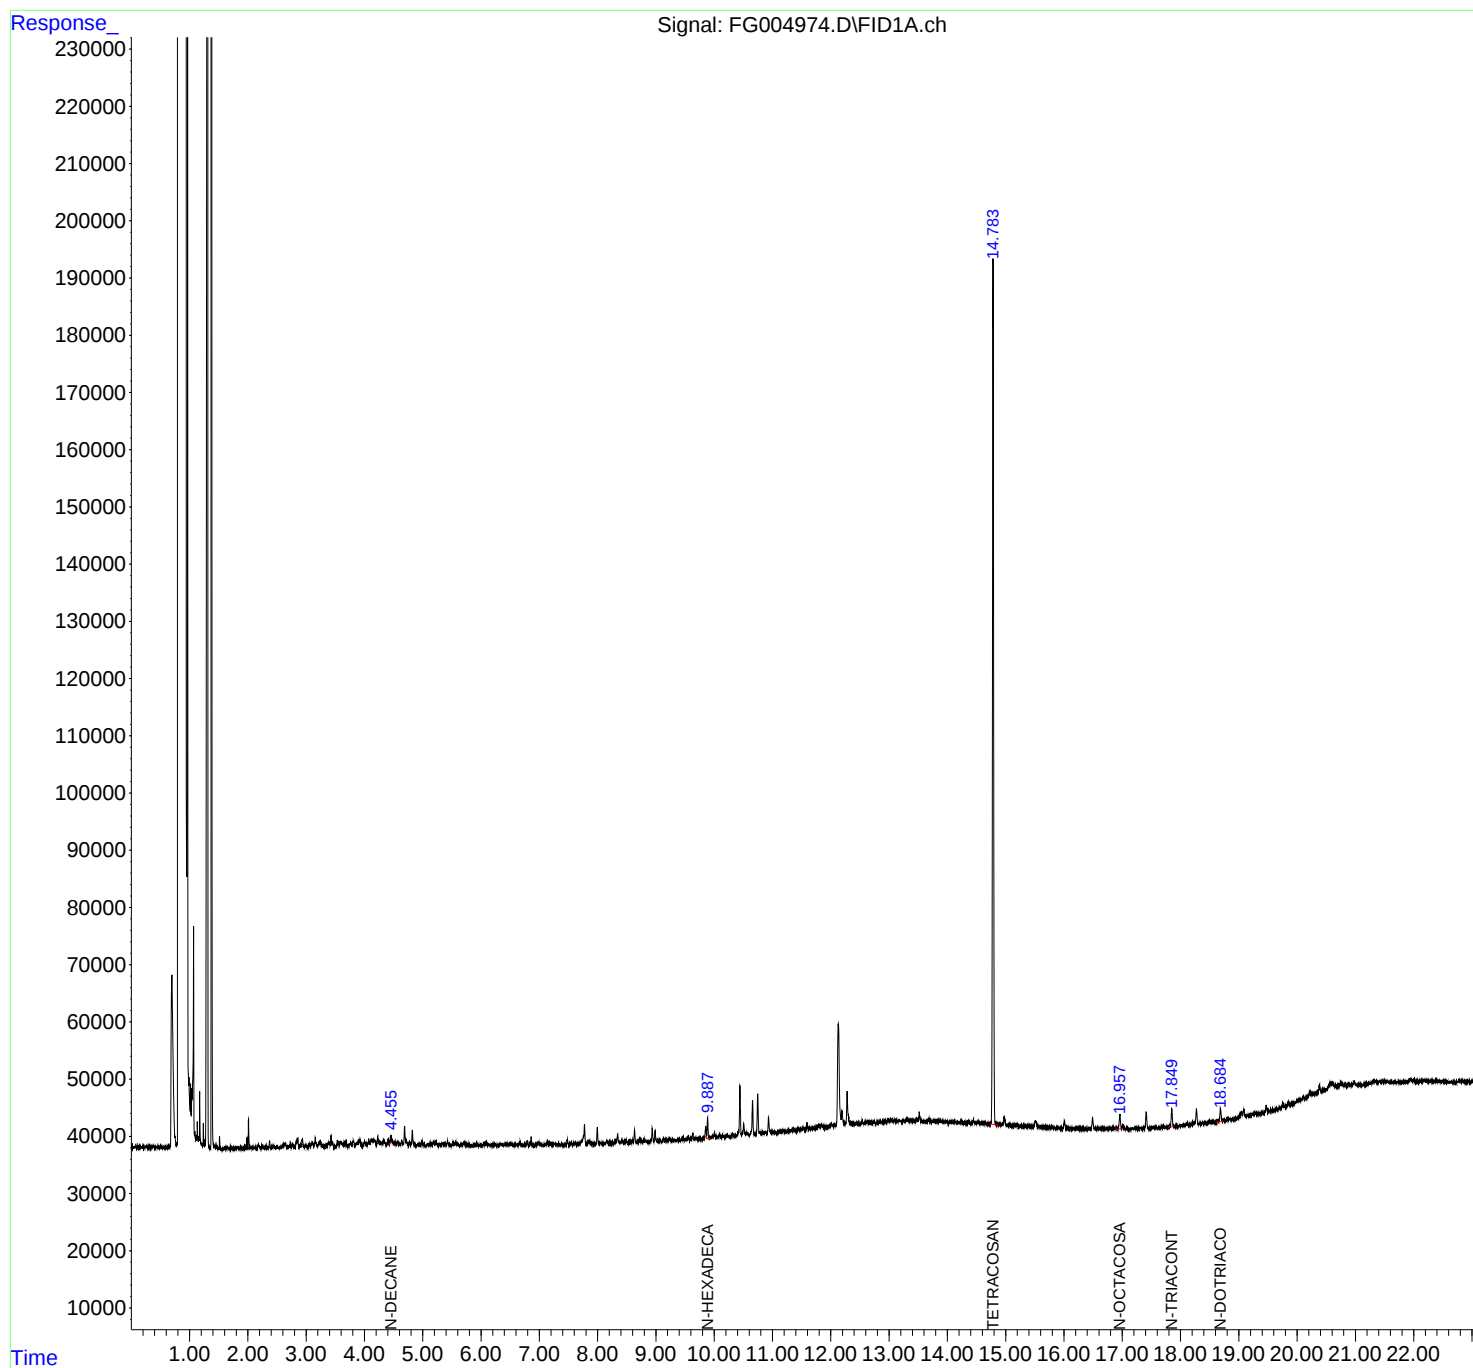


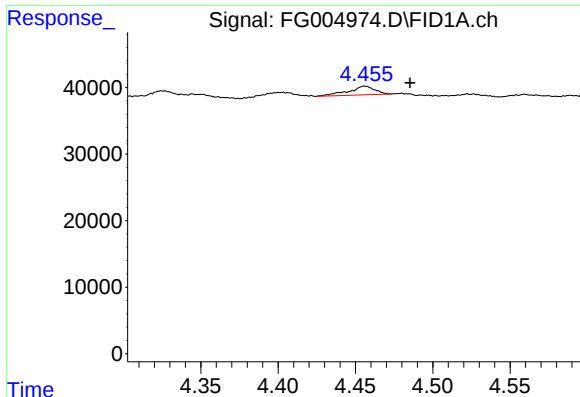

#2 N-DECANE


R.T.: 4.456 min
Delta R.T.: -0.029 min
Response: 15475
Conc: 0.11 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-00-20190515-A

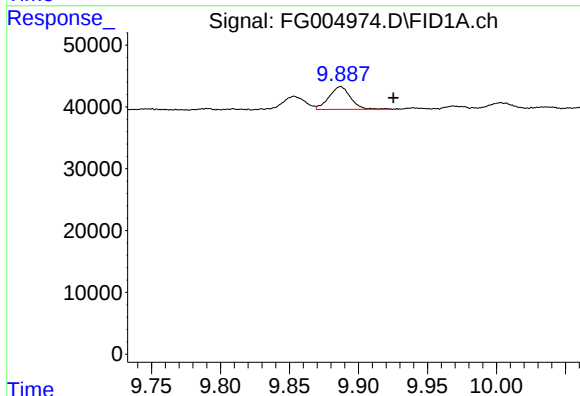


#5 N-HEXADECANE

R.T.: 9.887 min
Delta R.T.: -0.038 min
Response: 40098
Conc: 0.28 ug/ml

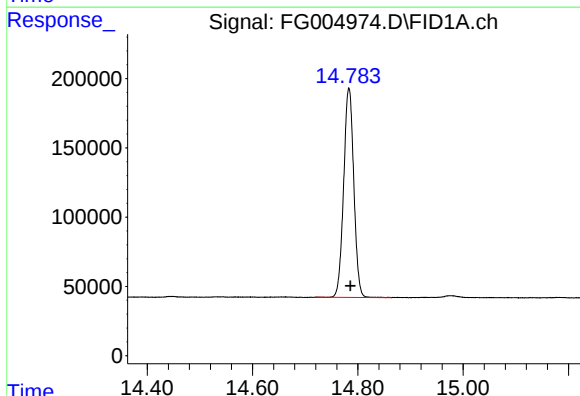


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.003 min
Response: 2019027
Conc: 16.82 ug/ml

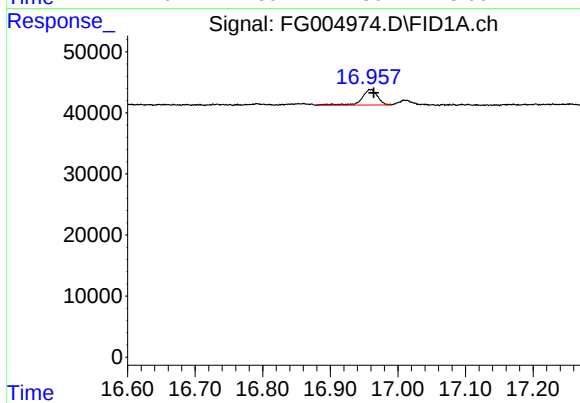

#12 N-OCTACOSANE


R.T.: 16.960 min
Delta R.T.: -0.004 min
Response: 40950
Conc: 0.32 ug/ml

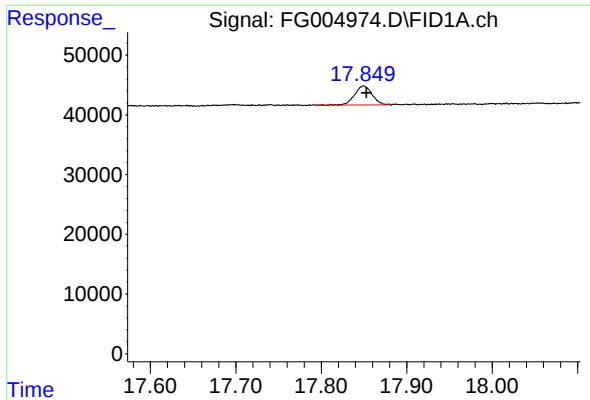

#13 N-TRIACONTANE

R.T.: 17.849 min
Delta R.T.: -0.003 min
Response: 45048
Conc: 0.36 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-00-20190515-A

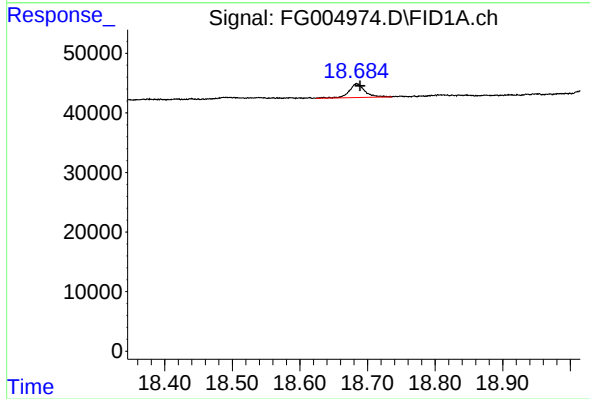

#14 N-DOTRIACONTANE

R.T.: 18.684 min
Delta R.T.: -0.005 min
Response: 37428
Conc: 0.31 ug/ml