

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
 Data File : FG004976.D
 Signal(s) : FID1A.ch
 Acq On : 17 May 2019 18:22
 Operator : AJ\SJ
 Sample : K2884-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 MW-07-20190515

Integration File: autoint1.e
 Quant Time: May 18 04:51:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2237580	18.645 ug/ml
Target Compounds			
3) N-DODECANE	6.505	32758	0.228 ug/ml
5) N-HEXADECANE	9.955	25795	0.179 ug/ml
12) N-OCTACOSANE	16.960	36329	0.286 ug/ml
13) N-TRIACONTANE	17.850	44088	0.351 ug/ml
14) N-DOTRIACONTANE	18.686	35469	0.296 ug/ml
16) N-HEXATRIACONTANE	20.212	10204	0.096 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
Data File : FG004976.D
Signal(s) : FID1A.ch
Acq On : 17 May 2019 18:22
Operator : AJ\SJ
Sample : K2884-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-07-20190515

Integration File: autoint1.e
Quant Time: May 18 04:51:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

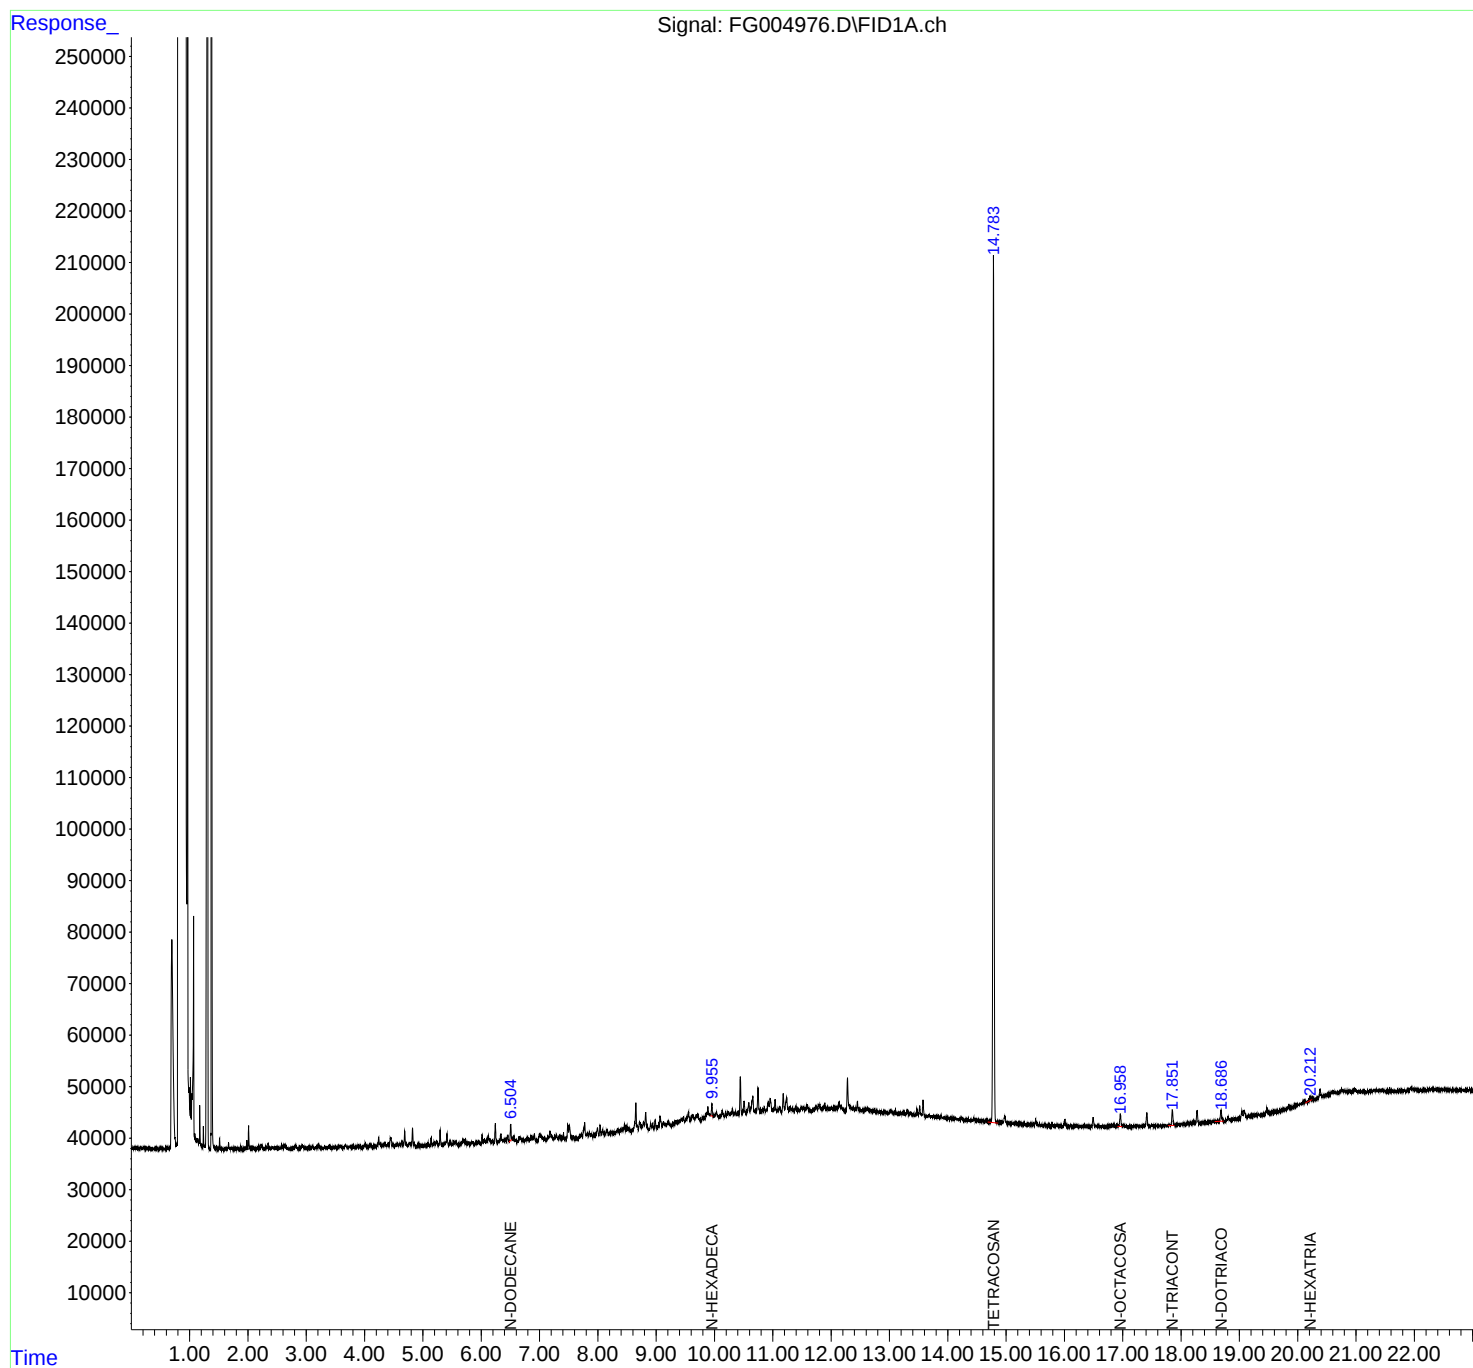


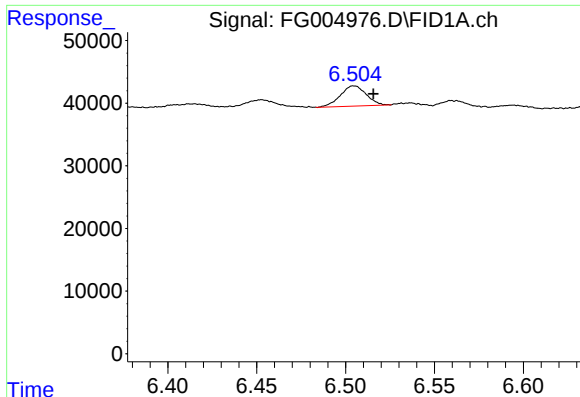

#3 N-DODECANE


R.T.: 6.505 min
Delta R.T.: -0.011 min
Response: 32758
Conc: 0.23 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-07-20190515

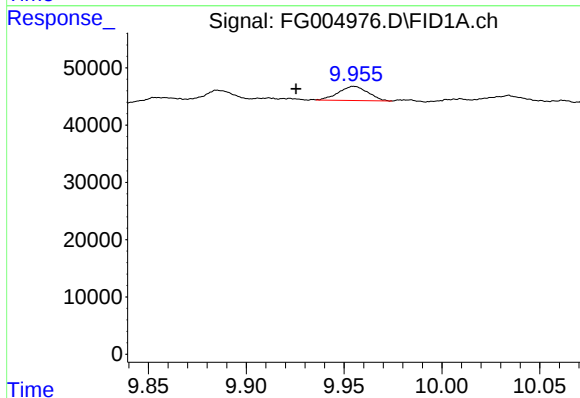


#5 N-HEXADECANE

R.T.: 9.955 min
Delta R.T.: 0.030 min
Response: 25795
Conc: 0.18 ug/ml

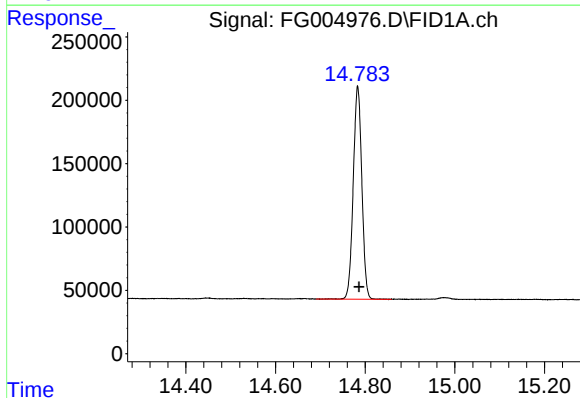


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.003 min
Response: 2237580
Conc: 18.65 ug/ml

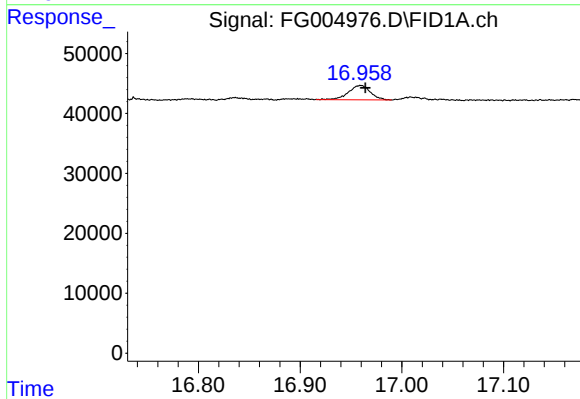

#12 N-OCTACOSANE


R.T.: 16.960 min
Delta R.T.: -0.005 min
Response: 36329
Conc: 0.29 ug/ml

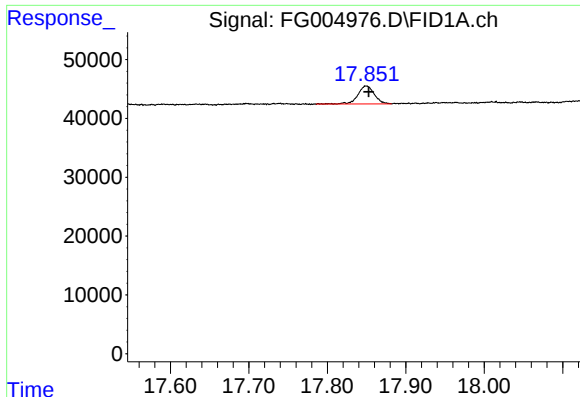

#13 N-TRIACONTANE


R.T.: 17.850 min
Delta R.T.: -0.003 min
Response: 44088
Conc: 0.35 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-07-20190515

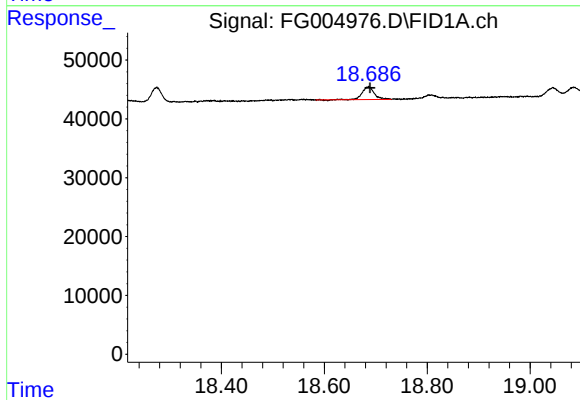

#14 N-DOTRIACONTANE

R.T.: 18.686 min
Delta R.T.: -0.003 min
Response: 35469
Conc: 0.30 ug/ml

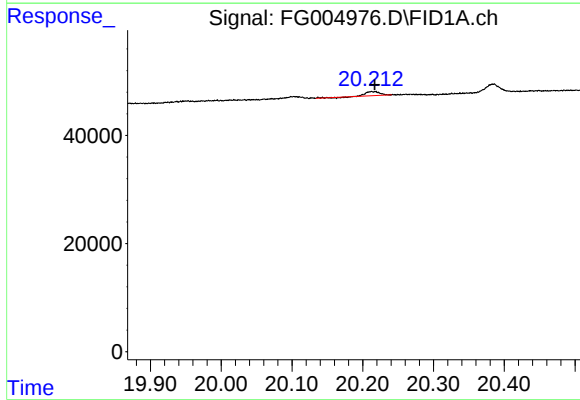

#16 N-HEXATRIACONTANE

R.T.: 20.212 min
Delta R.T.: -0.005 min
Response: 10204
Conc: 0.10 ug/ml