

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
 Data File : FG004977.D
 Signal(s) : FID1A.ch
 Acq On : 17 May 2019 18:52
 Operator : AJ\SJ
 Sample : K2884-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 EB-20190515

Integration File: autoint1.e
 Quant Time: May 18 04:52:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2253146	18.775 ug/ml
Target Compounds			
1) N-OCTANE	2.369	14048	0.102 ug/ml
12) N-OCTACOSANE	16.960	28039	0.221 ug/ml
13) N-TRIACONTANE	17.850	38382	0.305 ug/ml
14) N-DOTRIACONTANE	18.684	29550	0.247 ug/ml
16) N-HEXATRIACONTANE	20.216	2587	0.024 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
Data File : FG004977.D
Signal(s) : FID1A.ch
Acq On : 17 May 2019 18:52
Operator : AJ\SJ
Sample : K2884-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EB-20190515

Integration File: autoint1.e
Quant Time: May 18 04:52:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

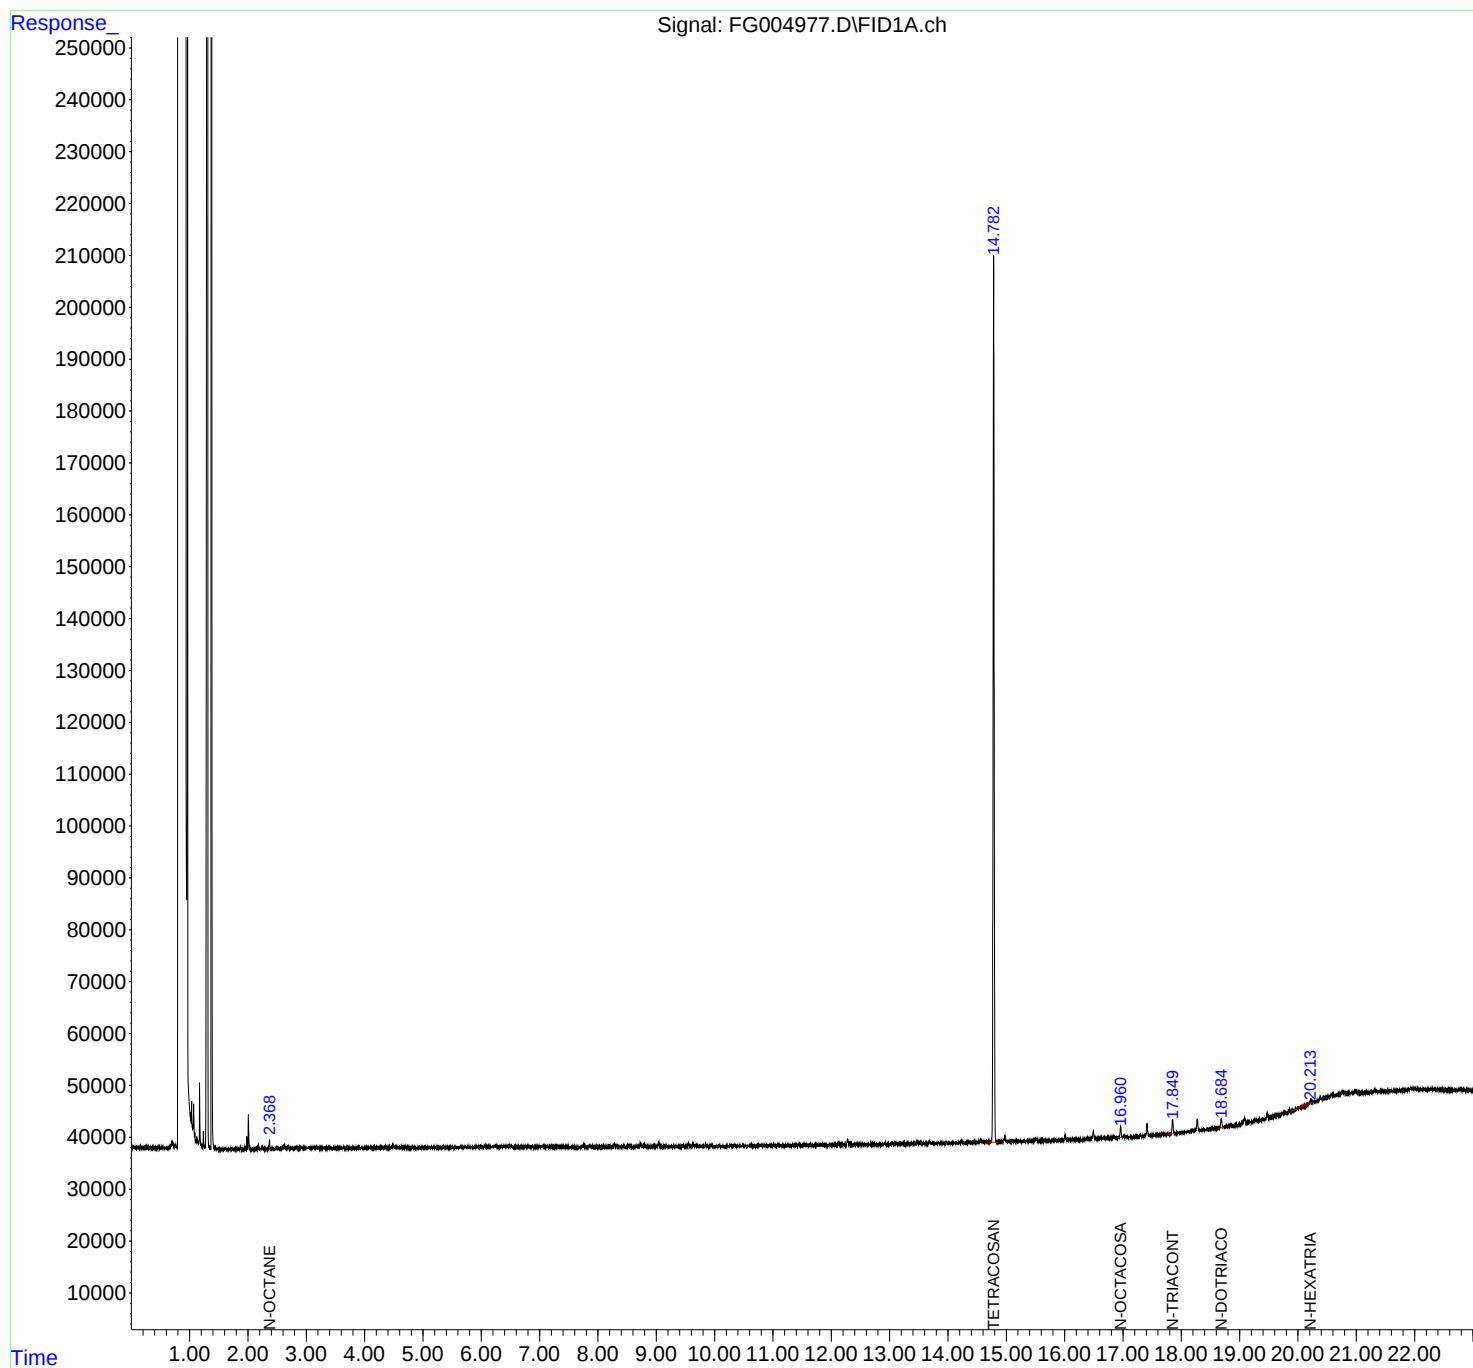


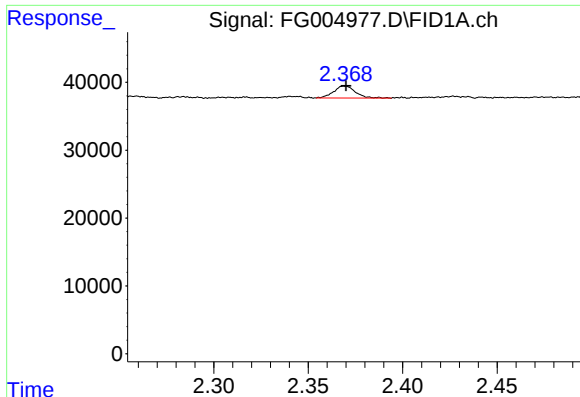

#1 N-OCTANE


R.T.: 2.369 min
Delta R.T.: 0.000 min
Response: 14048
Conc: 0.10 ug/ml

Instrument :
FID_G
ClientSampleId :
EB-20190515

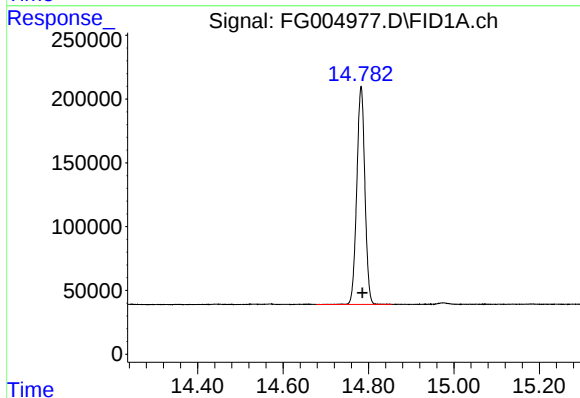


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.003 min
Response: 2253146
Conc: 18.78 ug/ml

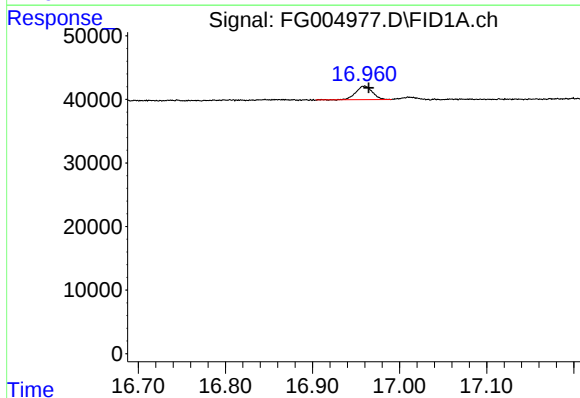


#12 N-OCTACOSANE

R.T.: 16.960 min
Delta R.T.: -0.005 min
Response: 28039
Conc: 0.22 ug/ml

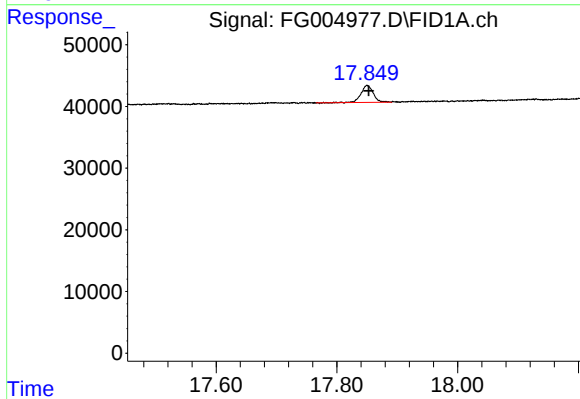

#13 N-TRIACONTANE


R.T.: 17.850 min
Delta R.T.: -0.003 min
Response: 38382
Conc: 0.31 ug/ml

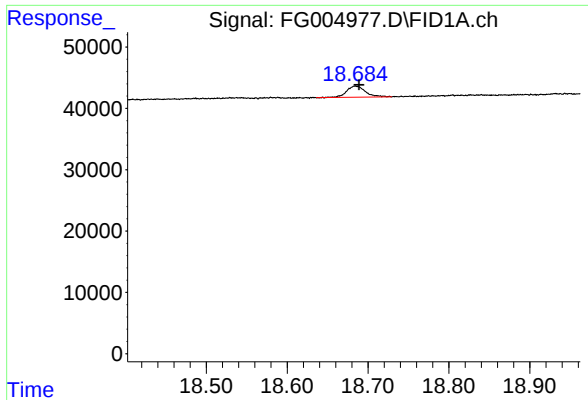

#14 N-DOTRIACONTANE

R.T.: 18.684 min
Delta R.T.: -0.004 min
Response: 29550
Conc: 0.25 ug/ml

Instrument :
FID_G
ClientSampleId :
EB-20190515

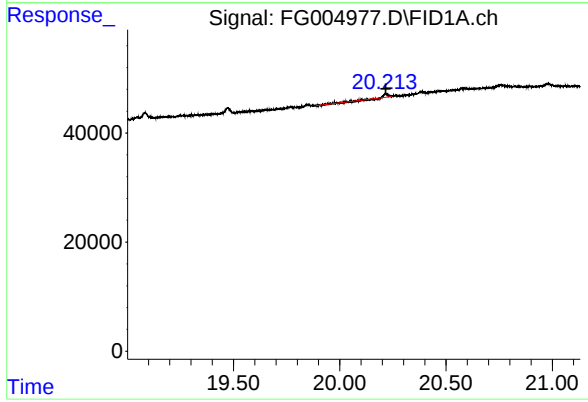

#16 N-HEXATRIACONTANE

R.T.: 20.216 min
Delta R.T.: -0.001 min
Response: 2587
Conc: 0.02 ug/ml