

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
Data File : FG004974.D
Signal(s) : FID1A.ch
Acq On : 17 May 2019 17:23
Operator : AJ\SJ
Sample : K2884-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-00-20190515-A

Integration File: autoint1.e
Quant Time: May 18 04:51:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2019027	16.824 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051719\
Data File : FG004974.D
Signal(s) : FID1A.ch
Acq On : 17 May 2019 17:23
Operator : AJ\SJ
Sample : K2884-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-00-20190515-A

Integration File: autoint1.e
Quant Time: May 18 04:51:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

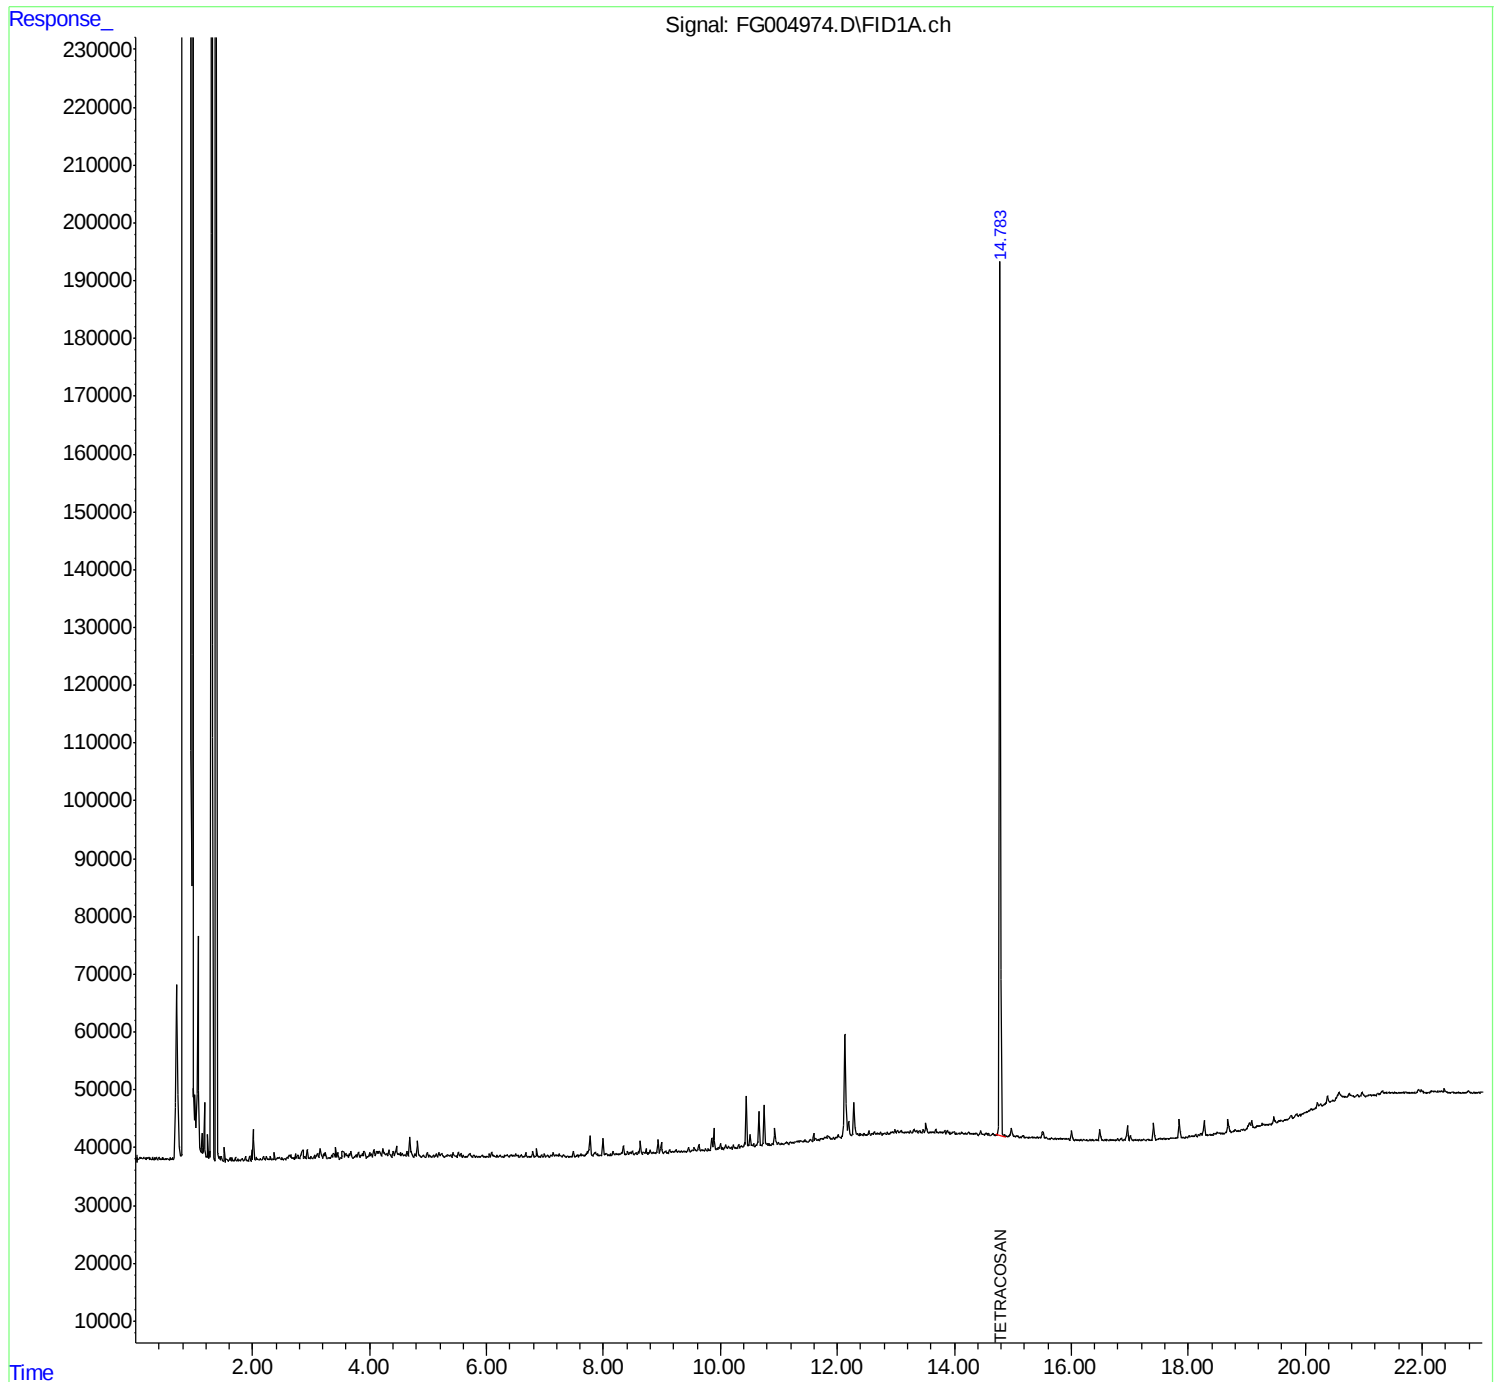

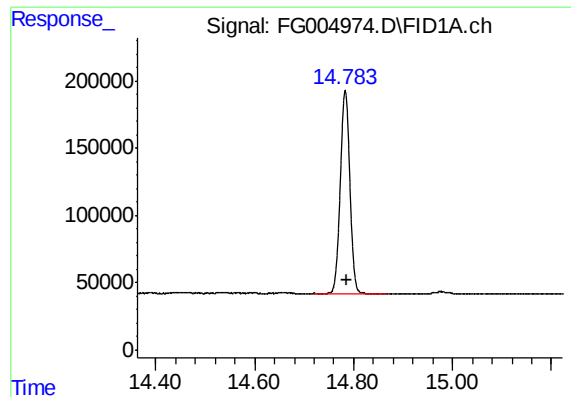

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.003 min
Response: 2019027
Conc: 16.82 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-00-20190515-A