

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051721\
 Data File : FG008097.D
 Signal(s) : FID1A.ch
 Acq On : 17 May 2021 12:23
 Operator : DD\AJ
 Sample : PB136186BL
 Misc : MDL-WATER-BL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 17 14:48:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
 Quant Title :
 QLast Update : Thu Apr 22 01:54:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	2365418	17.768 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.849	108161	0.757 ug/ml
14) N-DOTRIACONTANE	18.685	135480	0.993 ug/ml
15) N-TETRATRIACONTANE	19.469	96792	0.753 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051721\
Data File : FG008097.D
Signal(s) : FID1A.ch
Acq On : 17 May 2021 12:23
Operator : DD\AJ
Sample : PB136186BL
Misc : MDL-WATER-BL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 17 14:48:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

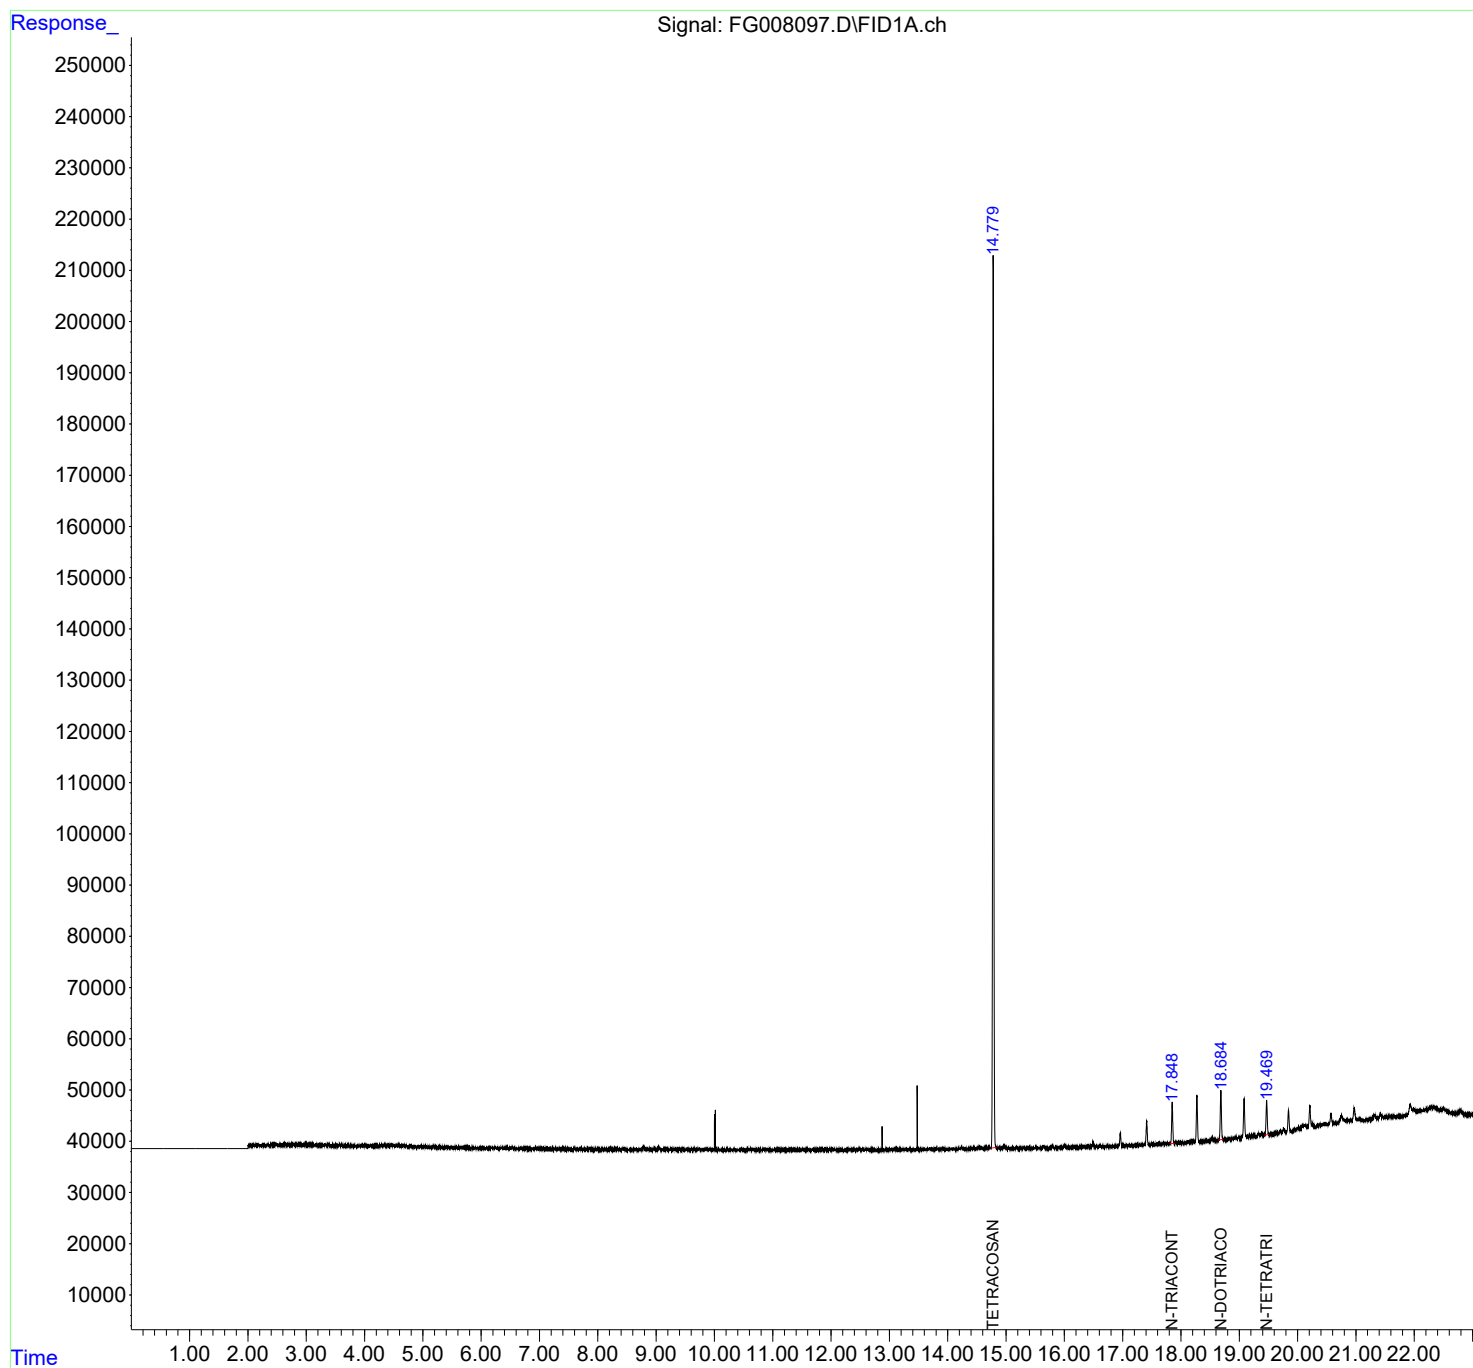


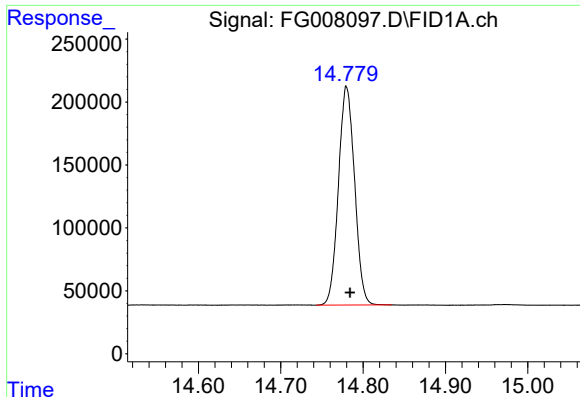

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.780 min
Delta R.T.: -0.004 min
Response: 2365418
Conc: 17.77 ug/ml

Instrument :
FID_G
ClientSampleId :

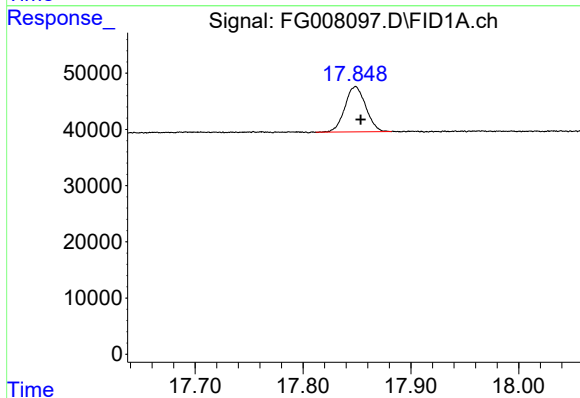


#13 N-TRIACONTANE

R.T.: 17.849 min
Delta R.T.: -0.005 min
Response: 108161
Conc: 0.76 ug/ml

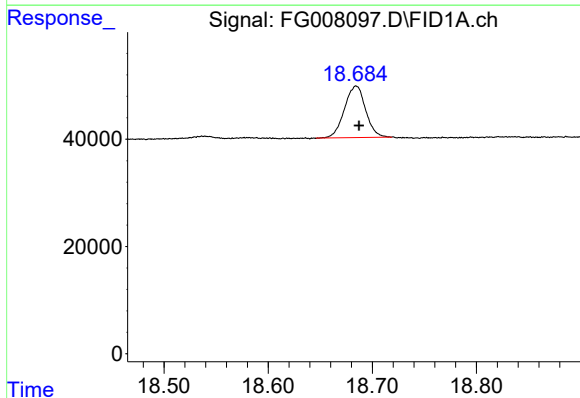

#14 N-DOTRIACONTANE

R.T.: 18.685 min
Delta R.T.: -0.003 min
Response: 135480
Conc: 0.99 ug/ml

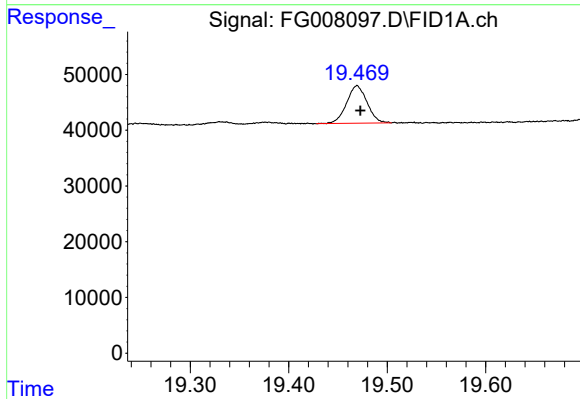

#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: -0.003 min
Response: 96792
Conc: 0.75 ug/ml