

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052019\
Data File : FG004983.D
Signal(s) : FID1A.ch
Acq On : 20 May 2019 10:57
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 21 01:06:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.513	3450376	24.050 ug/ml
11) N-HEXACOSANE	16.010	21712	0.165 ug/ml
12) N-OCTACOSANE	16.964	2975924	23.410 ug/ml
13) N-TRIACONTANE	17.850	59298	0.472 ug/ml
14) N-DOTRIACONTANE	18.687	57021	0.476 ug/ml
15) N-TETRATRIACONTANE	19.473	56674	0.504 ug/ml
16) N-HEXATRIACONTANE	20.214	16831	0.159 ug/ml
18) N-TETRACONTANE	21.996f	61886	0.635 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052019\
Data File : FG004983.D
Signal(s) : FID1A.ch
Acq On : 20 May 2019 10:57
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 21 01:06:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

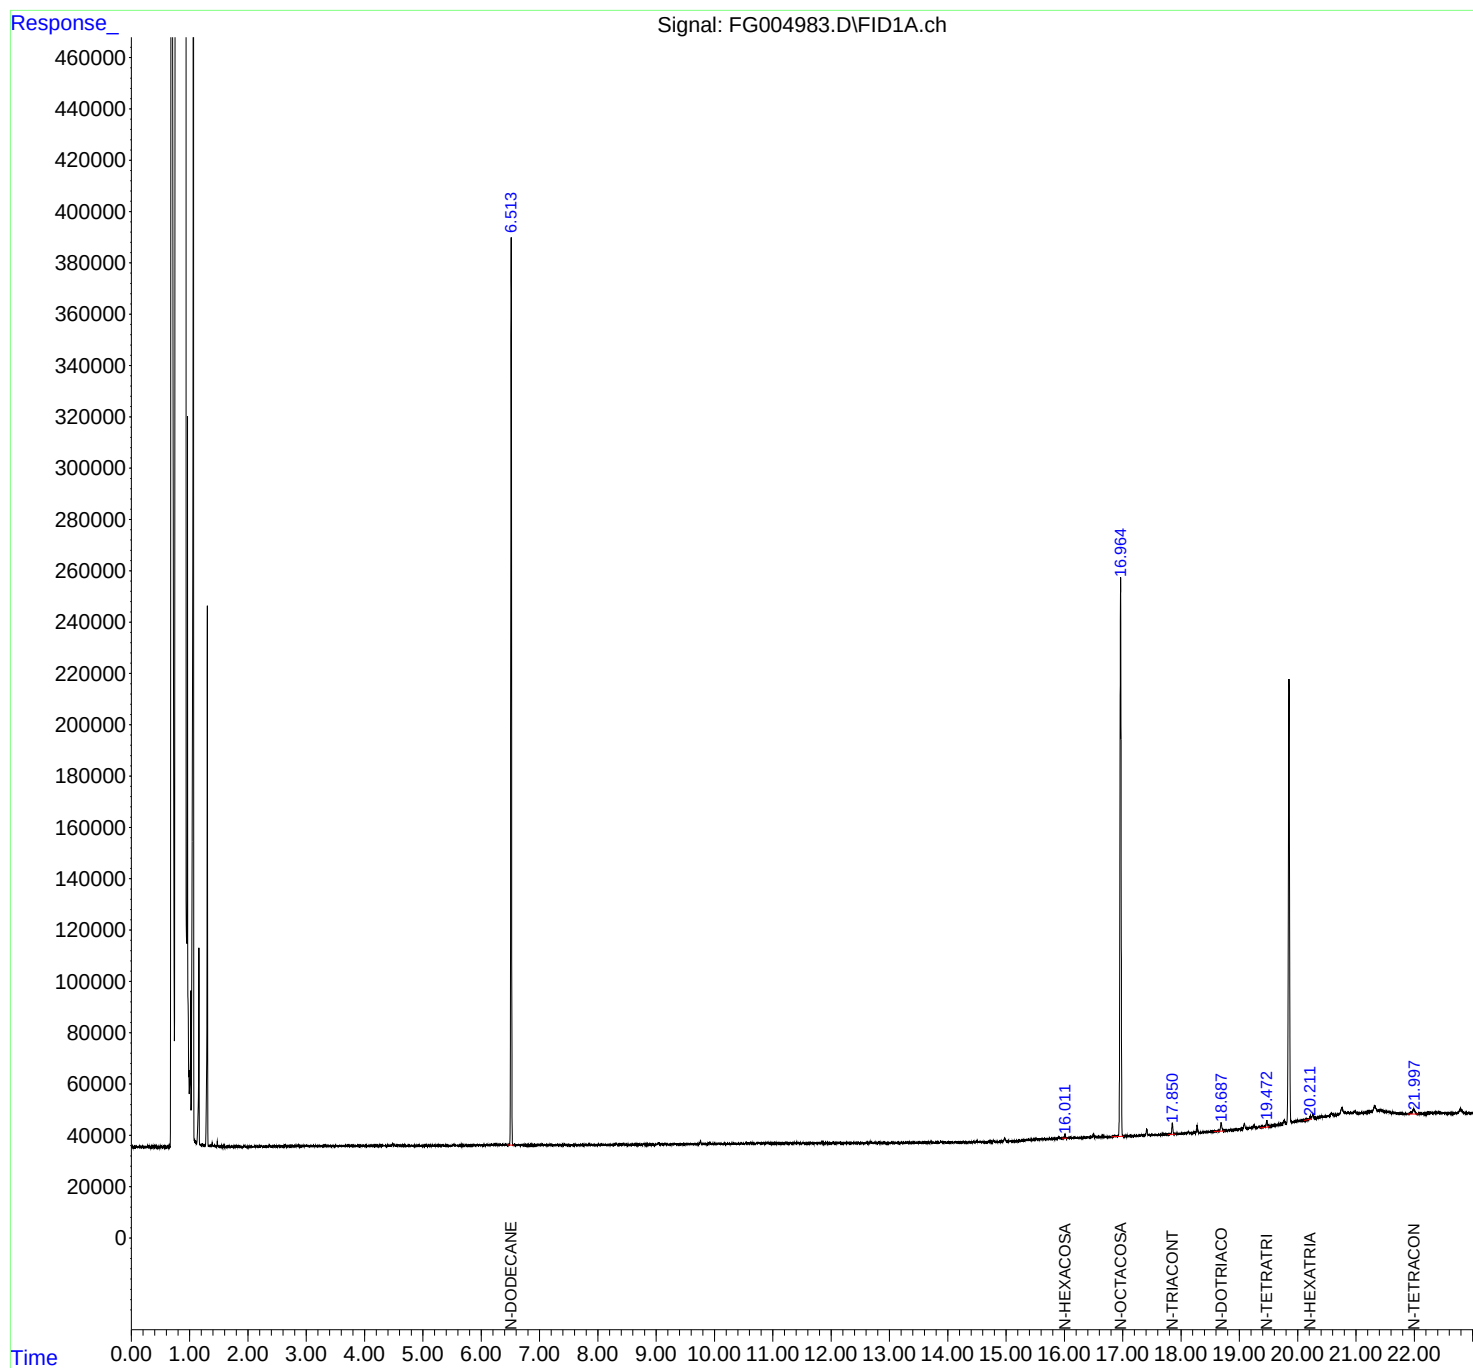

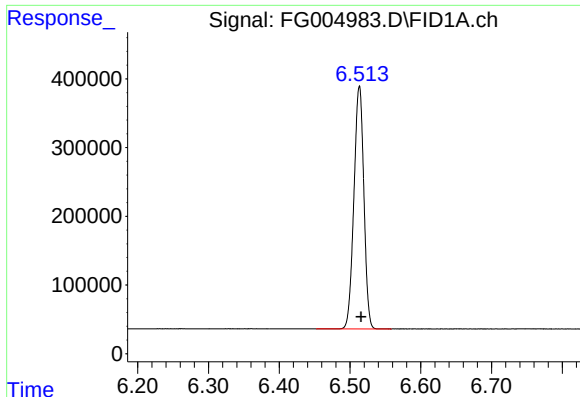


#3 N-DODECANE

R.T.: 6.513 min
Delta R.T.: -0.002 min
Response: 3450376
Conc: 24.05 ug/ml

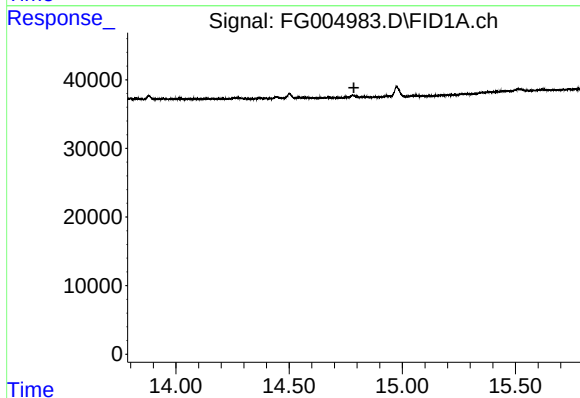


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

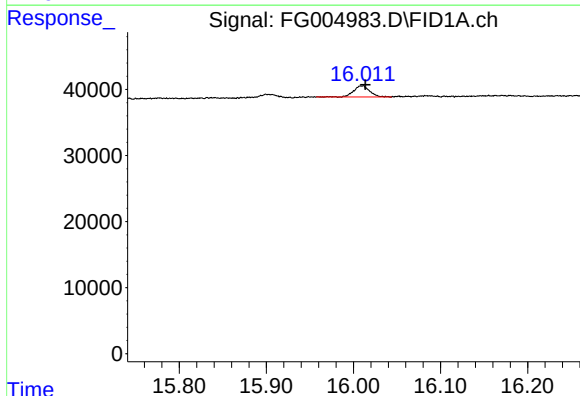


#11 N-HEXACOSANE

R.T.: 16.010 min
Delta R.T.: -0.004 min
Response: 21712
Conc: 0.17 ug/ml

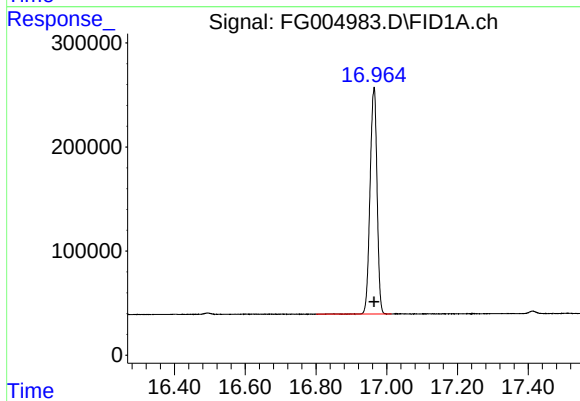


#12 N-OCTACOSANE

R.T.: 16.964 min
Delta R.T.: 0.000 min
Response: 2975924
Conc: 23.41 ug/ml

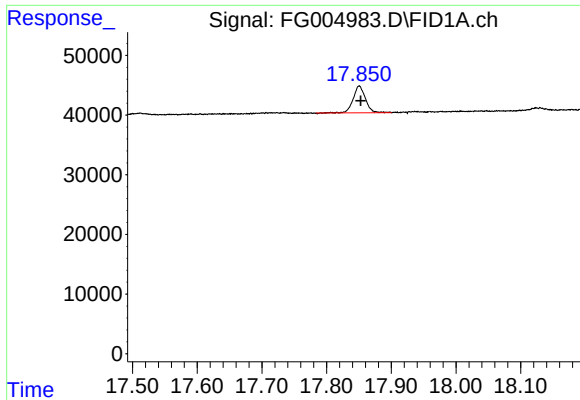


#13 N-TRIACONTANE

R.T.: 17.850 min
Delta R.T.: -0.002 min
Response: 59298
Conc: 0.47 ug/ml

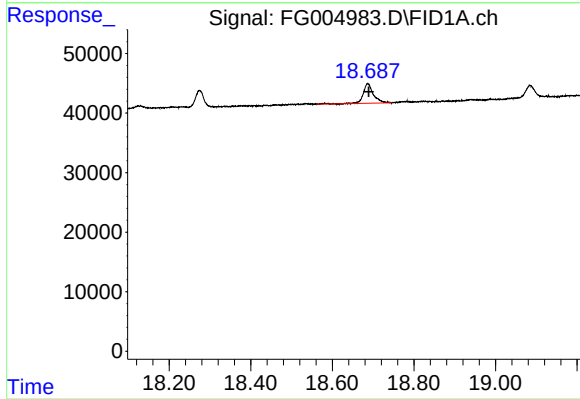


#14 N-DOTRIACONTANE

R.T.: 18.687 min
Delta R.T.: -0.002 min
Response: 57021
Conc: 0.48 ug/ml

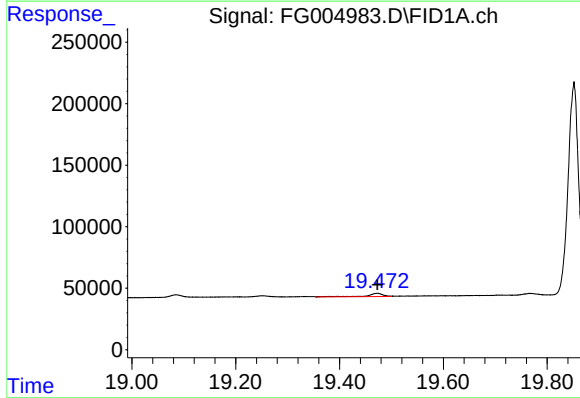


#15 N-TETRATRIACONTANE

R.T.: 19.473 min
Delta R.T.: 0.000 min
Response: 56674
Conc: 0.50 ug/ml

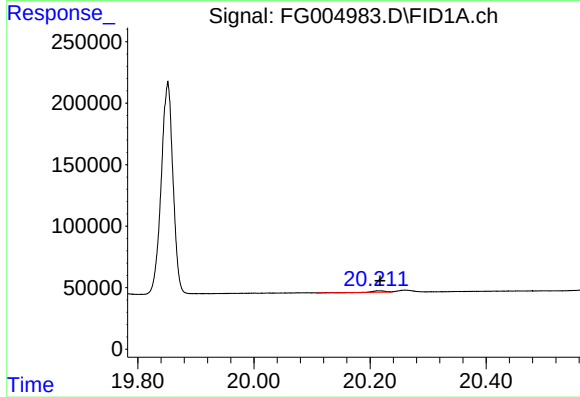

#16 N-HEXATRIACONTANE

R.T.: 20.214 min
Delta R.T.: -0.003 min
Response: 16831
Conc: 0.16 ug/ml

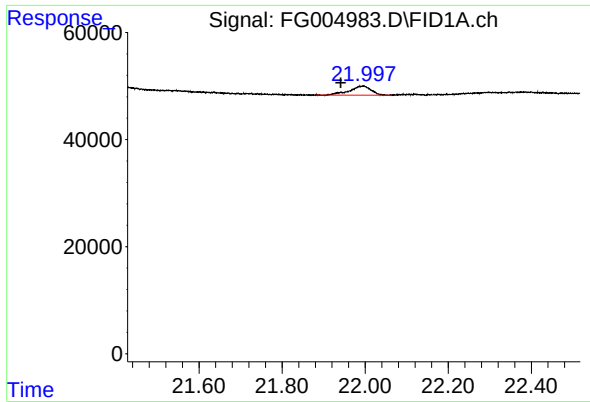

#18 N-TETRACONTANE

R.T.: 21.996 min
Delta R.T.: 0.056 min
Response: 61886
Conc: 0.64 ug/ml