

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052019\
 Data File : FG004984.D
 Signal(s) : FID1A.ch
 Acq On : 20 May 2019 11:27
 Operator : AJ\SJ
 Sample : PB119860BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 21 01:07:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.782	1985237	16.543 ug/ml
Target Compounds				
2)	N-DECANE	4.482	2443679	17.289 ug/ml
3)	N-DODECANE	6.512	2512586	17.513 ug/ml
4)	N-TETRADECANE	8.314	2509707	17.489 ug/ml
5)	N-HEXADECANE	9.920	2534312	17.545 ug/ml
6)	N-OCTADECANE	11.366	2535666	17.785 ug/ml
7)	N-EICOSANE	12.680	2531378	17.861 ug/ml
8)	N-DOCOSANE	13.881	2483145	17.918 ug/ml
10)	N-TETRACOSANE	14.986	2450095	18.085 ug/ml
11)	N-HEXACOSANE	16.009	2355896	17.941 ug/ml
12)	N-OCTACOSANE	16.959	2293501	18.042 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052019\
Data File : FG004984.D
Signal(s) : FID1A.ch
Acq On : 20 May 2019 11:27
Operator : AJ\SJ
Sample : PB119860BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 21 01:07:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

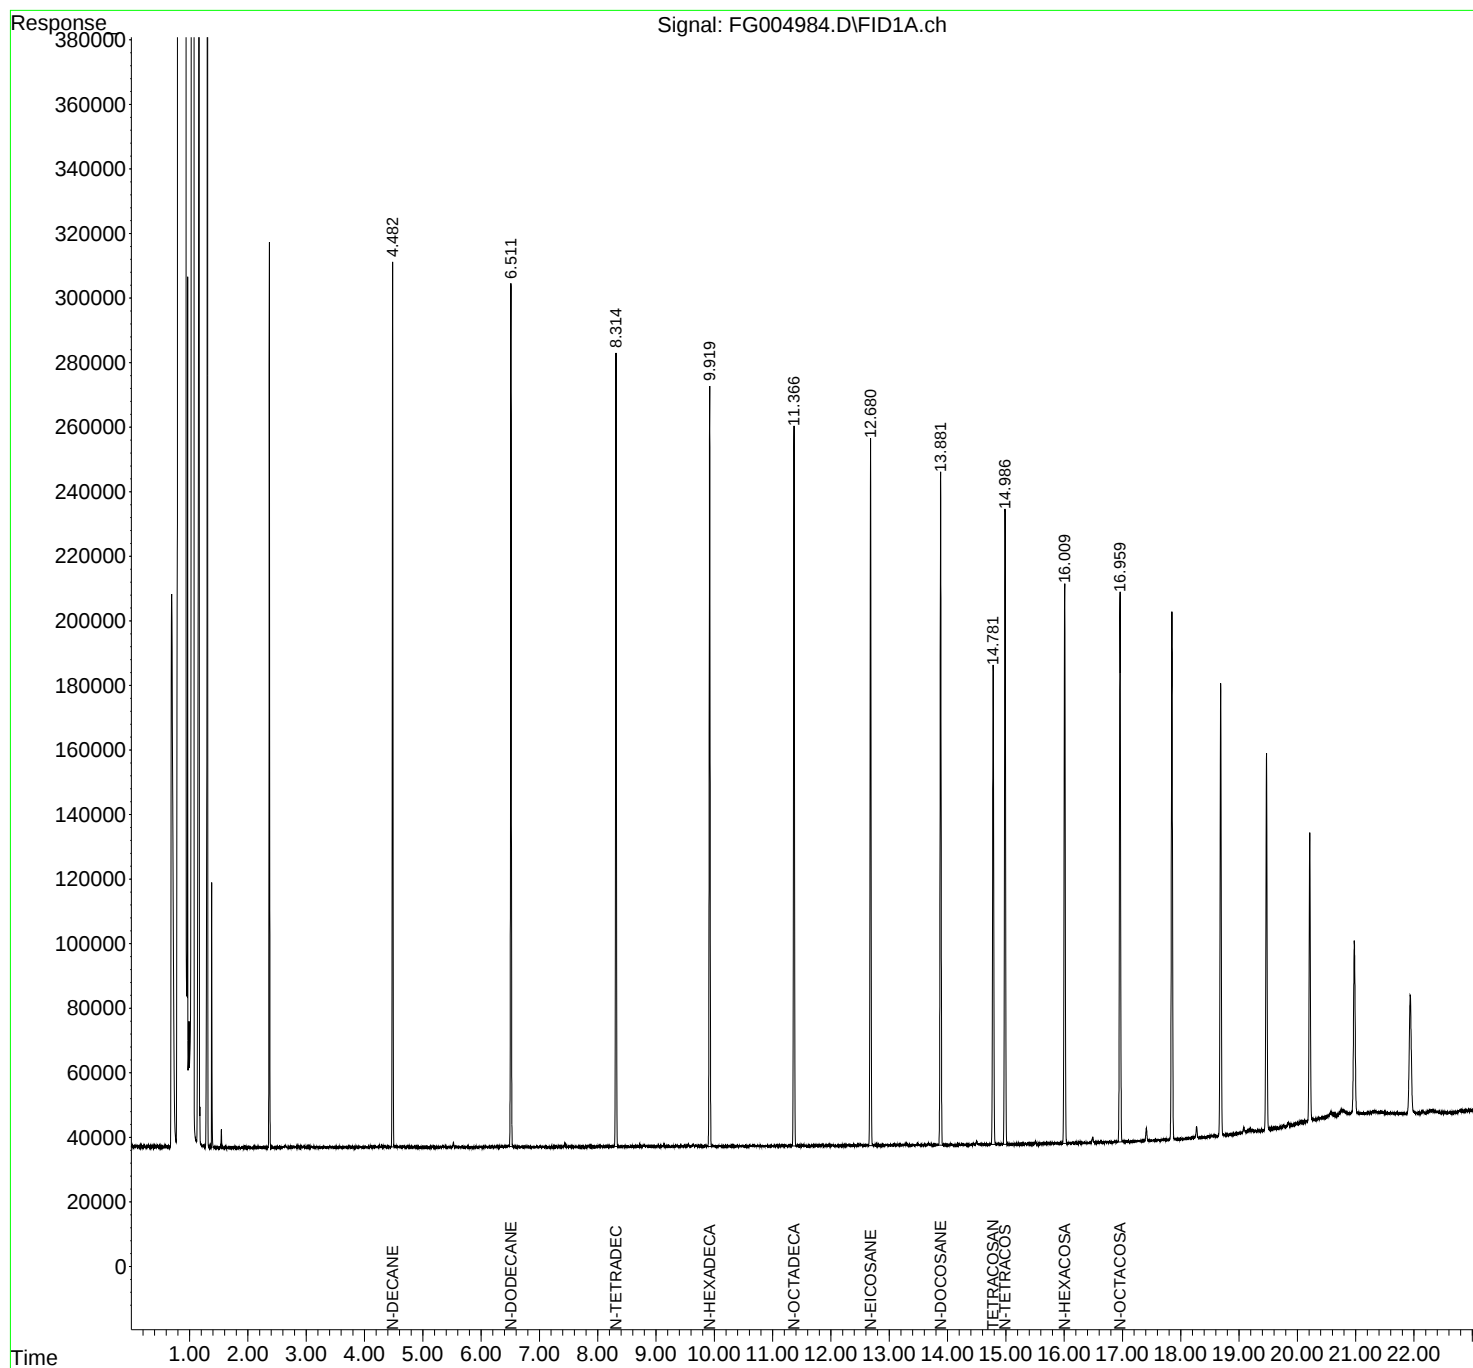

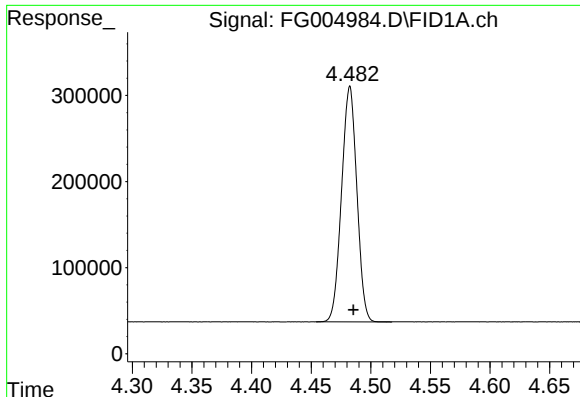


#2 N-DECANE

R.T.: 4.482 min
Delta R.T.: -0.003 min
Response: 2443679
Conc: 17.29 ug/ml

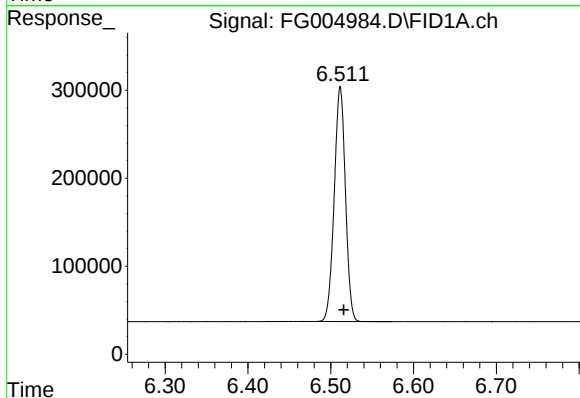


#3 N-DODECANE

R.T.: 6.512 min
Delta R.T.: -0.004 min
Response: 2512586
Conc: 17.51 ug/ml

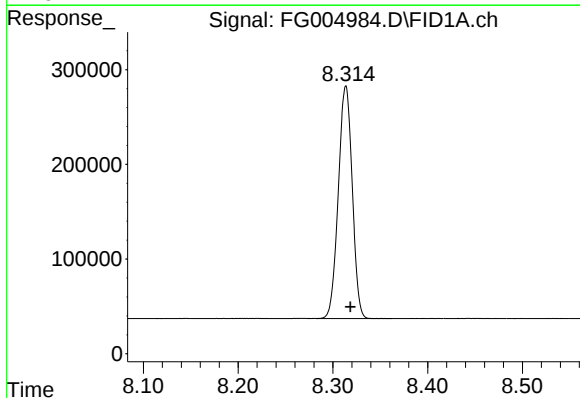


#4 N-TETRADECANE

R.T.: 8.314 min
Delta R.T.: -0.005 min
Response: 2509707
Conc: 17.49 ug/ml

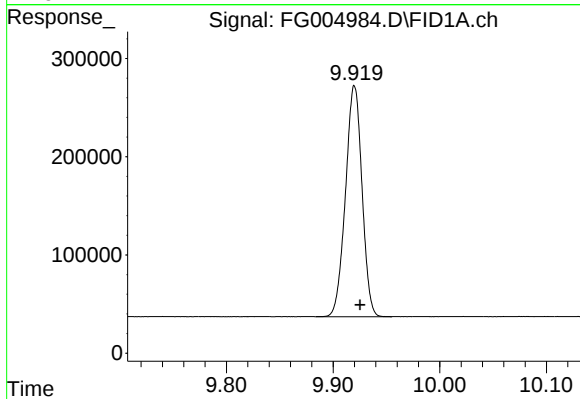


#5 N-HEXADECANE

R.T.: 9.920 min
Delta R.T.: -0.005 min
Response: 2534312
Conc: 17.54 ug/ml

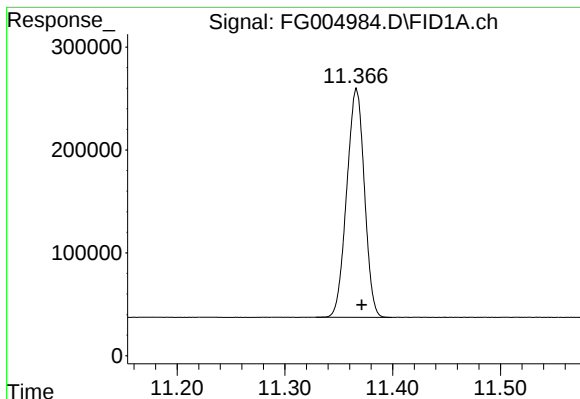


#6 N-OCTADECANE

R.T.: 11.366 min
Delta R.T.: -0.005 min
Response: 2535666
Conc: 17.78 ug/ml

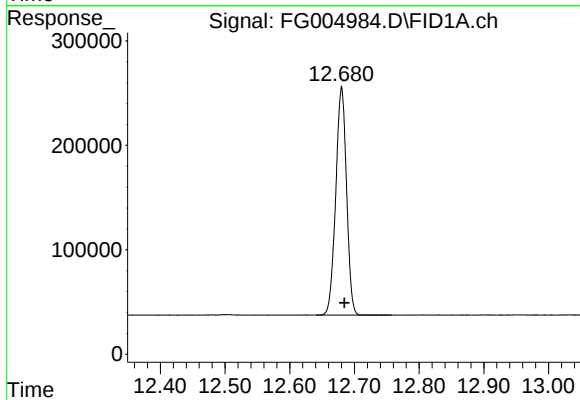


#7 N-EICOSANE

R.T.: 12.680 min
Delta R.T.: -0.004 min
Response: 2531378
Conc: 17.86 ug/ml

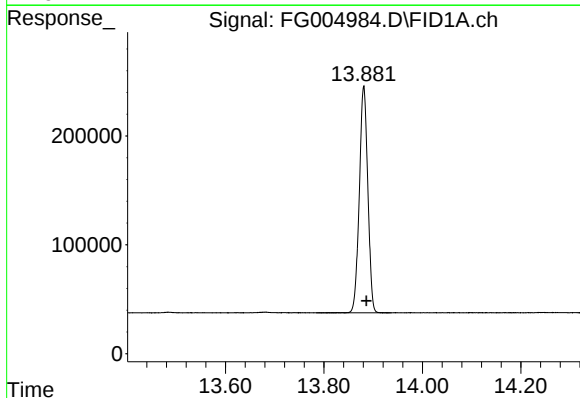


#8 N-DOCOSANE

R.T.: 13.881 min
Delta R.T.: -0.005 min
Response: 2483145
Conc: 17.92 ug/ml

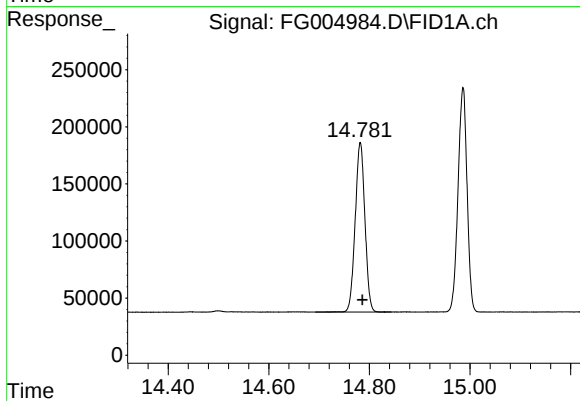


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.782 min
Delta R.T.: -0.004 min
Response: 1985237
Conc: 16.54 ug/ml

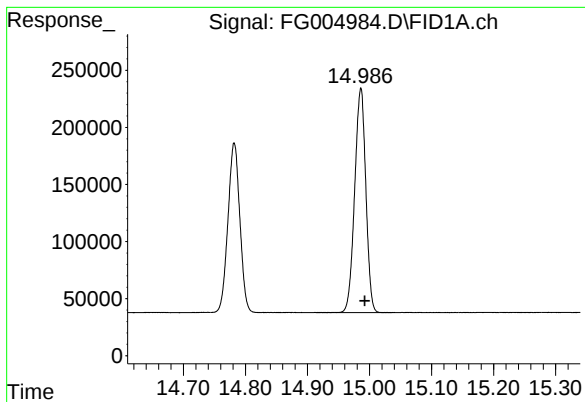


#10 N-TETRACOSANE

R.T.: 14.986 min
Delta R.T.: -0.006 min
Response: 2450095
Conc: 18.09 ug/ml

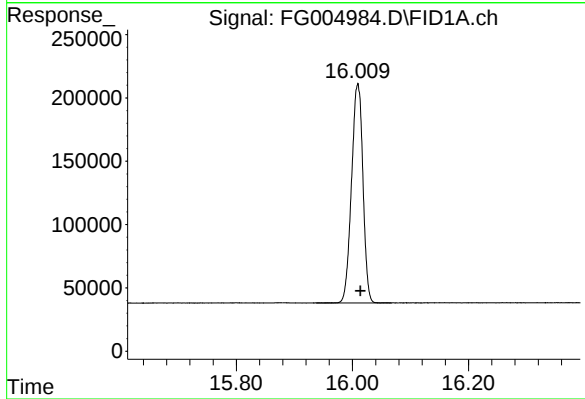

#11 N-HEXACOSANE

R.T.: 16.009 min
Delta R.T.: -0.004 min
Response: 2355896
Conc: 17.94 ug/ml

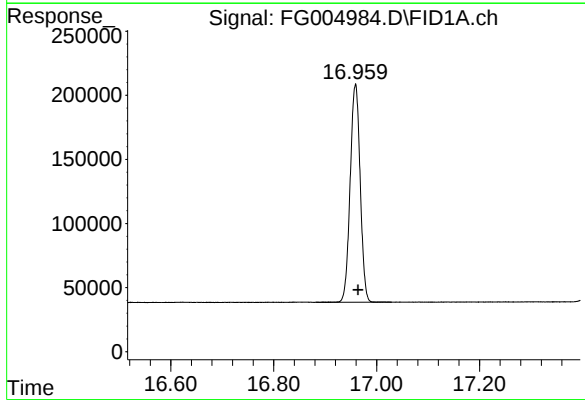

#12 N-OCTACOSANE

R.T.: 16.959 min
Delta R.T.: -0.005 min
Response: 2293501
Conc: 18.04 ug/ml