

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052019\
 Data File : FG004988.D
 Signal(s) : FID1A.ch
 Acq On : 20 May 2019 13:30
 Operator : AJ\SJ
 Sample : K2648-01MSD 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 21 01:08:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	403682	3.364 ug/mlm
Target Compounds			
2) N-DECANE	4.482	207544	1.468 ug/ml
3) N-DODECANE	6.511	308869	2.153 ug/ml
4) N-TETRADECANE	8.313	369924	2.578 ug/ml
5) N-HEXADECANE	9.919	415546	2.877 ug/ml
6) N-OCTADECANE	11.365	410526	2.879 ug/ml
7) N-EICOSANE	12.679	472119	3.331 ug/ml
8) N-DOCOSANE	13.881	418345	3.019 ug/ml
10) N-TETRACOSANE	14.974	1024614	7.563 ug/ml
11) N-HEXACOSANE	16.010	389898	2.969 ug/ml
12) N-OCTACOSANE	16.961	437671	3.443 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052019\
Data File : FG004988.D
Signal(s) : FID1A.ch
Acq On : 20 May 2019 13:30
Operator : AJ\SJ
Sample : K2648-01MSD 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 21 01:08:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

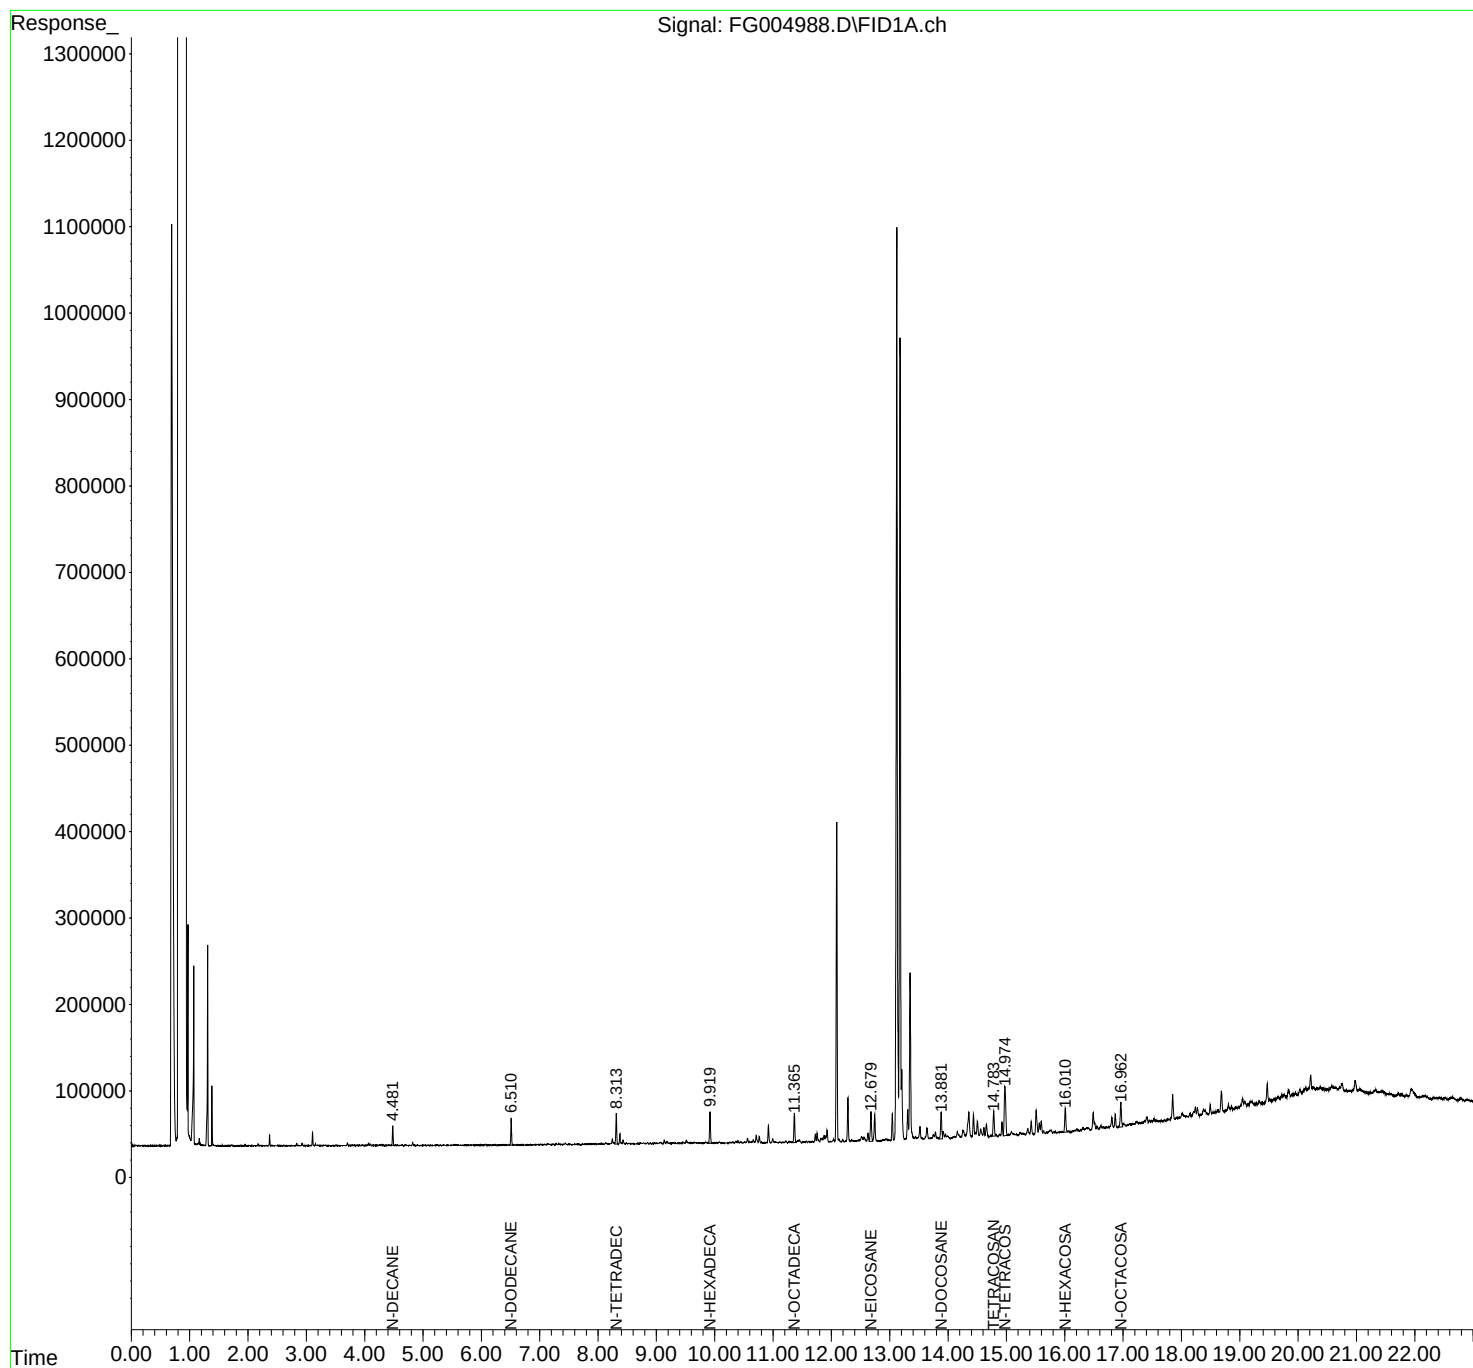

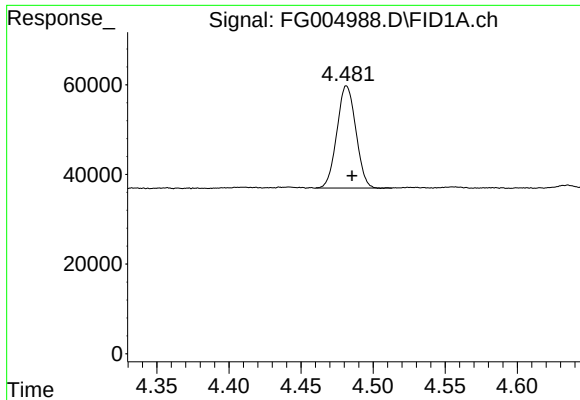


#2 N-DECANE

R.T.: 4.482 min
Delta R.T.: -0.004 min
Response: 207544
Conc: 1.47 ug/ml

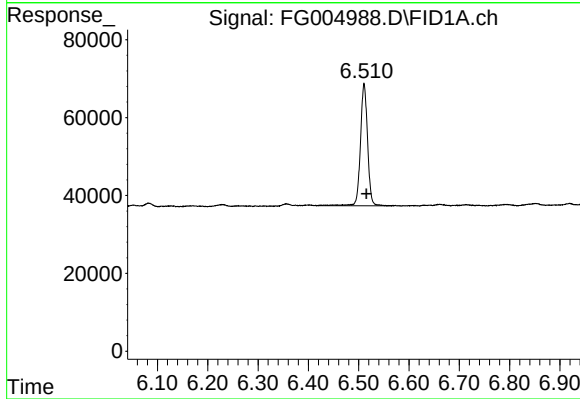


#3 N-DODECANE

R.T.: 6.511 min
Delta R.T.: -0.005 min
Response: 308869
Conc: 2.15 ug/ml

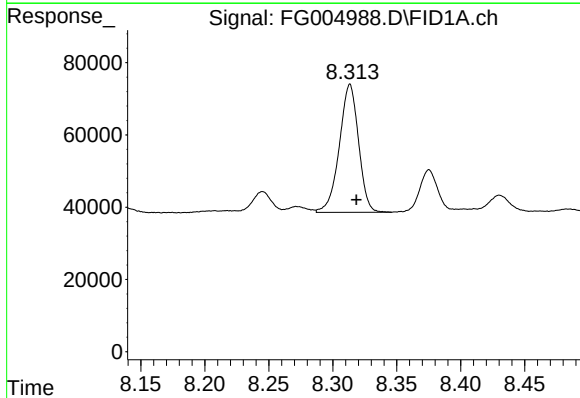


#4 N-TETRADECANE

R.T.: 8.313 min
Delta R.T.: -0.005 min
Response: 369924
Conc: 2.58 ug/ml

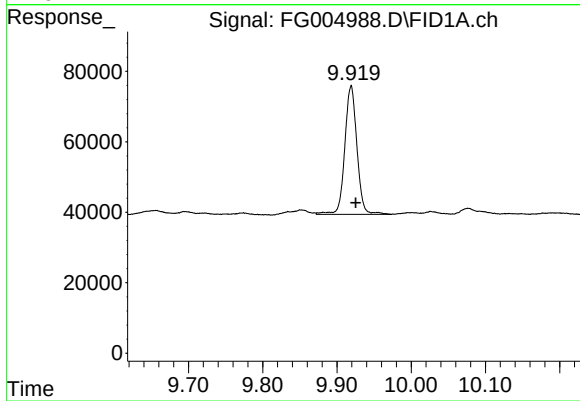


#5 N-HEXADECANE

R.T.: 9.919 min
Delta R.T.: -0.006 min
Response: 415546
Conc: 2.88 ug/ml

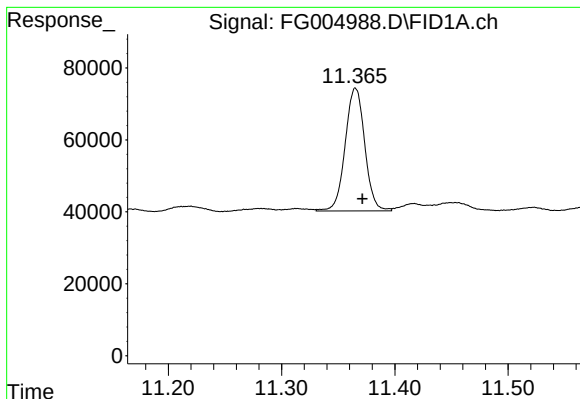


#6 N-OCTADECANE

R.T.: 11.365 min
Delta R.T.: -0.006 min
Response: 410526
Conc: 2.88 ug/ml

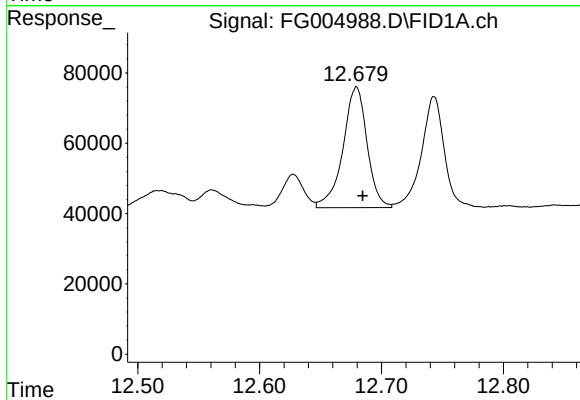


#7 N-EICOSANE

R.T.: 12.679 min
Delta R.T.: -0.005 min
Response: 472119
Conc: 3.33 ug/ml

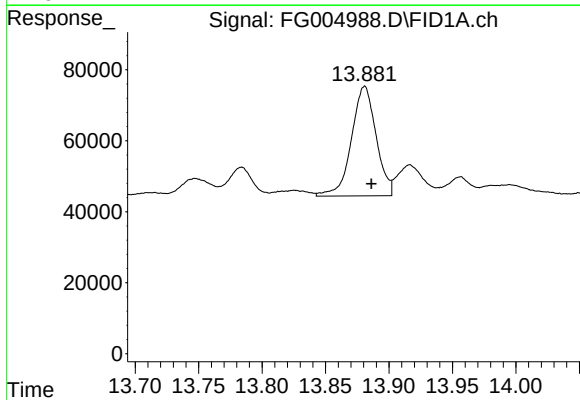


#8 N-DOCOSANE

R.T.: 13.881 min
Delta R.T.: -0.005 min
Response: 418345
Conc: 3.02 ug/ml

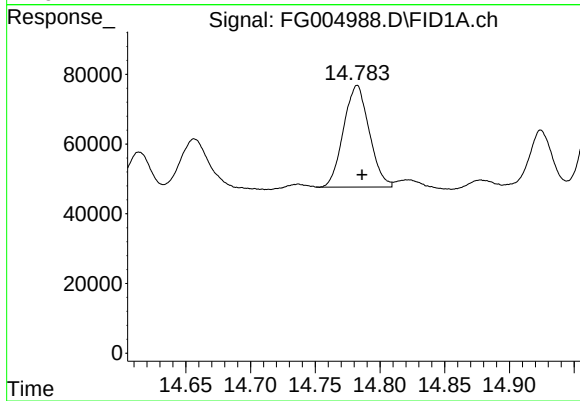


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.004 min
Response: 403682
Conc: 3.36 ug/ml m

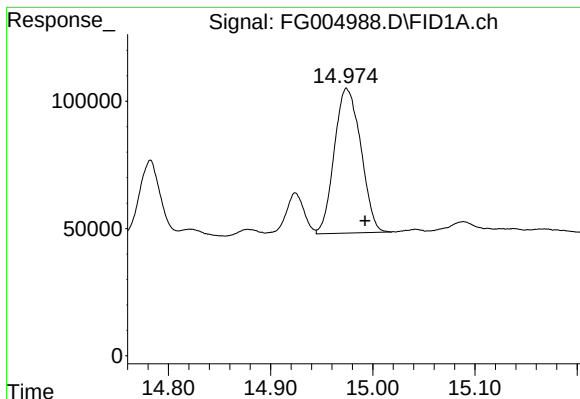


#10 N-TETRACOSANE

R.T.: 14.974 min
Delta R.T.: -0.018 min
Response: 1024614
Conc: 7.56 ug/ml

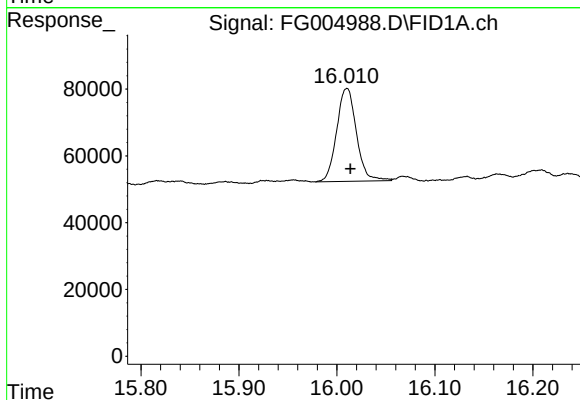

#11 N-HEXACOSANE

R.T.: 16.010 min
Delta R.T.: -0.003 min
Response: 389898
Conc: 2.97 ug/ml

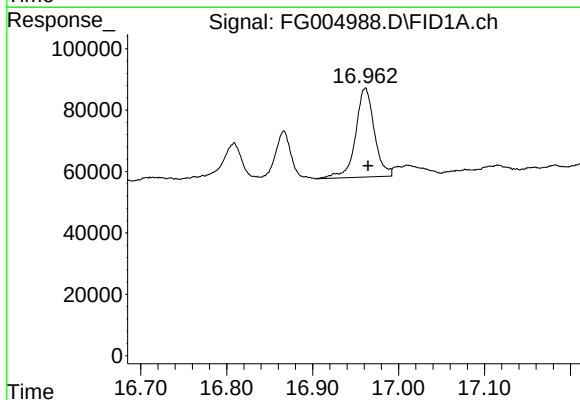

#12 N-OCTACOSANE

R.T.: 16.961 min
Delta R.T.: -0.003 min
Response: 437671
Conc: 3.44 ug/ml