

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052319\
Data File : FG005000.D
Signal(s) : FID1A.ch
Acq On : 23 May 2019 10:14
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 24 01:19:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.970	72186	0.533 ug/ml
13)	N-TRIACONTANE	17.844	33620	0.268 ug/ml
14)	N-DOTRIACONTANE	18.679	45144	0.377 ug/ml
15)	N-TETRATRIACONTANE	19.464	39324	0.349 ug/ml
16)	N-HEXATRIACONTANE	20.210	20719	0.195 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052319\
Data File : FG005000.D
Signal(s) : FID1A.ch
Acq On : 23 May 2019 10:14
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 24 01:19:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

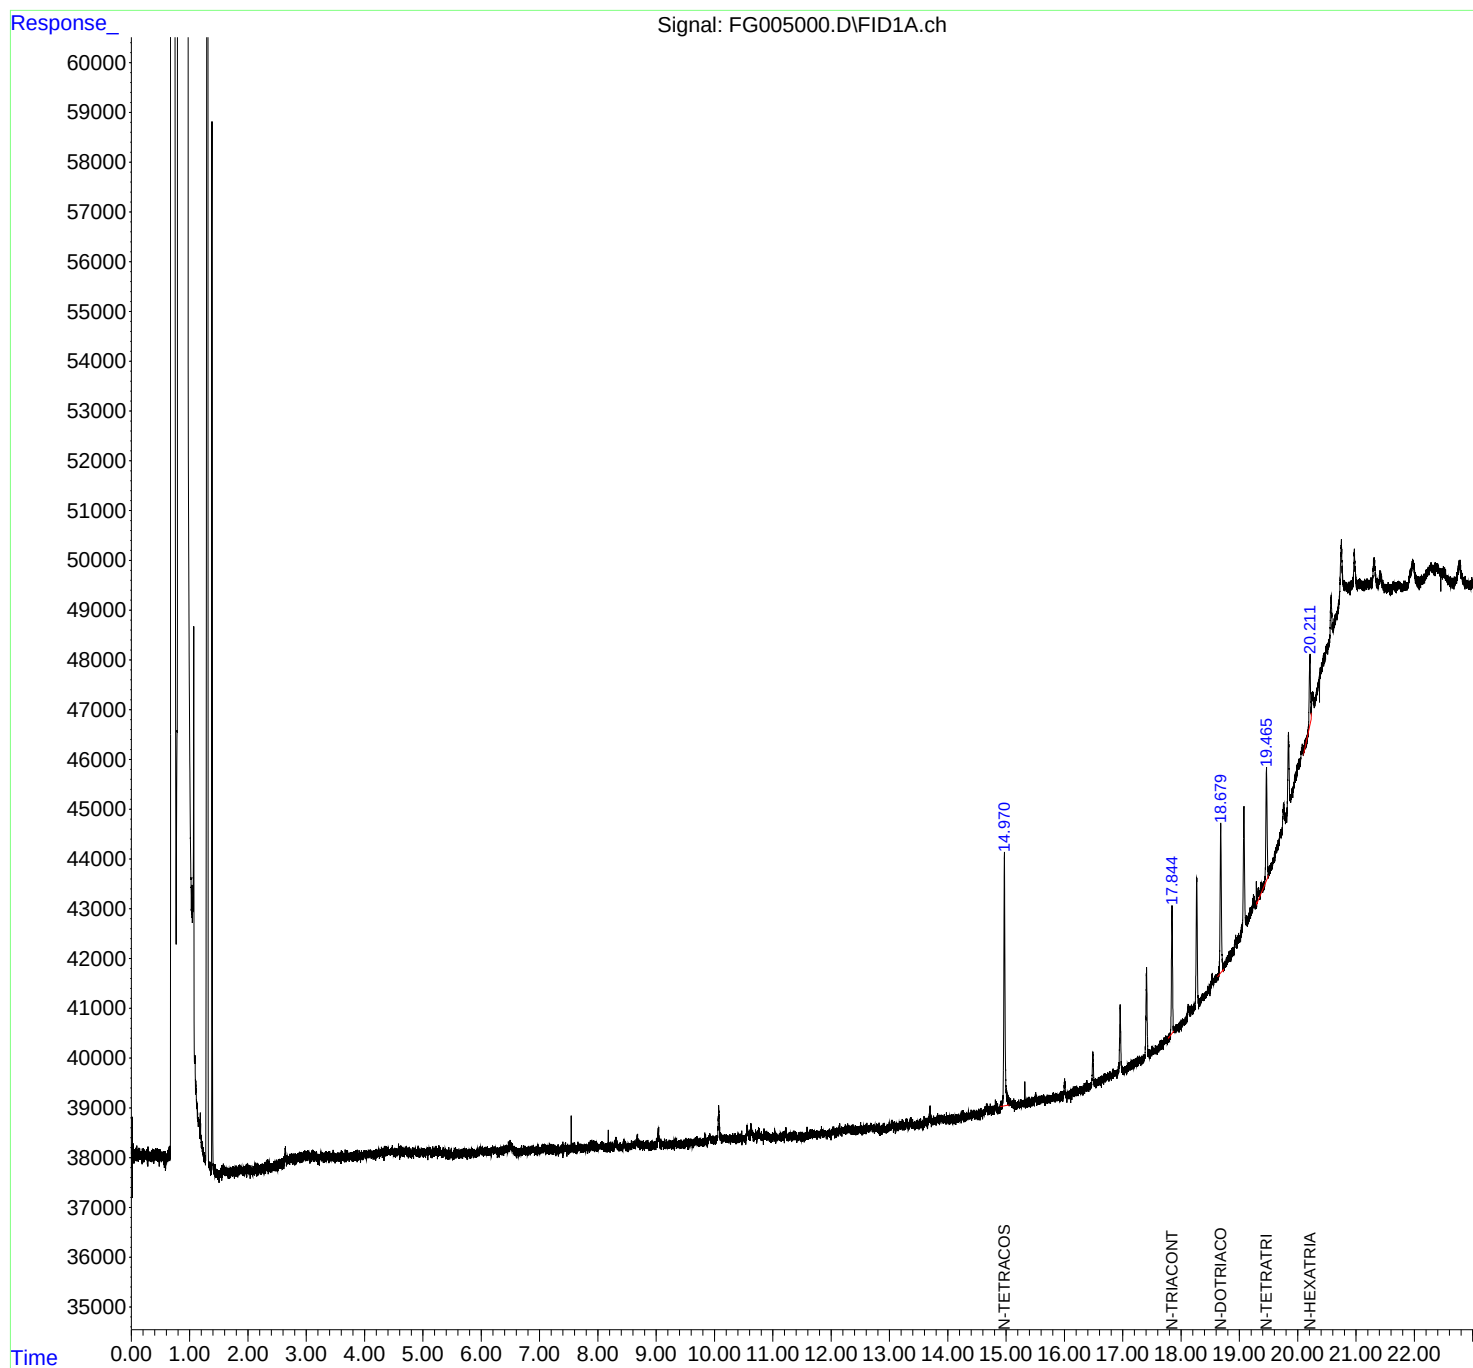

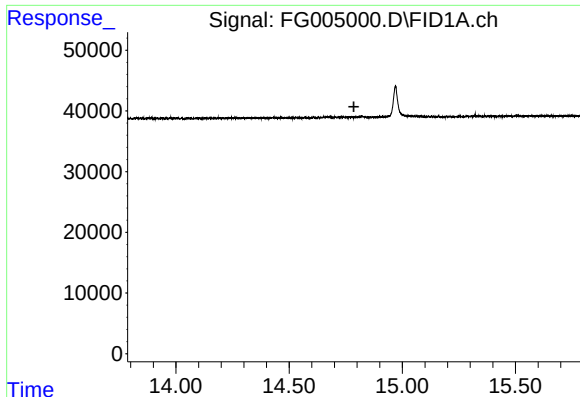


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.786 min
Response: 0
Conc: N.D.

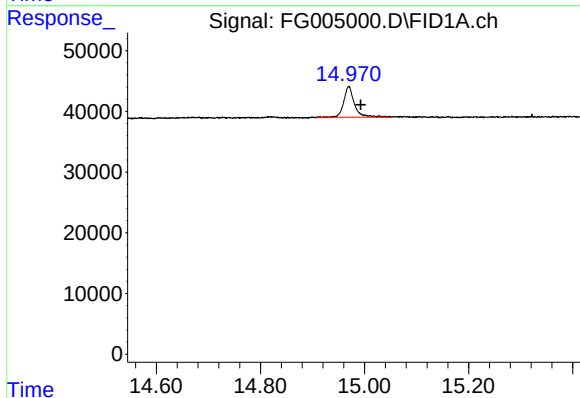


#10 N-TETRACOSANE

R.T.: 14.970 min
Delta R.T.: -0.022 min
Response: 72186
Conc: 0.53 ug/ml

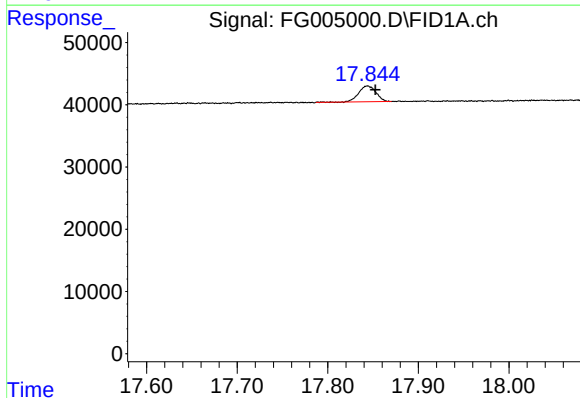


#13 N-TRIACONTANE

R.T.: 17.844 min
Delta R.T.: -0.009 min
Response: 33620
Conc: 0.27 ug/ml

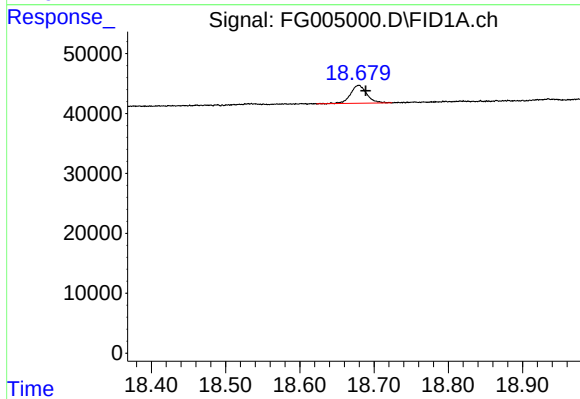


#14 N-DOTRIACONTANE

R.T.: 18.679 min
Delta R.T.: -0.009 min
Response: 45144
Conc: 0.38 ug/ml

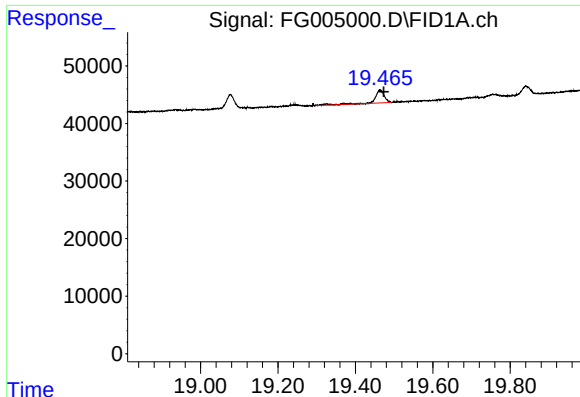

#15 N-TETRATRIACONTANE

R.T.: 19.464 min
Delta R.T.: -0.009 min
Response: 39324
Conc: 0.35 ug/ml

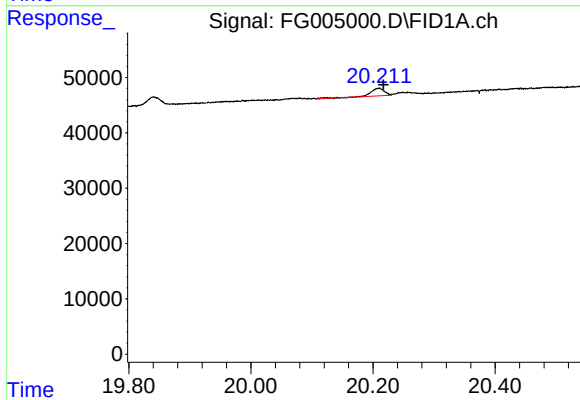

#16 N-HEXATRIACONTANE

R.T.: 20.210 min
Delta R.T.: -0.007 min
Response: 20719
Conc: 0.20 ug/ml