

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052423\
Data File : FG012008.D
Signal(s) : FID1A.ch
Acq On : 25 May 2023 00:56
Operator : YP\AJ
Sample : 02899-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 25 05:34:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050523.M
Quant Title :
QLast Update : Fri May 05 17:29:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.013	1365047	10.078 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.912	694563	5.068 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG052423\
Data File : FG012008.D
Signal(s) : FID1A.ch
Acq On : 25 May 2023 00:56
Operator : YP\AJ
Sample : 02899-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 25 05:34:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050523.M
Quant Title :
QLast Update : Fri May 05 17:29:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

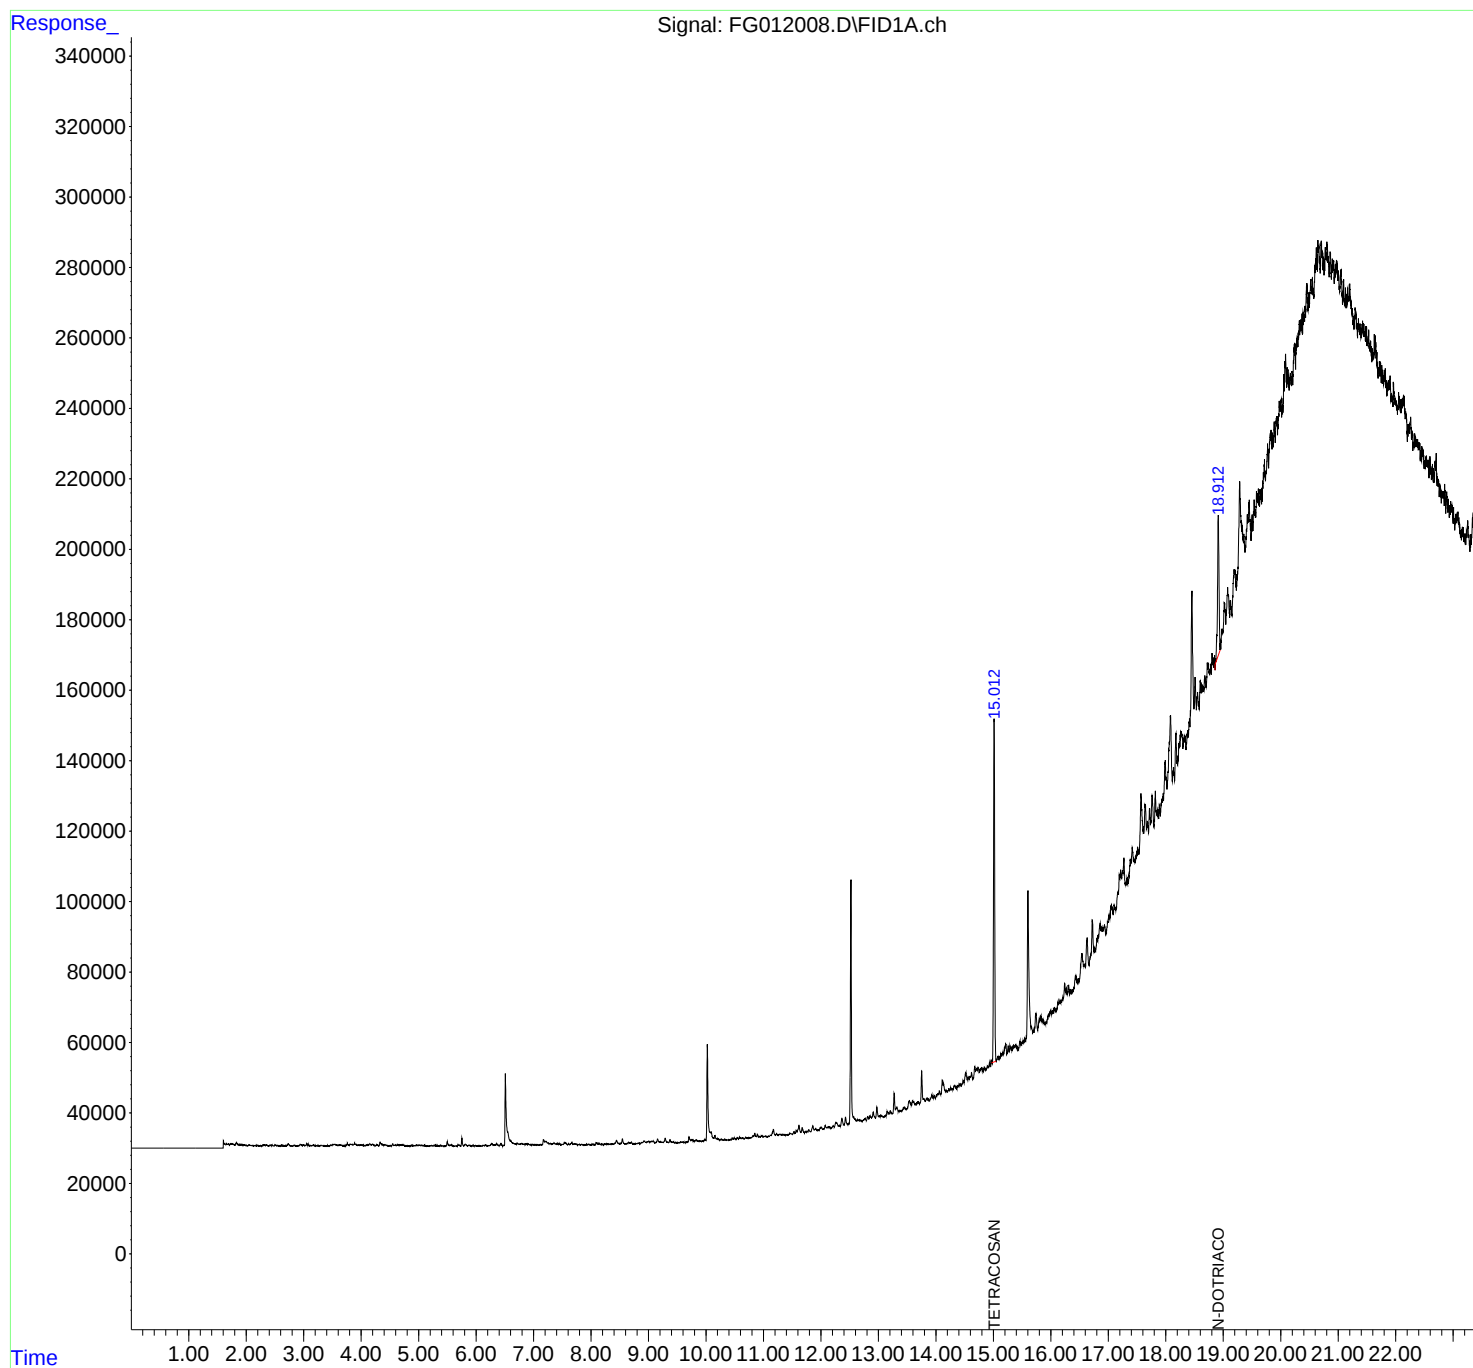


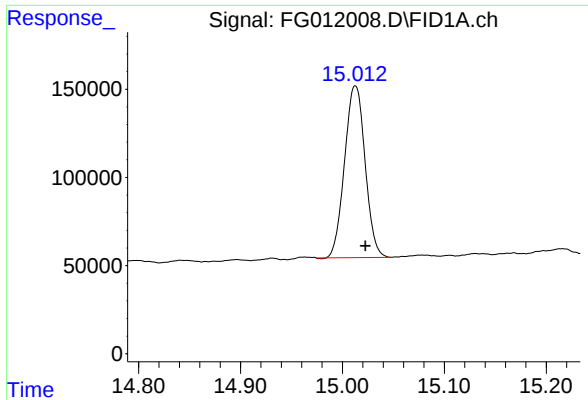

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.013 min
Delta R.T.: -0.010 min
Response: 1365047
Conc: 10.08 ug/ml

Instrument :
FID_G
ClientSampleId :

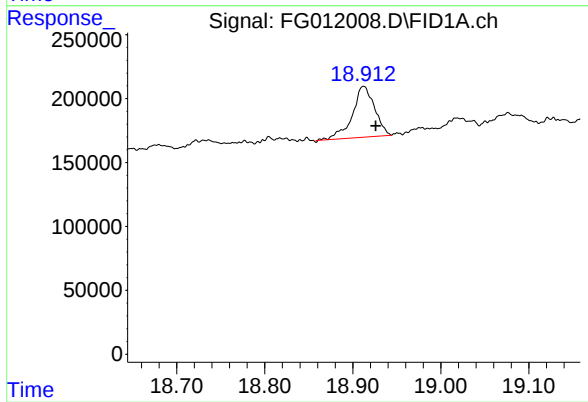

#14 N-DOTRIACONTANE

R.T.: 18.912 min
Delta R.T.: -0.014 min
Response: 694563
Conc: 5.07 ug/ml