

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG053119\
Data File : FG005061.D
Signal(s) : FID1A.ch
Acq On : 31 May 2019 21:16
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 31 23:21:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.978	109948	0.812 ug/ml
12)	N-OCTACOSANE	16.963	31816	0.250 ug/ml
13)	N-TRIACONTANE	17.853	39864	0.317 ug/ml
14)	N-DOTRIACONTANE	18.688	54570	0.455 ug/ml
15)	N-TETRATRIACONTANE	19.473	109728	0.975 ug/ml
16)	N-HEXATRIACONTANE	20.243	136895	1.290 ug/ml
17)	N-OCTATRIACONTANE	20.981	134664	1.390 ug/ml
18)	N-TETRACONTANE	21.955	71962	0.739 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG053119\
Data File : FG005061.D
Signal(s) : FID1A.ch
Acq On : 31 May 2019 21:16
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 31 23:21:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

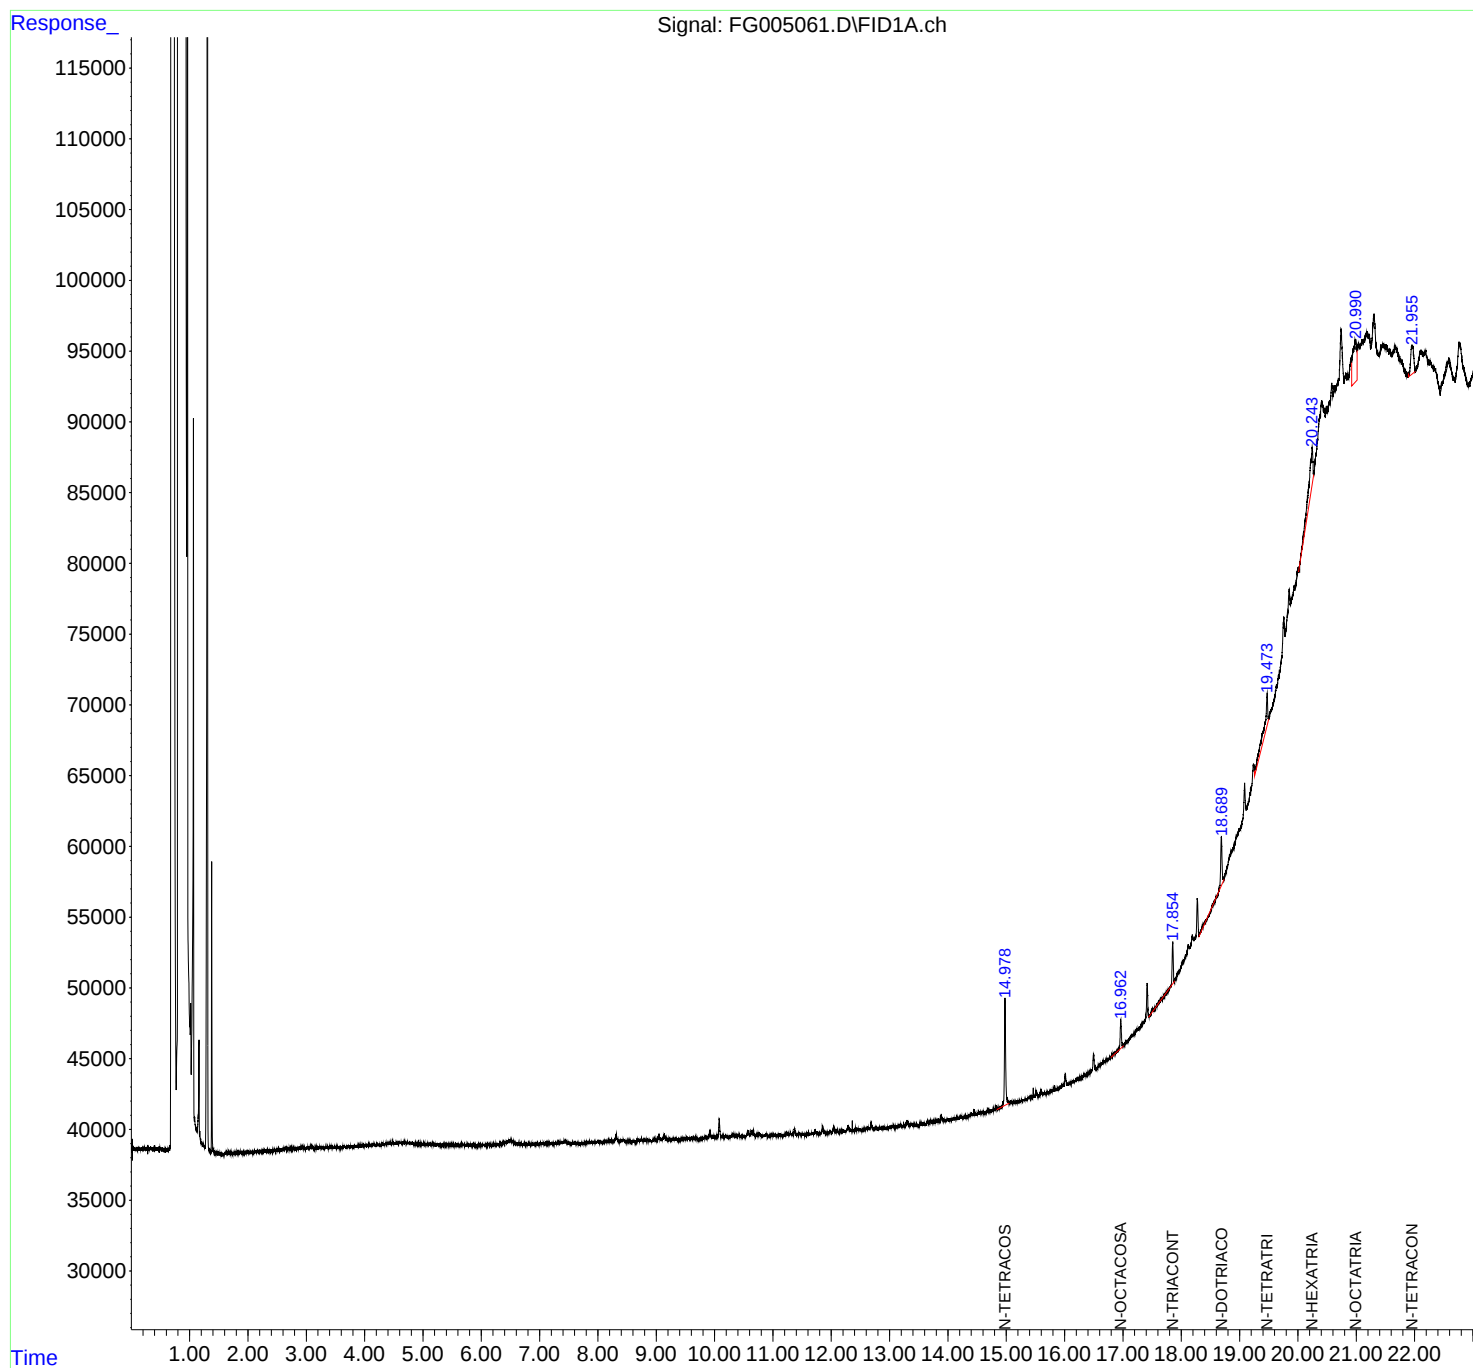

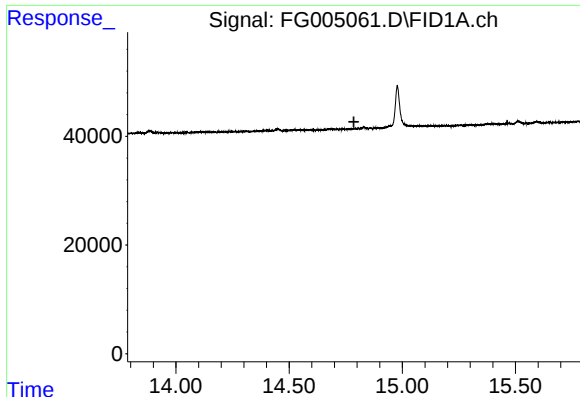


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.786 min
Response: 0
Conc: N.D.

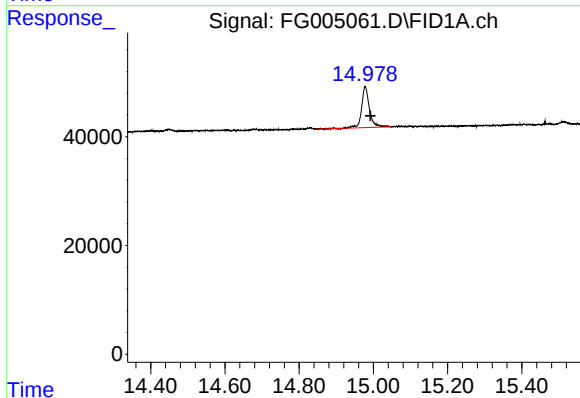


#10 N-TETRACOSANE

R.T.: 14.978 min
Delta R.T.: -0.014 min
Response: 109948
Conc: 0.81 ug/ml

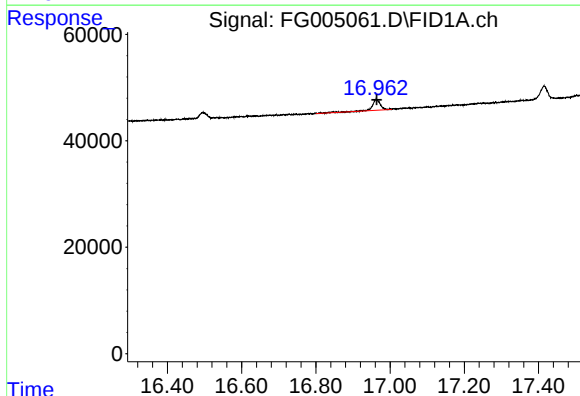


#12 N-OCTACOSANE

R.T.: 16.963 min
Delta R.T.: -0.002 min
Response: 31816
Conc: 0.25 ug/ml

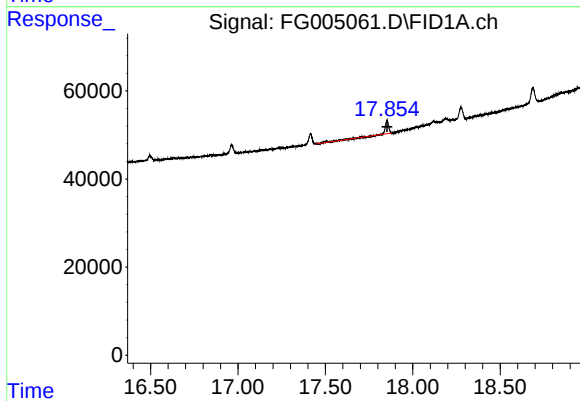


#13 N-TRIACONTANE

R.T.: 17.853 min
Delta R.T.: 0.000 min
Response: 39864
Conc: 0.32 ug/ml

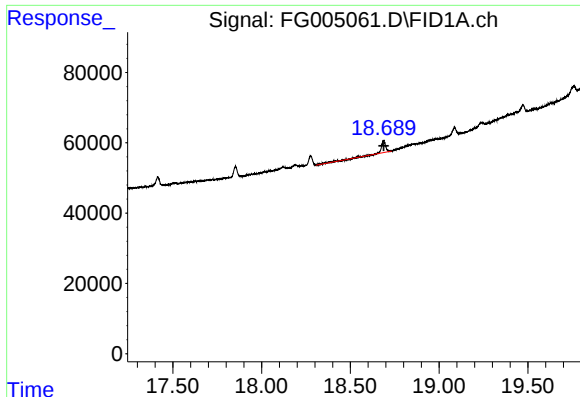


#14 N-DOTRIACONTANE

R.T.: 18.688 min
Delta R.T.: 0.000 min
Response: 54570
Conc: 0.46 ug/ml

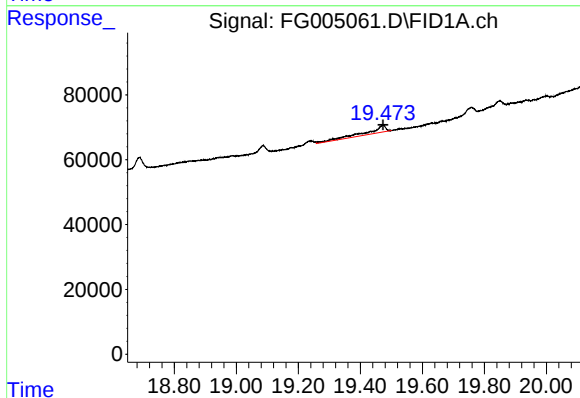


#15 N-TETRATRIACONTANE

R.T.: 19.473 min
Delta R.T.: 0.000 min
Response: 109728
Conc: 0.97 ug/ml

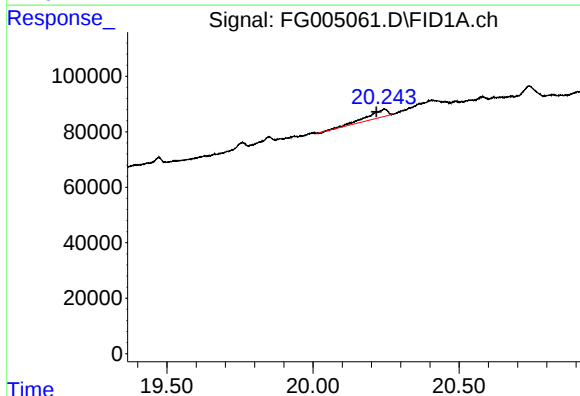


#16 N-HEXATRIACONTANE

R.T.: 20.243 min
Delta R.T.: 0.026 min
Response: 136895
Conc: 1.29 ug/ml

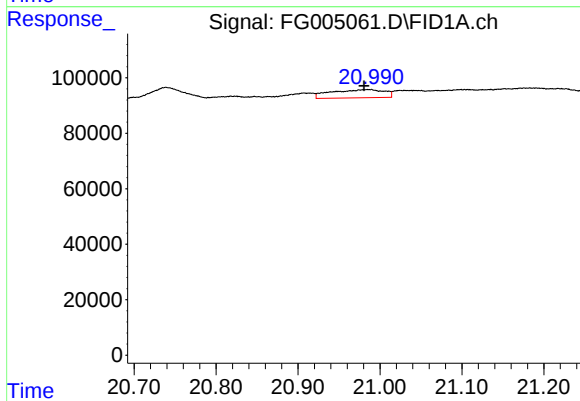

#17 N-OCTATRIACONTANE

R.T.: 20.981 min
Delta R.T.: 0.000 min
Response: 134664
Conc: 1.39 ug/ml

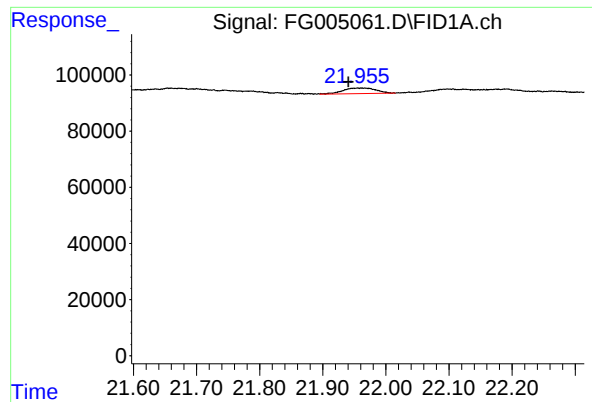

#18 N-TETRACONTANE

R.T.: 21.955 min
Delta R.T.: 0.015 min
Response: 71962
Conc: 0.74 ug/ml