

Data Path : P:\HPCHEM1\FID_G\Data\FG060118\
 Data File : FG001088.D
 Signal(s) : FID1A.ch
 Acq On : 01 Jun 2018 13:36
 Operator : UA\AJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 01 14:06:01 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 14:05:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.542	5874346	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.196	6516006	50.000 ug/ml
2) N-DECANE	4.284	6588944	50.000 ug/ml
3) N-DODECANE	6.300	6663141	50.000 ug/ml
4) N-TETRADECANE	8.093	6718815	50.000 ug/ml
5) N-HEXADECANE	9.692	6767509	50.000 ug/ml
6) N-OCTADECANE	11.133	6808063	50.000 ug/ml
7) N-EICOSANE	12.442	6761570	50.000 ug/ml
8) N-DOCOSANE	13.642	6725572	50.000 ug/ml
10) N-TETRACOSANE	14.746	6665203	50.000 ug/ml
11) N-HEXACOSANE	15.768	6634343	50.000 ug/ml
12) N-OCTACOSANE	16.719	6585860	50.000 ug/ml
13) N-TRIACONTANE	17.608	6535598	50.000 ug/ml
14) N-DOTRIACONTANE	18.443	6352661	50.000 ug/ml
15) N-TETRATRIACONTANE	19.230	6281973	50.000 ug/ml
16) N-HEXATRIACONTANE	19.972	6015493	50.000 ug/ml
17) N-OCTATRIACONTANE	20.695	5429592	50.000 ug/ml
18) N-TETRACONTANE	21.556	5349600	50.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG060118\
Data File : FG001088.D
Signal(s) : FID1A.ch
Acq On : 01 Jun 2018 13:36
Operator : UA\AJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 01 14:06:01 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 14:05:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

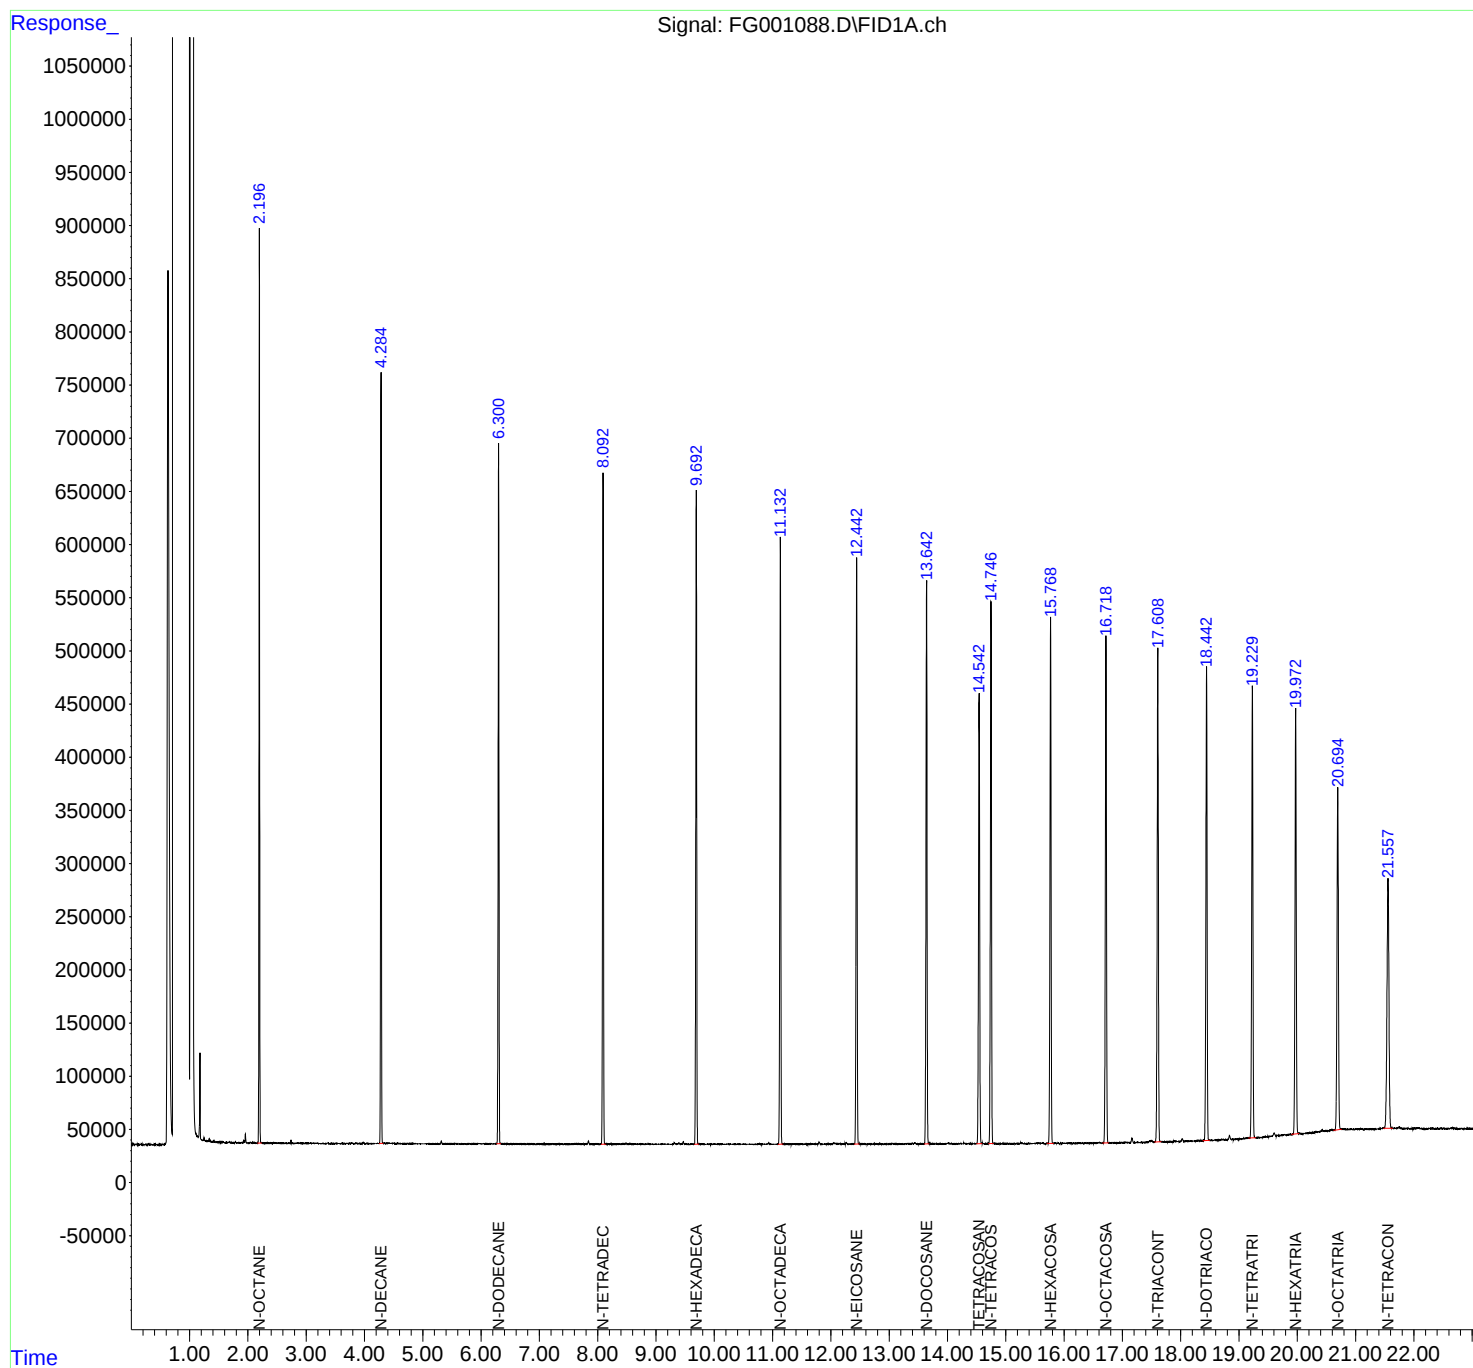


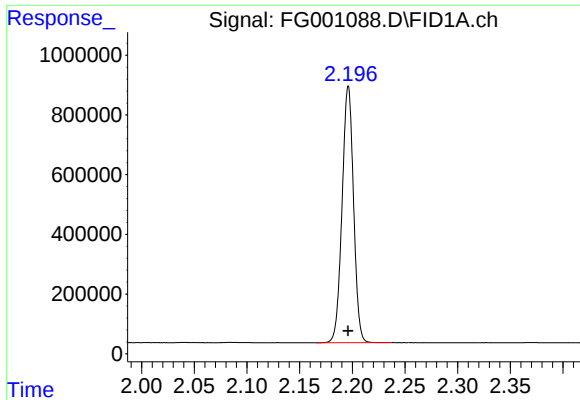

#1 N-OCTANE


R.T.: 2.196 min
Delta R.T.: 0.000 min
Response: 6516006
Conc: 50.00 ug/ml

Instrument :
FID_G
ClientSampleId :

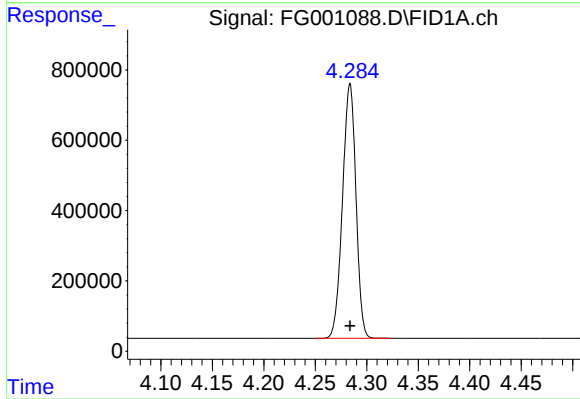


#2 N-DECANE

R.T.: 4.284 min
Delta R.T.: 0.000 min
Response: 6588944
Conc: 50.00 ug/ml

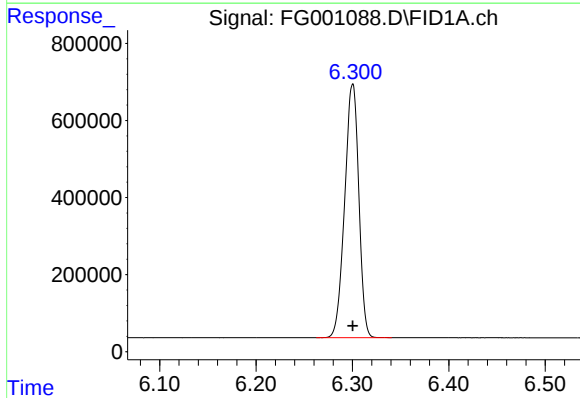


#3 N-DODECANE

R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 6663141
Conc: 50.00 ug/ml

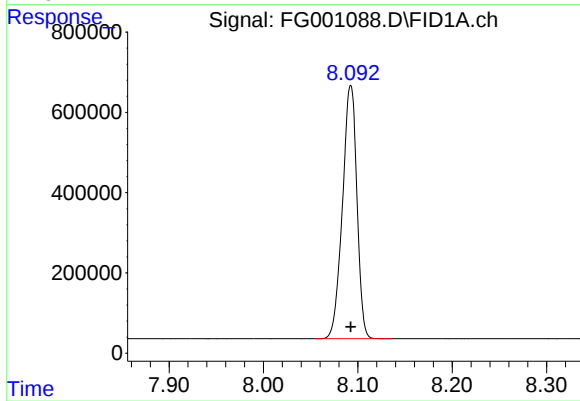

#4 N-TETRADECANE


R.T.: 8.093 min
Delta R.T.: 0.000 min
Response: 6718815
Conc: 50.00 ug/ml

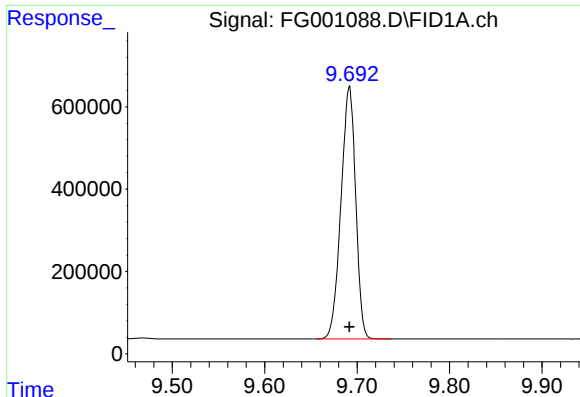

#5 N-HEXADECANE


R.T.: 9.692 min
Delta R.T.: 0.000 min
Response: 6767509
Conc: 50.00 ug/ml

Instrument :
FID_G
ClientSampleId :

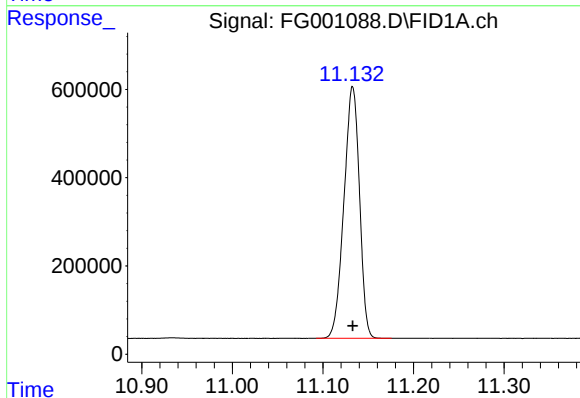


#6 N-OCTADECANE

R.T.: 11.133 min
Delta R.T.: 0.000 min
Response: 6808063
Conc: 50.00 ug/ml

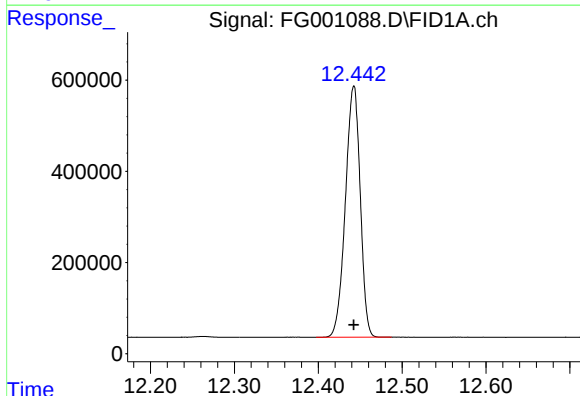


#7 N-EICOSANE

R.T.: 12.442 min
Delta R.T.: 0.000 min
Response: 6761570
Conc: 50.00 ug/ml

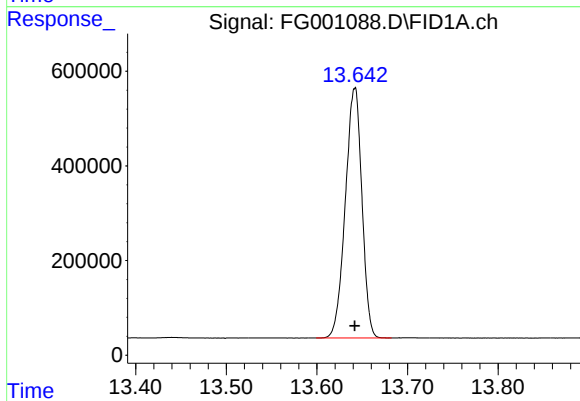

#8 N-DOCOSANE


R.T.: 13.642 min
Delta R.T.: 0.000 min
Response: 6725572
Conc: 50.00 ug/ml

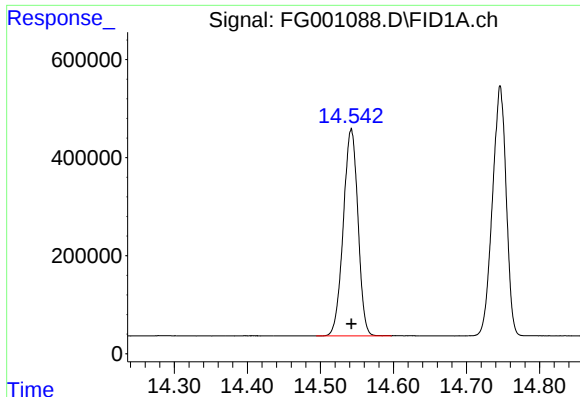

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.542 min
Delta R.T.: 0.000 min
Response: 5874346
Conc: 50.00 ug/ml

Instrument :
FID_G
ClientSampleId :

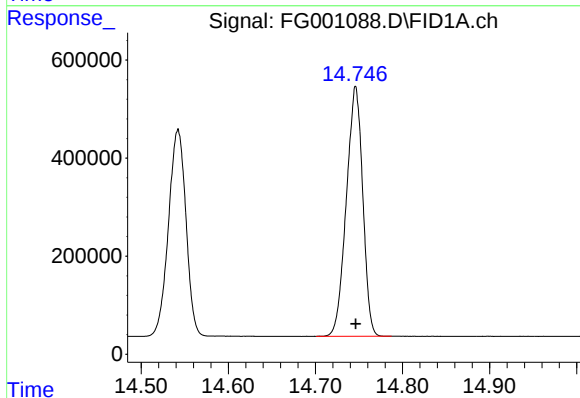


#10 N-TETRACOSANE

R.T.: 14.746 min
Delta R.T.: 0.000 min
Response: 6665203
Conc: 50.00 ug/ml

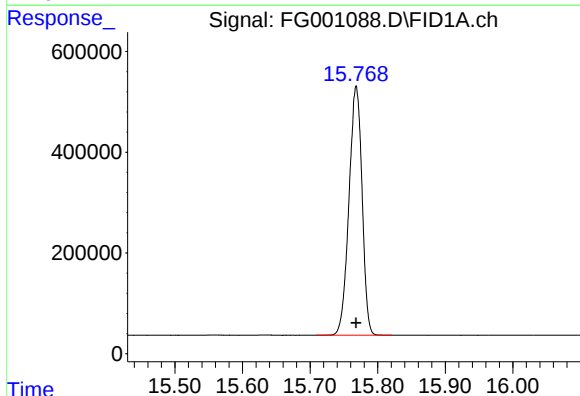


#11 N-HEXACOSANE

R.T.: 15.768 min
Delta R.T.: 0.000 min
Response: 6634343
Conc: 50.00 ug/ml

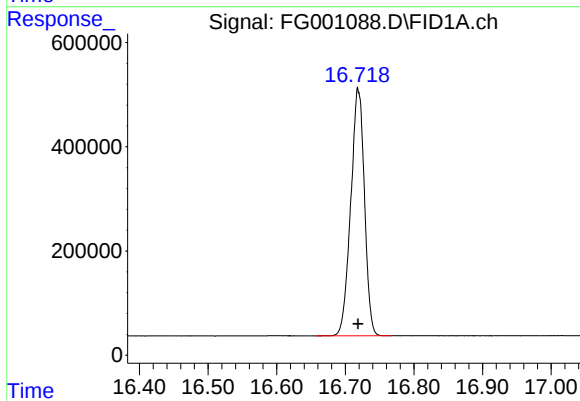

#12 N-OCTACOSANE


R.T.: 16.719 min
Delta R.T.: 0.000 min
Response: 6585860
Conc: 50.00 ug/ml

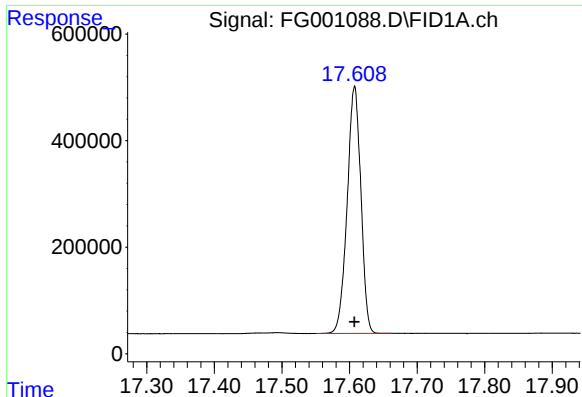

#13 N-TRIACONTANE


R.T.: 17.608 min
Delta R.T.: 0.000 min
Response: 6535598
Conc: 50.00 ug/ml

Instrument :
FID_G
ClientSampleId :

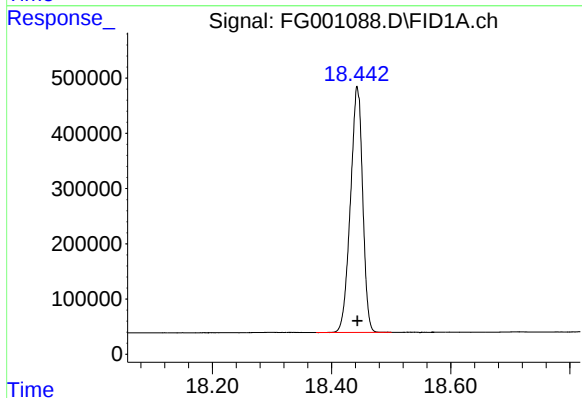


#14 N-DOTRIACONTANE

R.T.: 18.443 min
Delta R.T.: 0.000 min
Response: 6352661
Conc: 50.00 ug/ml

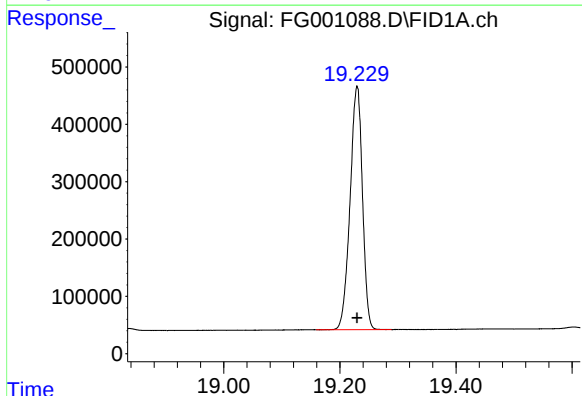


#15 N-TETRATRIACONTANE

R.T.: 19.230 min
Delta R.T.: 0.000 min
Response: 6281973
Conc: 50.00 ug/ml

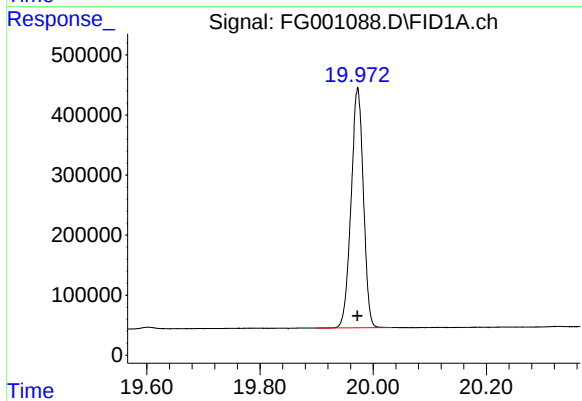

#16 N-HEXATRIACONTANE


R.T.: 19.972 min
Delta R.T.: 0.000 min
Response: 6015493
Conc: 50.00 ug/ml

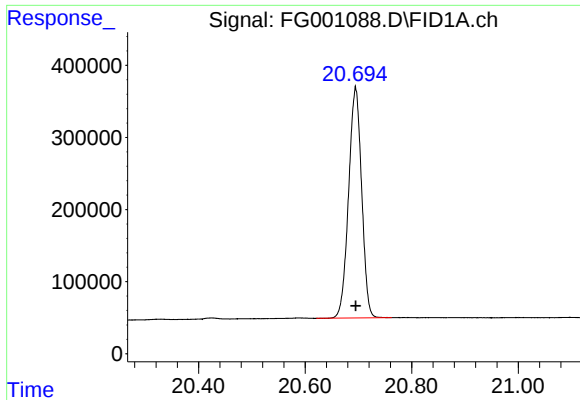

#17 N-OCTATRIACONTANE

R.T.: 20.695 min
Delta R.T.: 0.000 min
Response: 5429592
Conc: 50.00 ug/ml

Instrument :
FID_G
ClientSampleId :

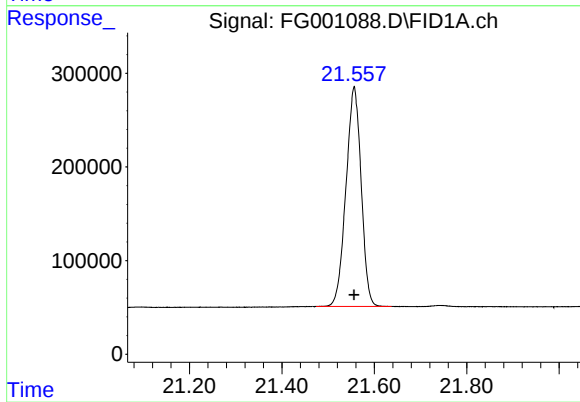

#18 N-TETRACONTANE

R.T.: 21.556 min
Delta R.T.: 0.000 min
Response: 5349600
Conc: 50.00 ug/ml