

Data Path : P:\HPCHEM1\FID_G\Data\FG060118\
 Data File : FG001094.D
 Signal(s) : FID1A.ch
 Acq On : 01 Jun 2018 16:36
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 05:36:27 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.543	5936569	48.561 ug/ml
Target Compounds			
1) N-OCTANE	2.195	6518058	48.070 ug/ml
2) N-DECANE	4.284	6601292	48.159 ug/ml
3) N-DODECANE	6.300	6683364	48.211 ug/ml
4) N-TETRADECANE	8.092	6742636	48.253 ug/ml
5) N-HEXADECANE	9.692	6794164	48.279 ug/ml
6) N-OCTADECANE	11.134	6836287	48.227 ug/ml
7) N-EICOSANE	12.443	6794454	48.250 ug/ml
8) N-DOCOSANE	13.642	6758870	48.227 ug/ml
10) N-TETRACOSANE	14.745	6710143	48.257 ug/ml
11) N-HEXACOSANE	15.768	6699082	48.359 ug/ml
12) N-OCTACOSANE	16.720	6671755	48.354 ug/ml
13) N-TRIACONTANE	17.610	6643648	48.419 ug/ml
14) N-DOTRIACONTANE	18.444	6477576	48.431 ug/ml
15) N-TETRATRIACONTANE	19.231	6415739	48.702 ug/ml
16) N-HEXATRIACONTANE	19.975	6141799	48.868 ug/ml
17) N-OCTATRIACONTANE	20.695	5537048	48.850 ug/ml
18) N-TETRACONTANE	21.558	5430835	48.460 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG060118\
Data File : FG001094.D
Signal(s) : FID1A.ch
Acq On : 01 Jun 2018 16:36
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 05:36:27 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

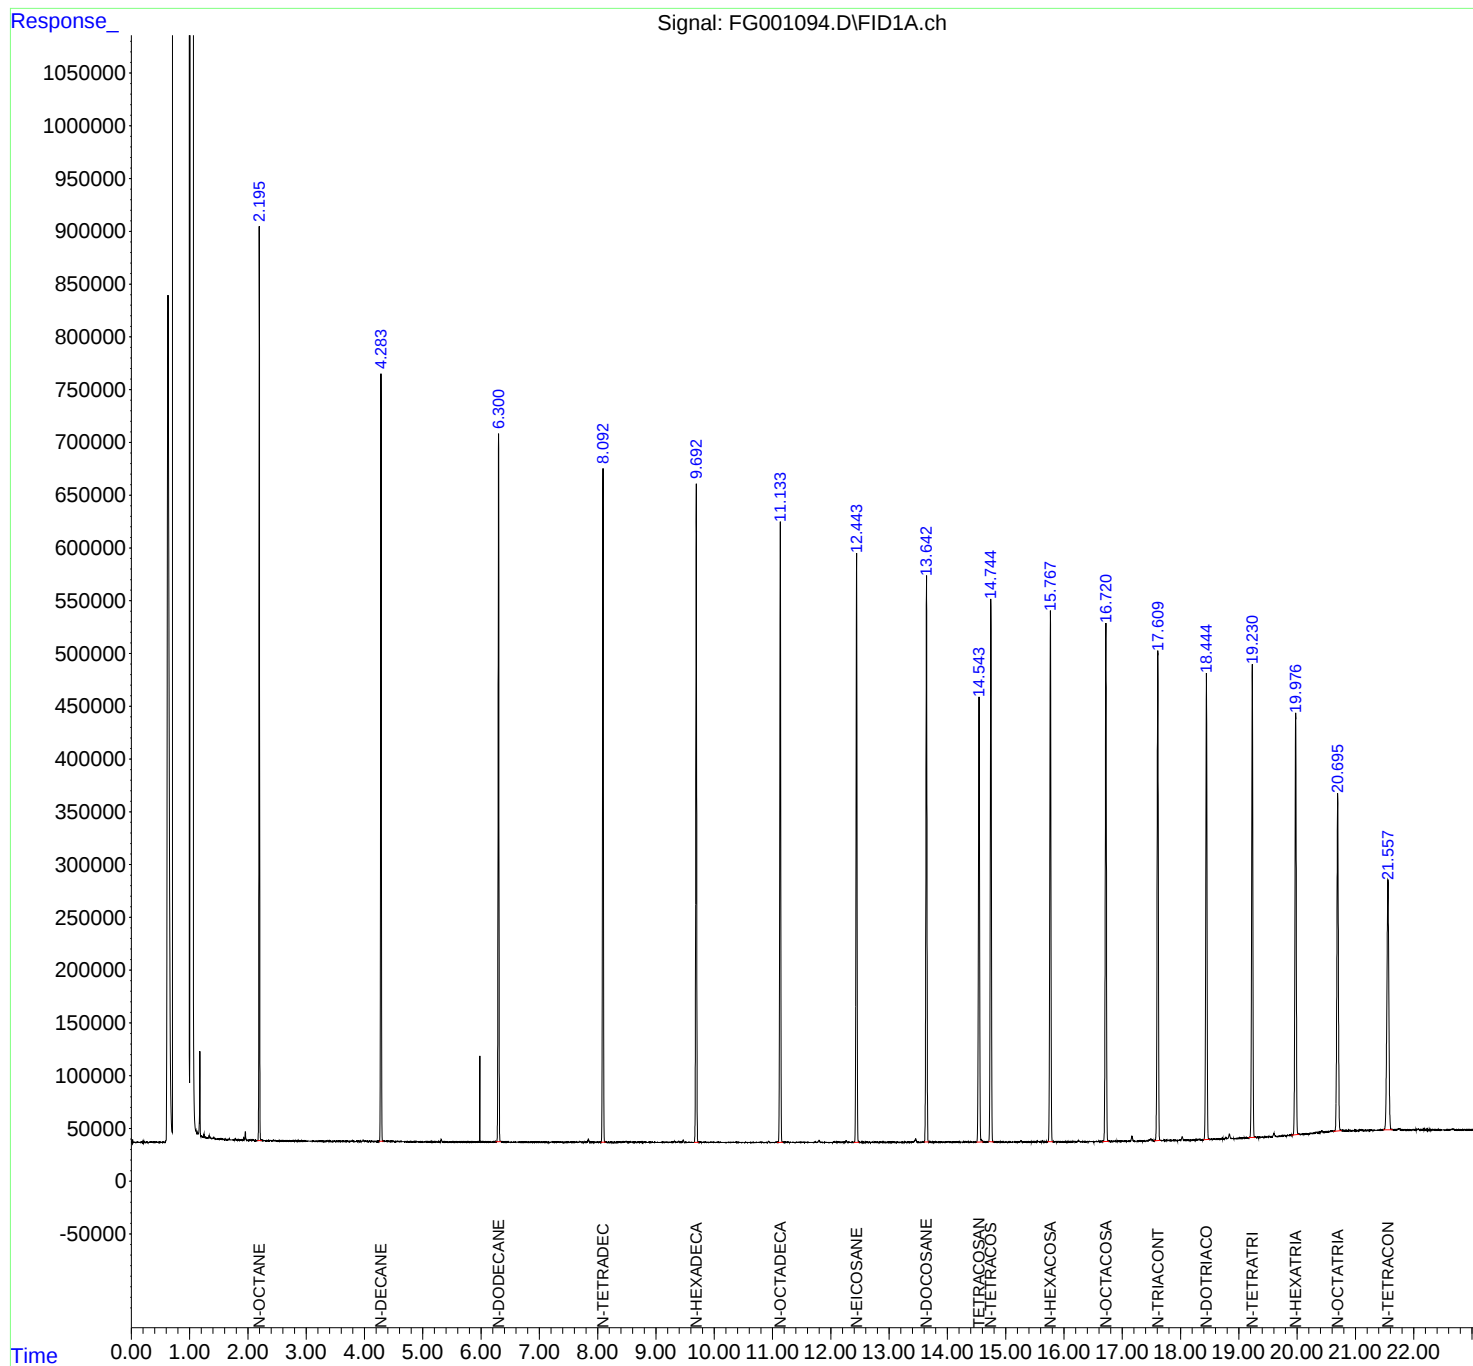


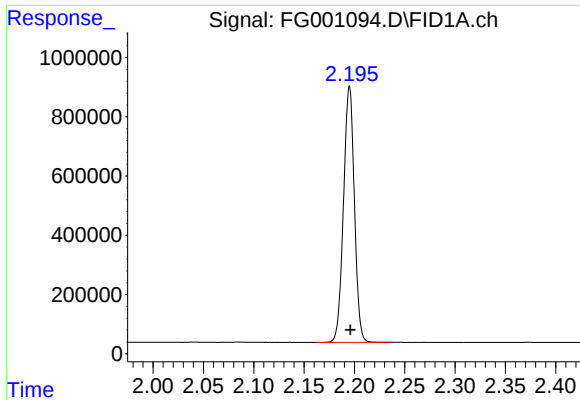

#1 N-OCTANE


R.T.: 2.195 min
Delta R.T.: 0.000 min
Response: 6518058
Conc: 48.07 ug/ml

Instrument :
FID_G
ClientSampleId :

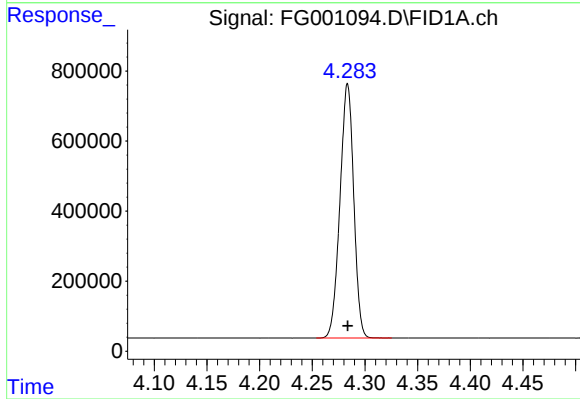


#2 N-DECANE

R.T.: 4.284 min
Delta R.T.: 0.000 min
Response: 6601292
Conc: 48.16 ug/ml

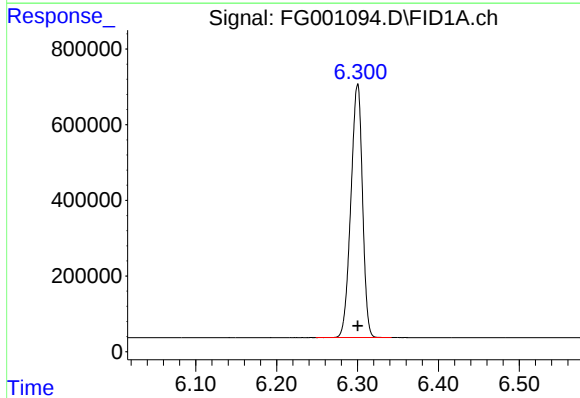


#3 N-DODECANE

R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 6683364
Conc: 48.21 ug/ml

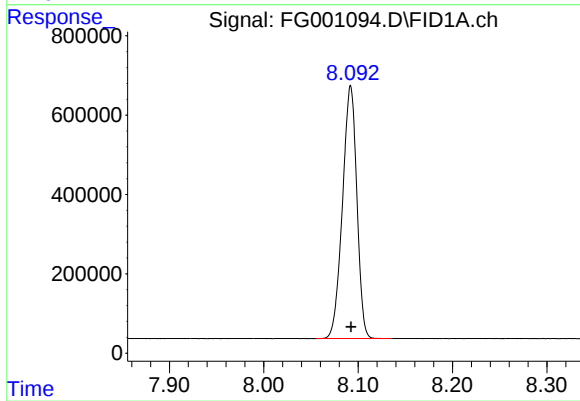

#4 N-TETRADECANE


R.T.: 8.092 min
Delta R.T.: 0.000 min
Response: 6742636
Conc: 48.25 ug/ml

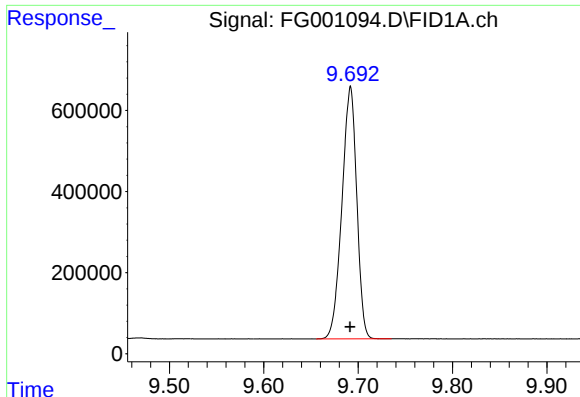

#5 N-HEXADECANE


R.T.: 9.692 min
Delta R.T.: 0.000 min
Response: 6794164
Conc: 48.28 ug/ml

Instrument :
FID_G
ClientSampleId :

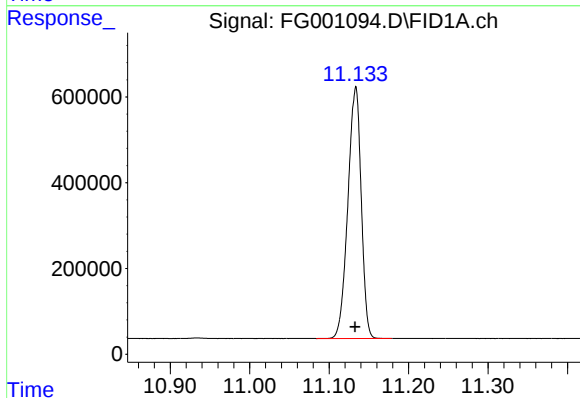


#6 N-OCTADECANE

R.T.: 11.134 min
Delta R.T.: 0.000 min
Response: 6836287
Conc: 48.23 ug/ml

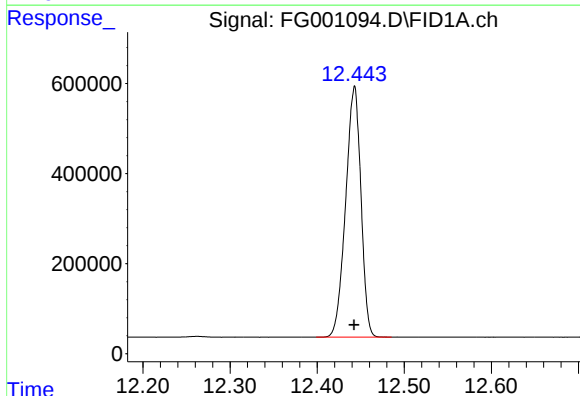


#7 N-EICOSANE

R.T.: 12.443 min
Delta R.T.: 0.000 min
Response: 6794454
Conc: 48.25 ug/ml

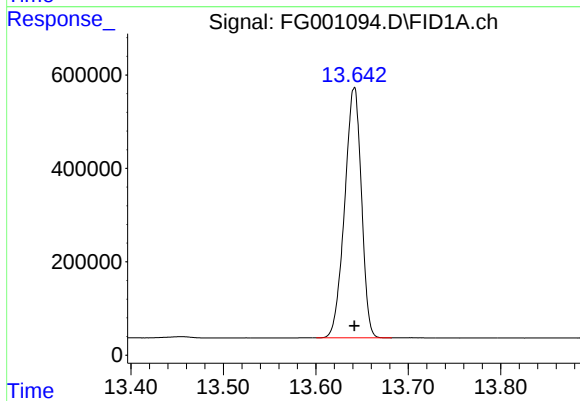

#8 N-DOCOSANE


R.T.: 13.642 min
Delta R.T.: 0.000 min
Response: 6758870
Conc: 48.23 ug/ml

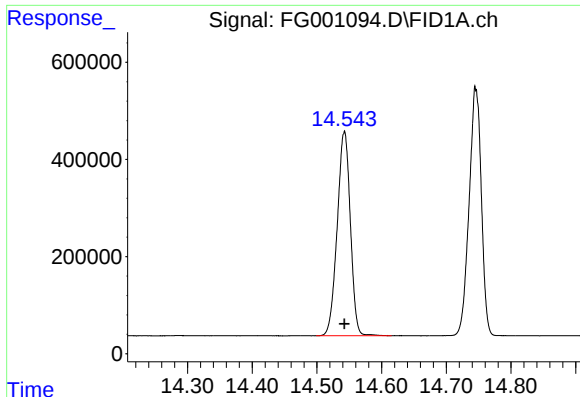

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.543 min
Delta R.T.: 0.000 min
Response: 5936569
Conc: 48.56 ug/ml

Instrument :
FID_G
ClientSampleId :

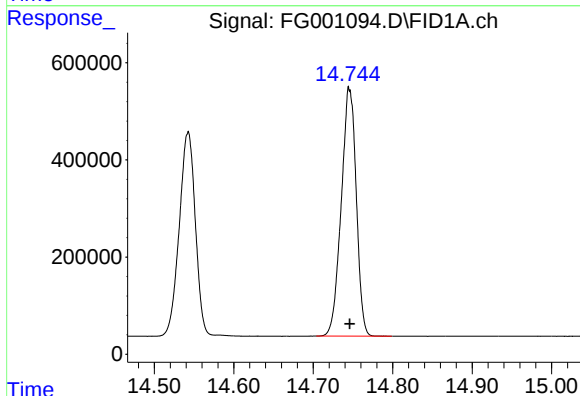


#10 N-TETRACOSANE

R.T.: 14.745 min
Delta R.T.: 0.000 min
Response: 6710143
Conc: 48.26 ug/ml

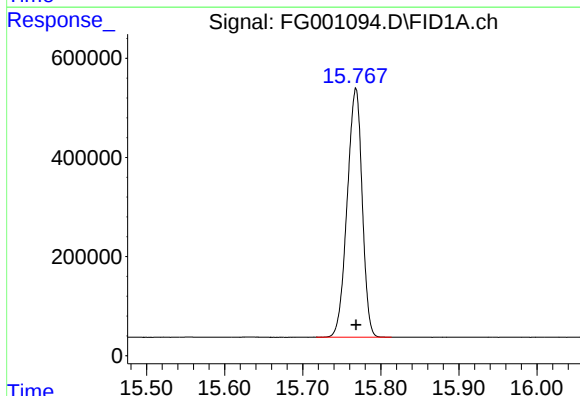


#11 N-HEXACOSANE

R.T.: 15.768 min
Delta R.T.: 0.000 min
Response: 6699082
Conc: 48.36 ug/ml

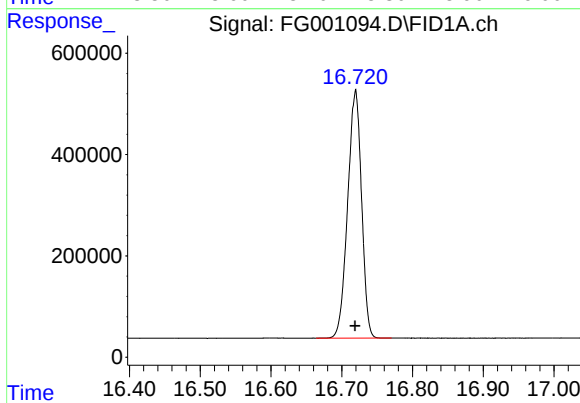

#12 N-OCTACOSANE


R.T.: 16.720 min
Delta R.T.: 0.000 min
Response: 6671755
Conc: 48.35 ug/ml

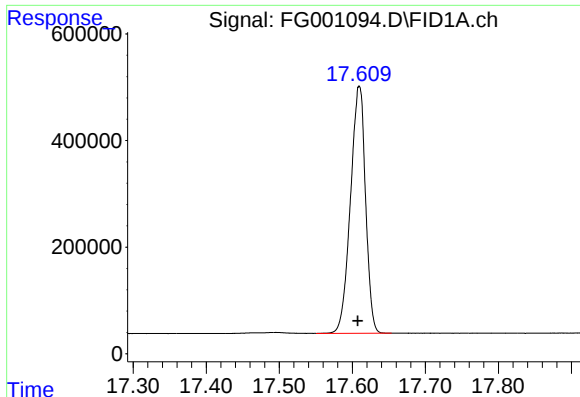

#13 N-TRIACONTANE


R.T.: 17.610 min
Delta R.T.: 0.002 min
Response: 6643648
Conc: 48.42 ug/ml

Instrument :
FID_G
ClientSampleId :

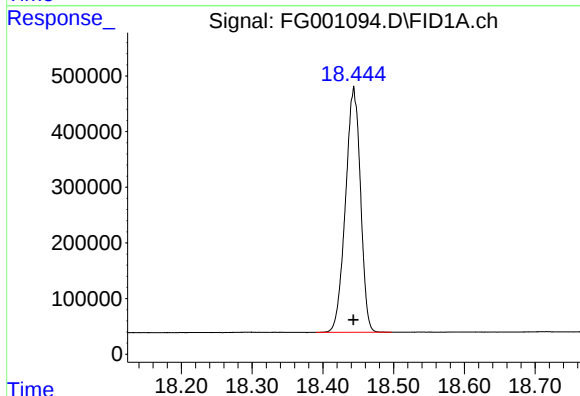


#14 N-DOTRIACONTANE

R.T.: 18.444 min
Delta R.T.: 0.000 min
Response: 6477576
Conc: 48.43 ug/ml

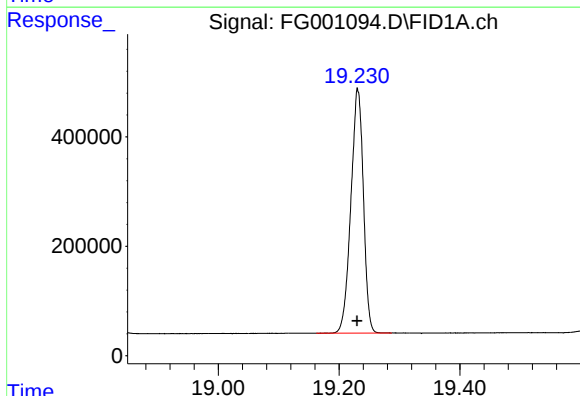


#15 N-TETRATRIACONTANE

R.T.: 19.231 min
Delta R.T.: 0.001 min
Response: 6415739
Conc: 48.70 ug/ml

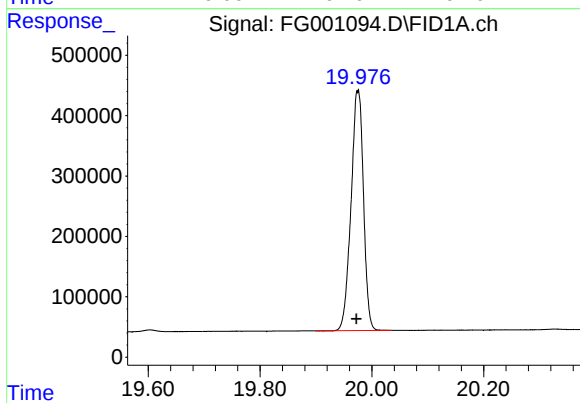

#16 N-HEXATRIACONTANE


R.T.: 19.975 min
Delta R.T.: 0.002 min
Response: 6141799
Conc: 48.87 ug/ml

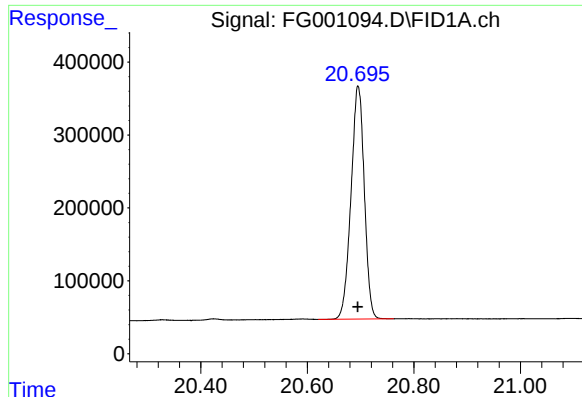

#17 N-OCTATRIACONTANE

R.T.: 20.695 min
Delta R.T.: 0.000 min
Response: 5537048
Conc: 48.85 ug/ml

Instrument :
FID_G
ClientSampleId :

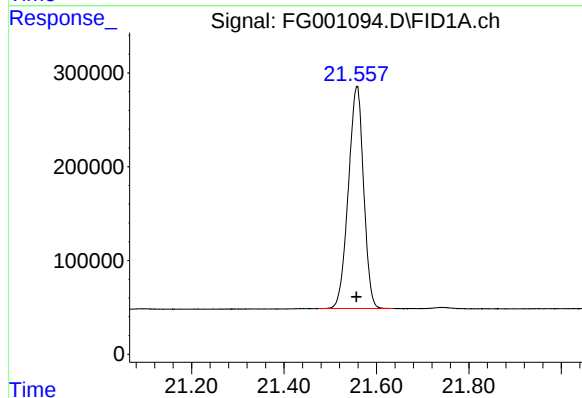

#18 N-TETRACONTANE

R.T.: 21.558 min
Delta R.T.: 0.002 min
Response: 5430835
Conc: 48.46 ug/ml