

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060122\
 Data File : FG009802.D
 Signal(s) : FID1A.ch
 Acq On : 01 Jun 2022 14:45
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 04:05:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.544	3926138	31.121 ug/ml
12)	N-OCTACOSANE	17.026	3323611	29.045 ug/ml
13)	N-TRIACONTANE	17.914	186276	1.730 ug/ml
14)	N-DOTRIACONTANE	18.750	243707	2.315 ug/ml
15)	N-TETRATRIACONTANE	19.534	184422	1.921 ug/ml
16)	N-HEXATRIACONTANE	20.277	110570	1.368 ug/ml
17)	N-OCTATRIACONTANE	20.999	81475	1.135 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060122\
Data File : FG009802.D
Signal(s) : FID1A.ch
Acq On : 01 Jun 2022 14:45
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 04:05:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

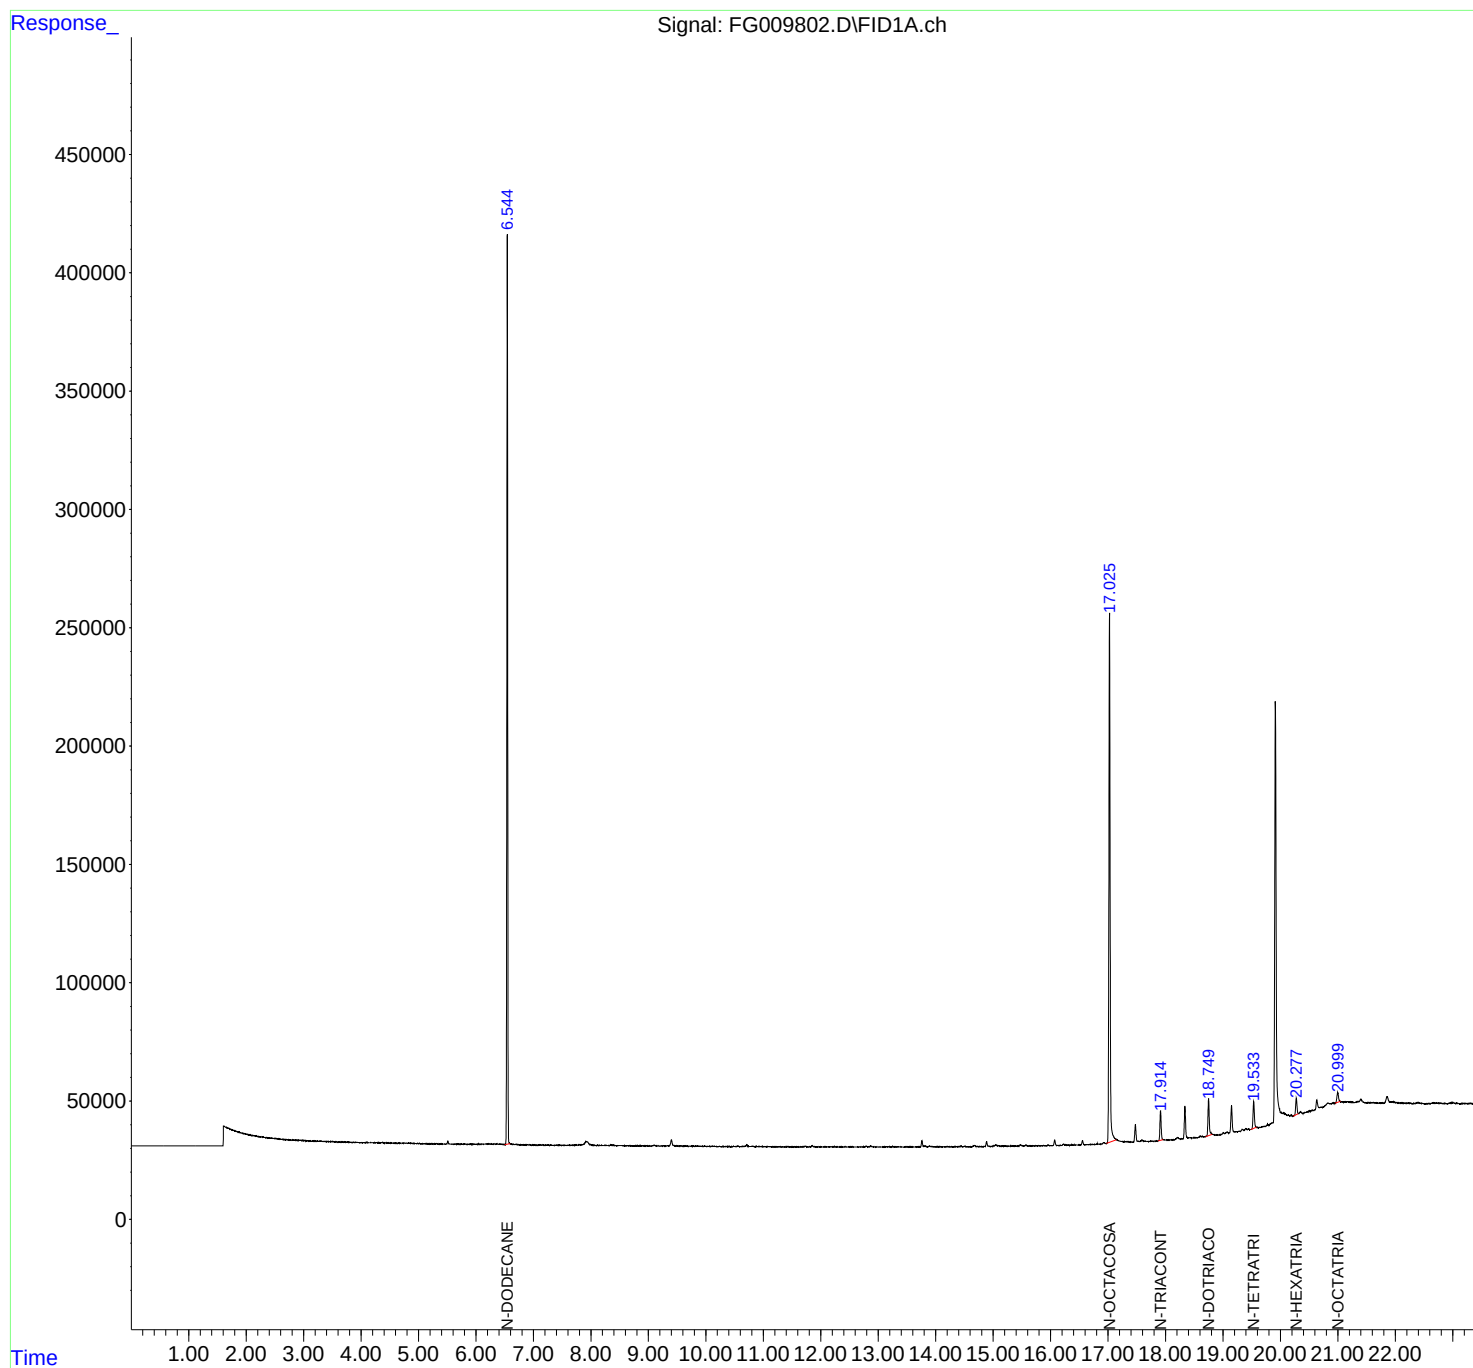


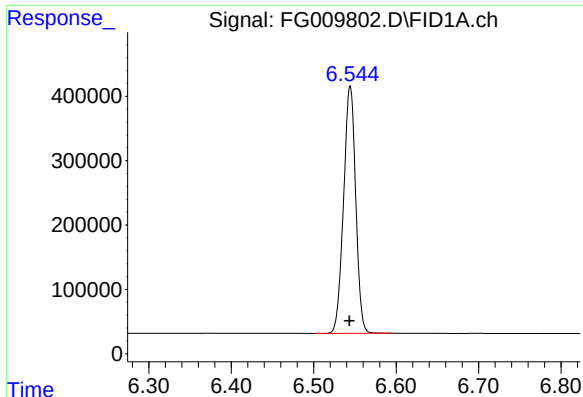

#3 N-DODECANE


R.T.: 6.544 min
Delta R.T.: 0.001 min
Response: 3926138
Conc: 31.12 ug/ml

Instrument :
FID_G
ClientSampleId :

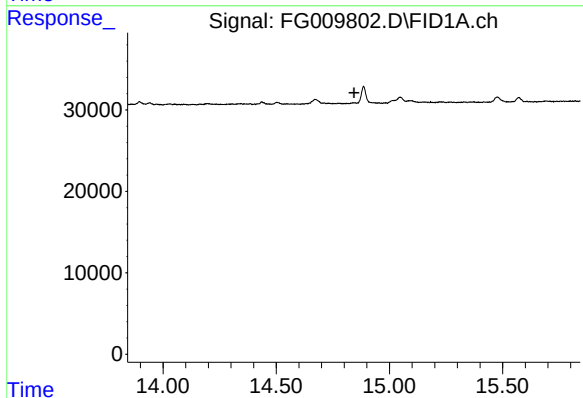


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.843 min
Response: 0
Conc: N.D.

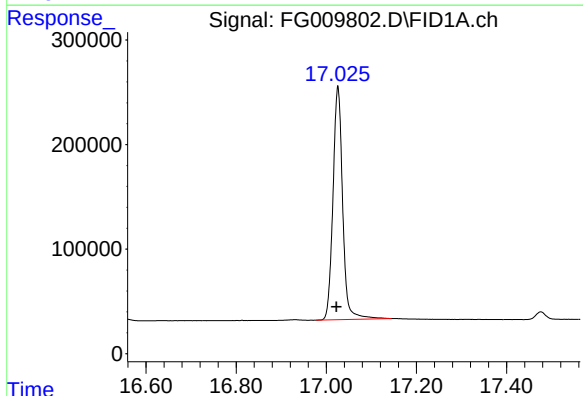


#12 N-OCTACOSANE

R.T.: 17.026 min
Delta R.T.: 0.003 min
Response: 3323611
Conc: 29.04 ug/ml

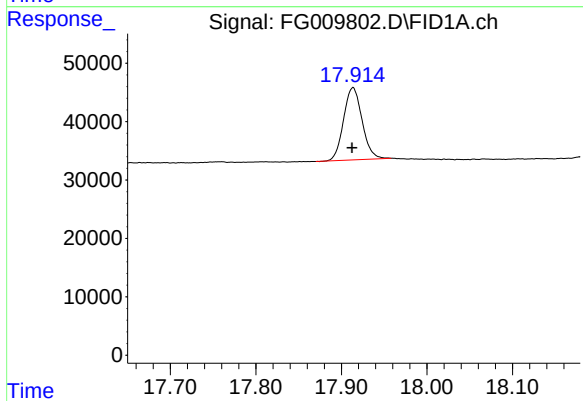

#13 N-TRIACONTANE


R.T.: 17.914 min
Delta R.T.: 0.001 min
Response: 186276
Conc: 1.73 ug/ml

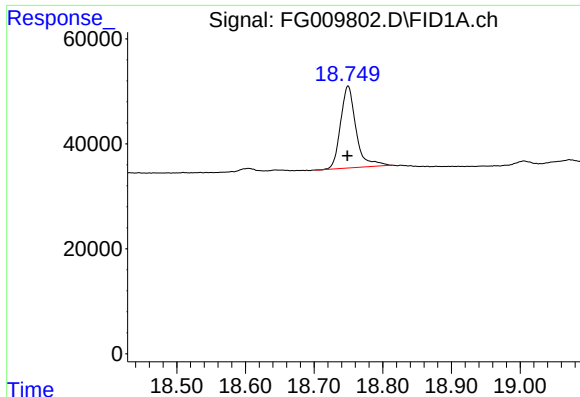

#14 N-DOTRIACONTANE


R.T.: 18.750 min
Delta R.T.: 0.001 min
Response: 243707
Conc: 2.32 ug/ml

Instrument :
FID_G
ClientSampleId :

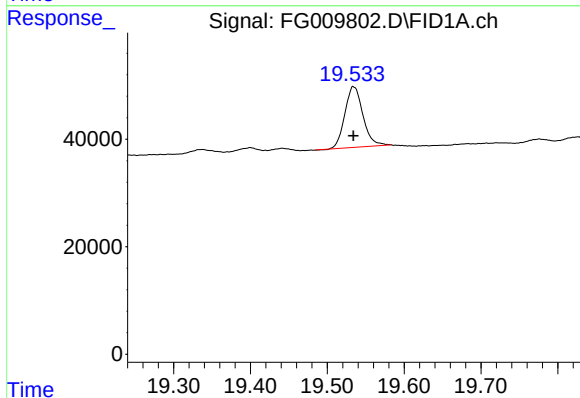


#15 N-TETRATRIACONTANE

R.T.: 19.534 min
Delta R.T.: 0.000 min
Response: 184422
Conc: 1.92 ug/ml

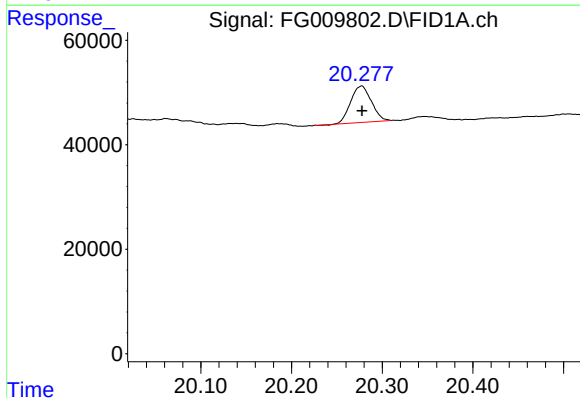

#16 N-HEXATRIACONTANE

R.T.: 20.277 min
Delta R.T.: 0.000 min
Response: 110570
Conc: 1.37 ug/ml

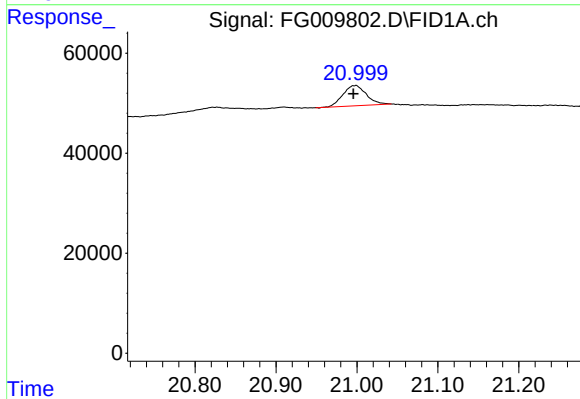

#17 N-OCTATRIACONTANE

R.T.: 20.999 min
Delta R.T.: 0.003 min
Response: 81475
Conc: 1.13 ug/ml