

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060122\
Data File : FG009804.D
Signal(s) : FID1A.ch
Acq On : 01 Jun 2022 15:43
Operator : AJ\MA
Sample : N2656-15 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 04:06:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2)	N-DECANE	4.367	365298	2.893 ug/ml
3)	N-DODECANE	6.543	475580	3.770 ug/ml
4)	N-TETRADECANE	8.373	587063	4.620 ug/ml
5)	N-HEXADECANE	9.983	723079	5.733 ug/ml
6)	N-OCTADECANE	11.428	527610	4.180 ug/ml
7)	N-EICOSANE	12.740	303308	2.480 ug/ml
8)	N-DOCOSANE	13.941	127412	1.057 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060122\
Data File : FG009804.D
Signal(s) : FID1A.ch
Acq On : 01 Jun 2022 15:43
Operator : AJ\MA
Sample : N2656-15 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 04:06:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

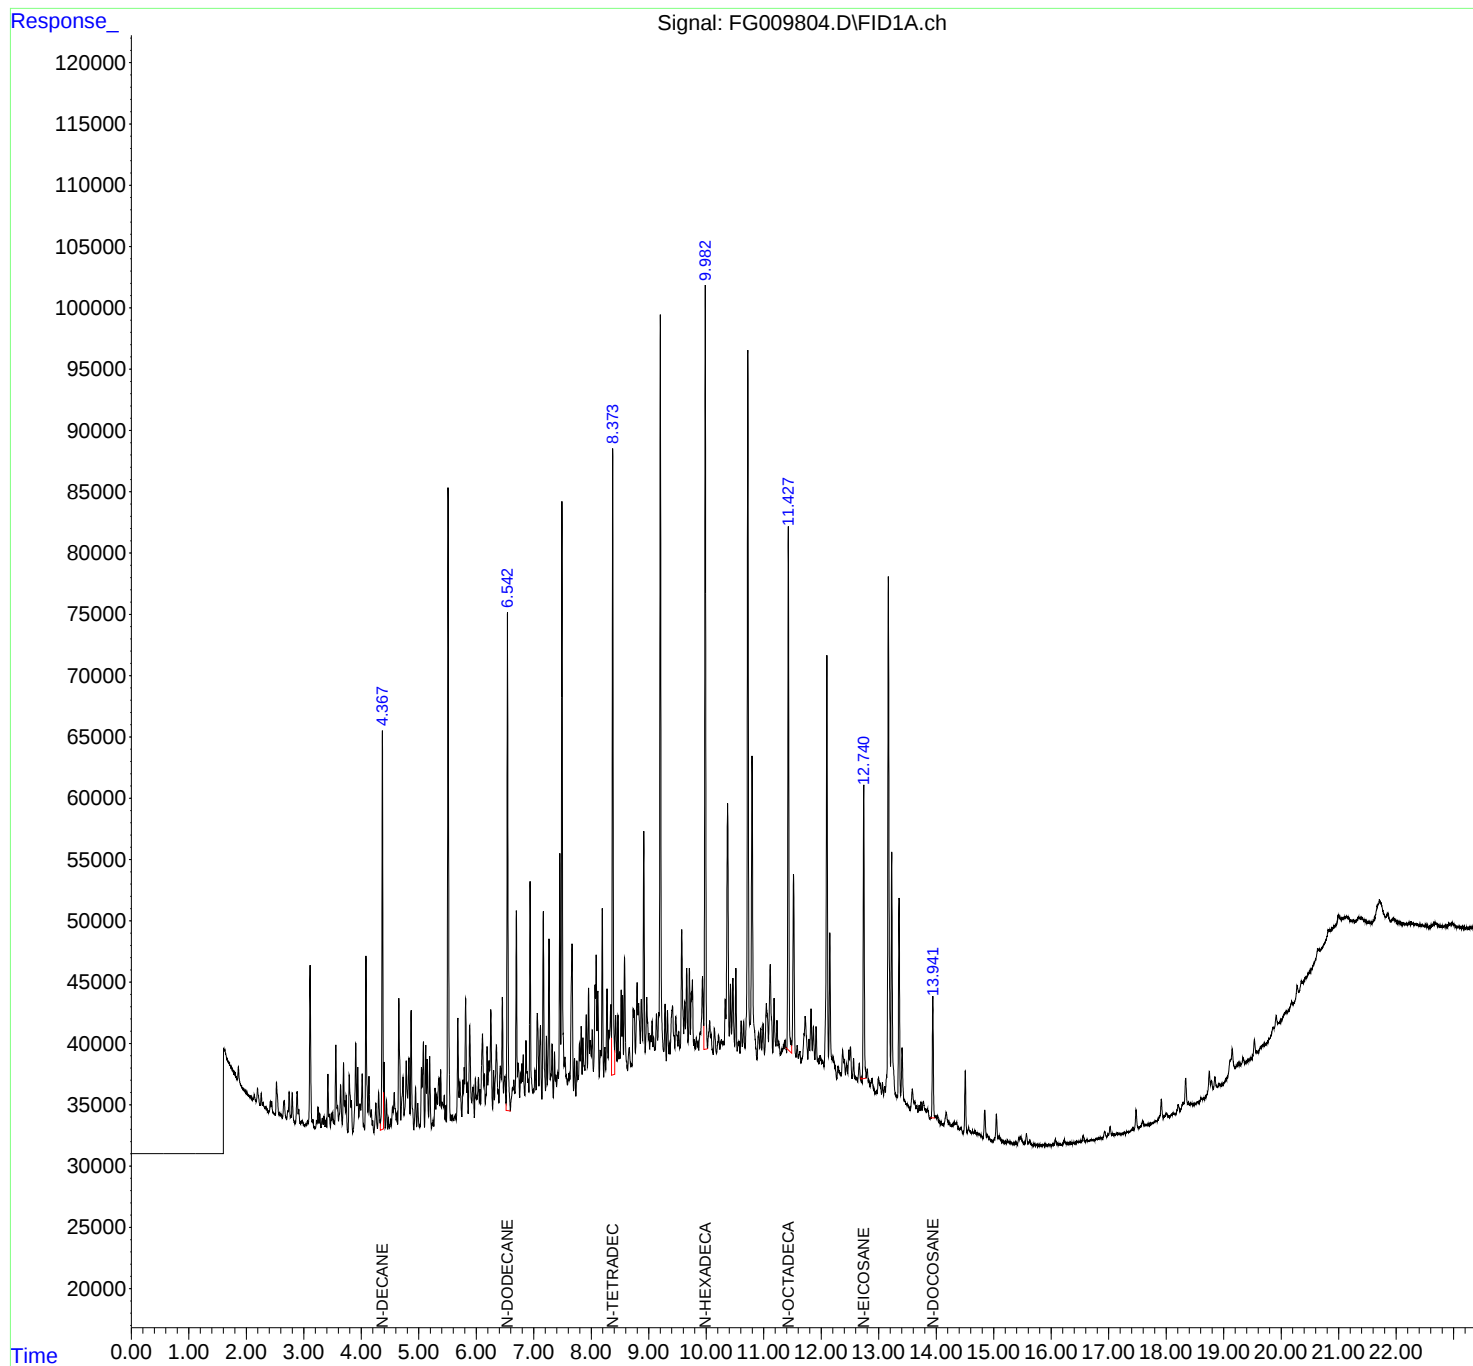


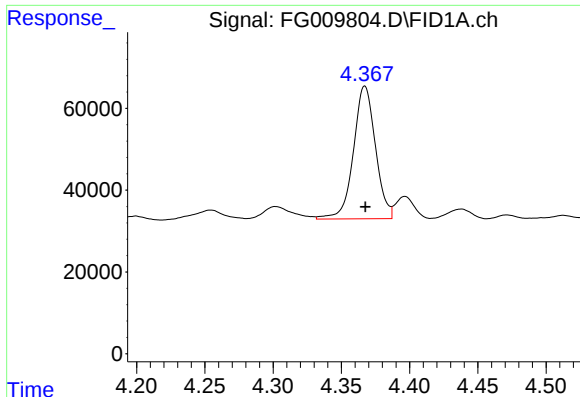

#2 N-DECANE


R.T.: 4.367 min
Delta R.T.: 0.000 min
Response: 365298
Conc: 2.89 ug/ml

Instrument :
FID_G
ClientSampleId :

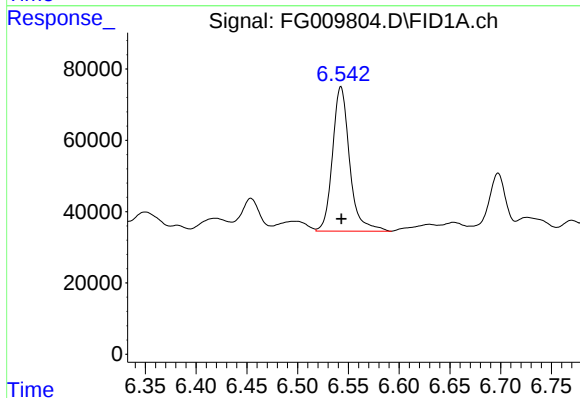


#3 N-DODECANE

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 475580
Conc: 3.77 ug/ml

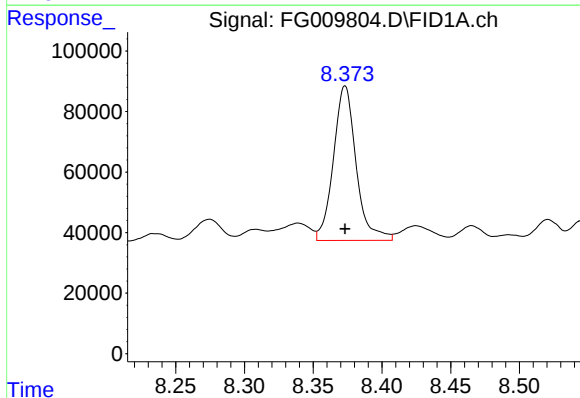


#4 N-TETRADECANE

R.T.: 8.373 min
Delta R.T.: 0.000 min
Response: 587063
Conc: 4.62 ug/ml

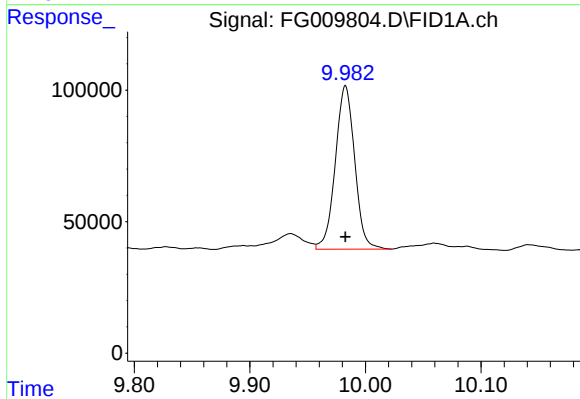

#5 N-HEXADECANE


R.T.: 9.983 min
Delta R.T.: 0.000 min
Response: 723079
Conc: 5.73 ug/ml

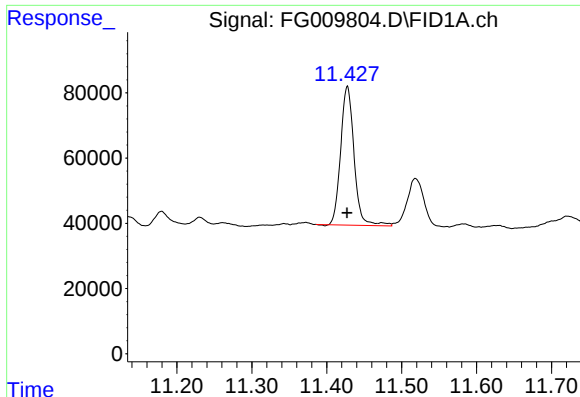

#6 N-OCTADECANE


R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 527610
Conc: 4.18 ug/ml

Instrument :
FID_G
ClientSampleId :

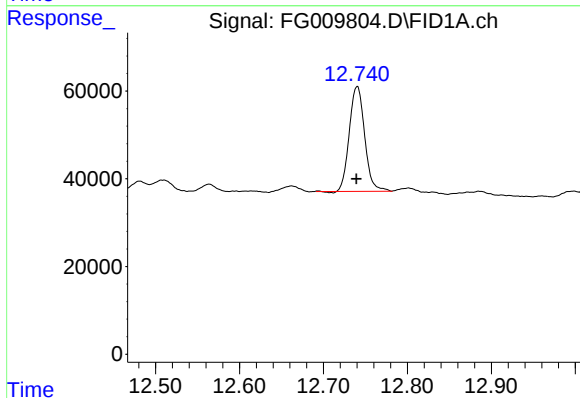


#7 N-EICOSANE

R.T.: 12.740 min
Delta R.T.: 0.001 min
Response: 303308
Conc: 2.48 ug/ml

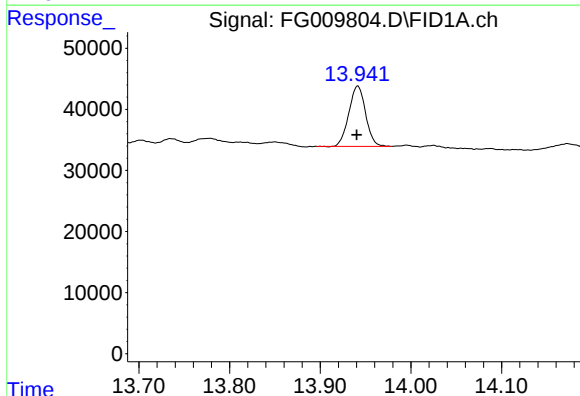

#8 N-DOCOSANE

R.T.: 13.941 min
Delta R.T.: 0.001 min
Response: 127412
Conc: 1.06 ug/ml

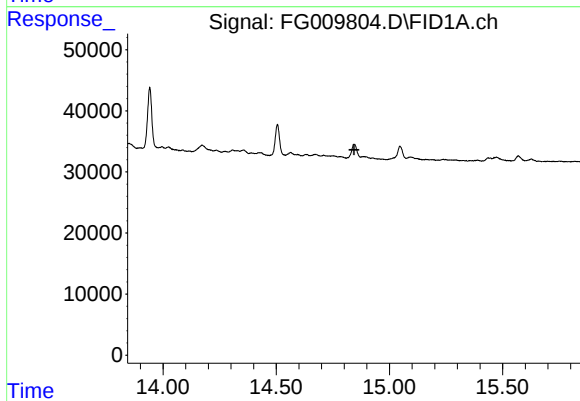

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.843 min
Response: 0
Conc: N.D.