

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060221\
 Data File : FG008135.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jun 2021 15:29
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 03 02:09:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.511	5045007	37.817 ug/ml
11) N-HEXACOSANE	16.009	114144	0.868 ug/ml
12) N-OCTACOSANE	16.966	6183813	47.710 ug/ml
13) N-TRIACONTANE	17.852	589321	4.616 ug/ml
14) N-DOTRIACONTANE	18.686	722819	5.817 ug/ml
15) N-TETRATRIACONTANE	19.471	577177	4.934 ug/ml
16) N-HEXATRIACONTANE	20.213	390281	3.524 ug/ml
17) N-OCTATRIACONTANE	20.975	270134	2.615 ug/ml
18) N-TETRACONTANE	21.934	163274	1.521 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060221\
Data File : FG008135.D
Signal(s) : FID1A.ch
Acq On : 02 Jun 2021 15:29
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 03 02:09:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

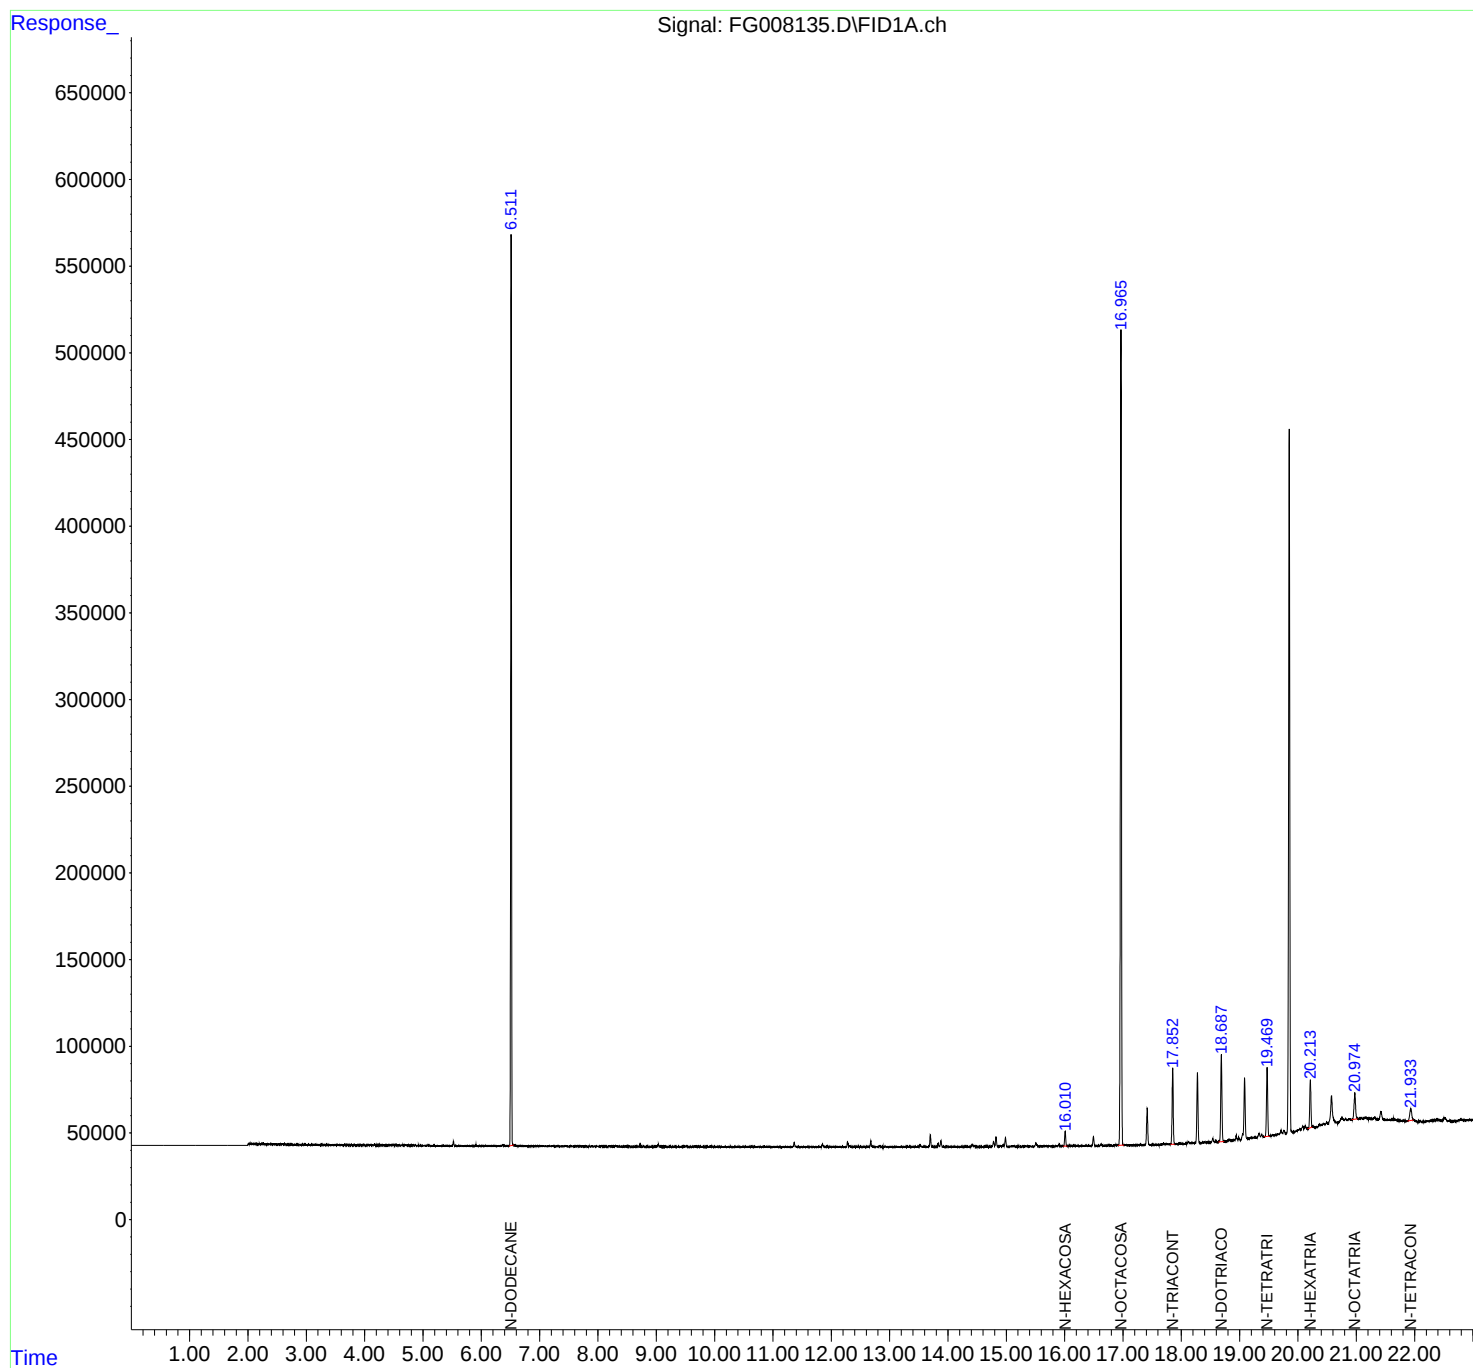


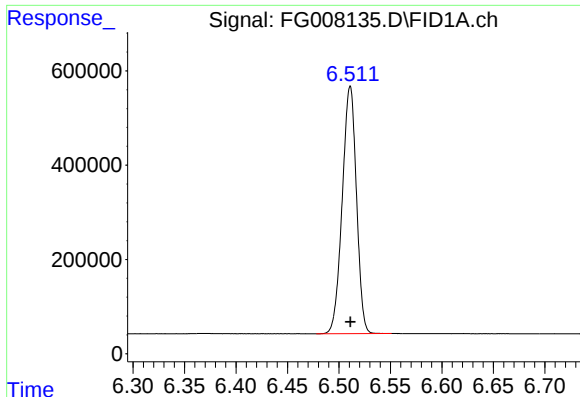

#3 N-DODECANE


R.T.: 6.511 min
Delta R.T.: 0.000 min
Response: 5045007
Conc: 37.82 ug/ml

Instrument :
FID_G
ClientSampleId :

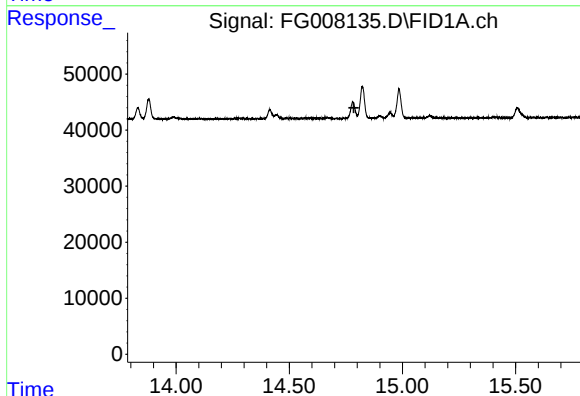


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

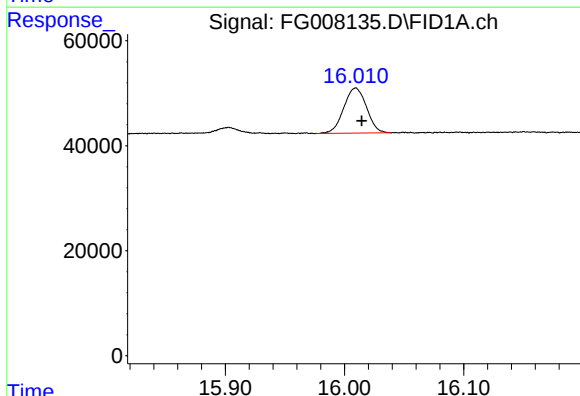


#11 N-HEXACOSANE

R.T.: 16.009 min
Delta R.T.: -0.005 min
Response: 114144
Conc: 0.87 ug/ml

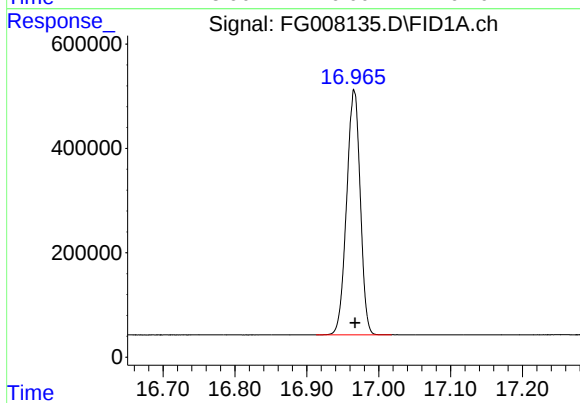

#12 N-OCTACOSANE


R.T.: 16.966 min
Delta R.T.: -0.001 min
Response: 6183813
Conc: 47.71 ug/ml

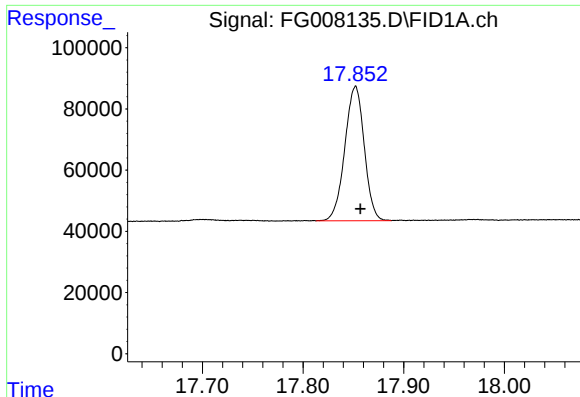

#13 N-TRIACONTANE


R.T.: 17.852 min
Delta R.T.: -0.005 min
Response: 589321
Conc: 4.62 ug/ml

Instrument :
FID_G
ClientSampleId :

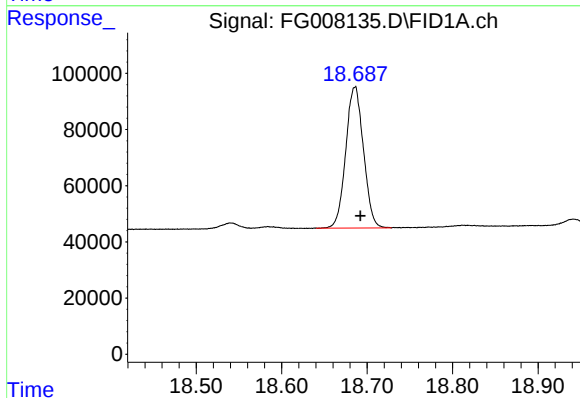


#14 N-DOTRIACONTANE

R.T.: 18.686 min
Delta R.T.: -0.006 min
Response: 722819
Conc: 5.82 ug/ml

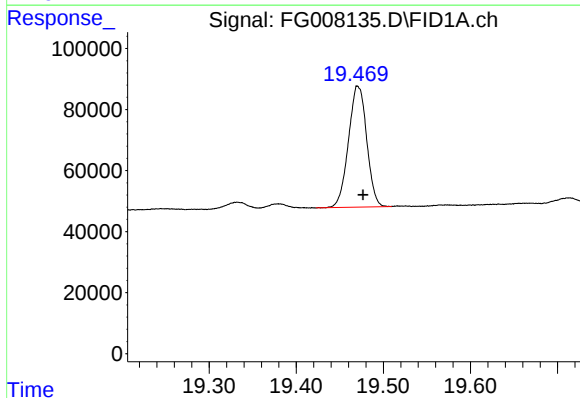


#15 N-TETRATRIACONTANE

R.T.: 19.471 min
Delta R.T.: -0.006 min
Response: 577177
Conc: 4.93 ug/ml

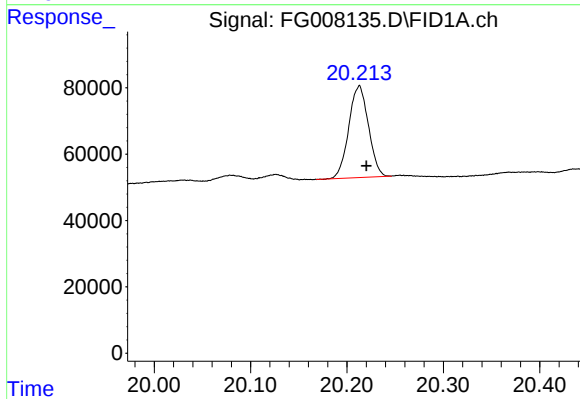

#16 N-HEXATRIACONTANE


R.T.: 20.213 min
Delta R.T.: -0.007 min
Response: 390281
Conc: 3.52 ug/ml

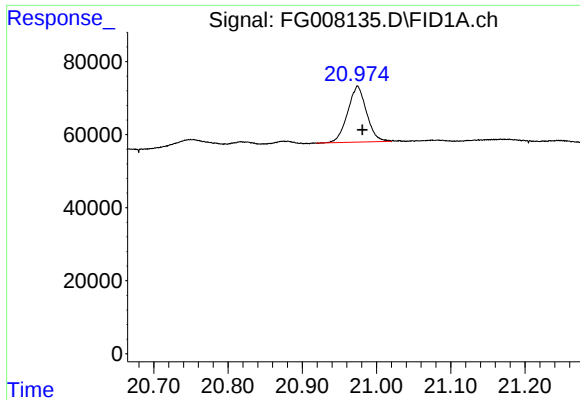

#17 N-OCTATRIACONTANE

R.T.: 20.975 min
Delta R.T.: -0.006 min
Response: 270134
Conc: 2.62 ug/ml

Instrument :
FID_G
ClientSampleId :

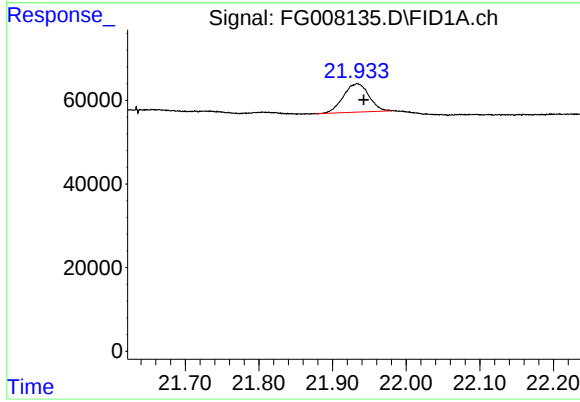

#18 N-TETRACONTANE

R.T.: 21.934 min
Delta R.T.: -0.009 min
Response: 163274
Conc: 1.52 ug/ml