

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060319\
 Data File : FG005073.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jun 2019 15:32
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Jun 04 00:55:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
 Quant Title :
 QLast Update : Thu May 09 14:52:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.792	5639586	46.994 ug/ml
Target Compounds			
2) N-DECANE	4.485	7702201	54.493 ug/ml
3) N-DODECANE	6.517	7561844	52.708 ug/ml
4) N-TETRADECANE	8.321	7304993	50.904 ug/ml
5) N-HEXADECANE	9.929	7130788	49.366 ug/ml
6) N-OCTADECANE	11.375	6843199	47.998 ug/ml
7) N-EICOSANE	12.689	6692143	47.220 ug/ml
8) N-DOCOSANE	13.891	6501147	46.910 ug/ml
10) N-TETRACOSANE	14.997	6492341	47.923 ug/ml
11) N-HEXACOSANE	16.020	6330743	48.210 ug/ml
12) N-OCTACOSANE	16.971	6333578	49.823 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060319\
Data File : FG005073.D
Signal(s) : FID1A.ch
Acq On : 03 Jun 2019 15:32
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Jun 04 00:55:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

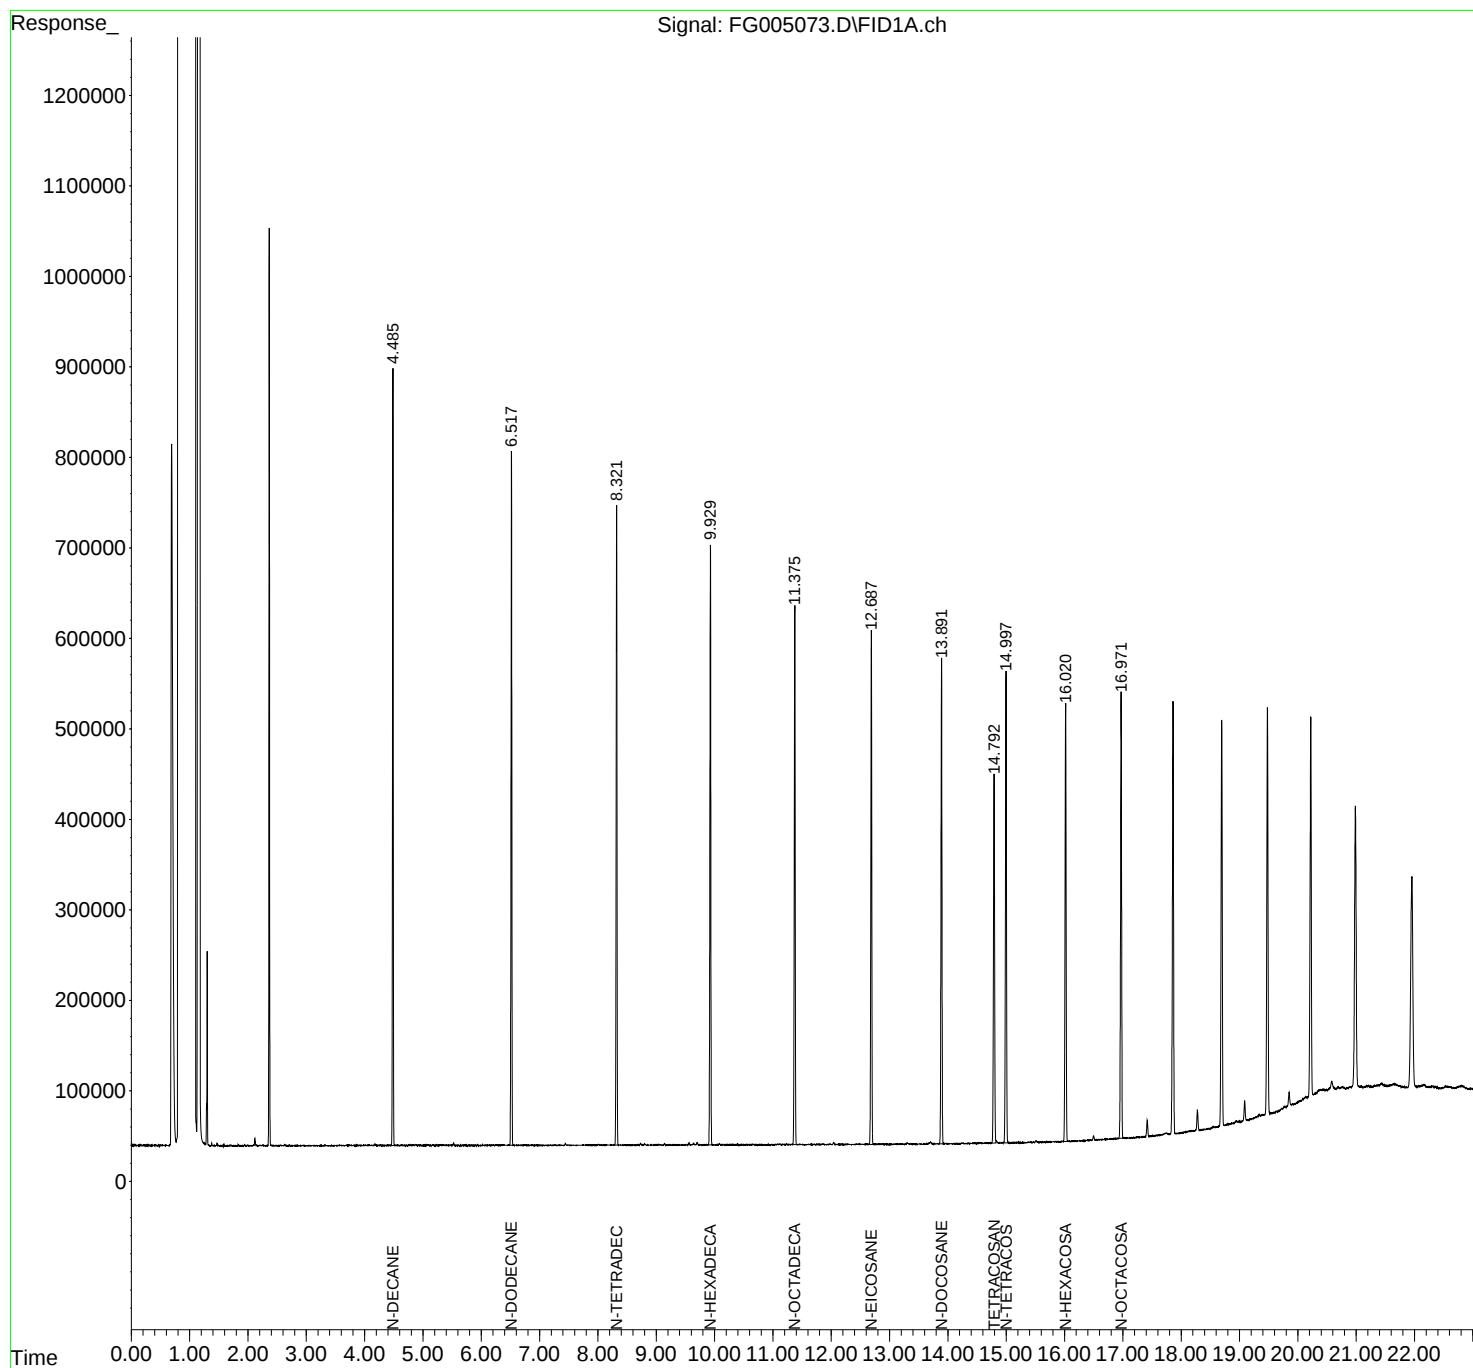

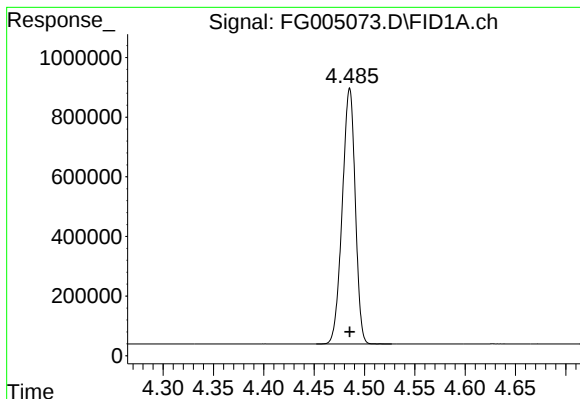


#2 N-DECANE

R.T.: 4.485 min
Delta R.T.: 0.000 min
Response: 7702201
Conc: 54.49 ug/ml

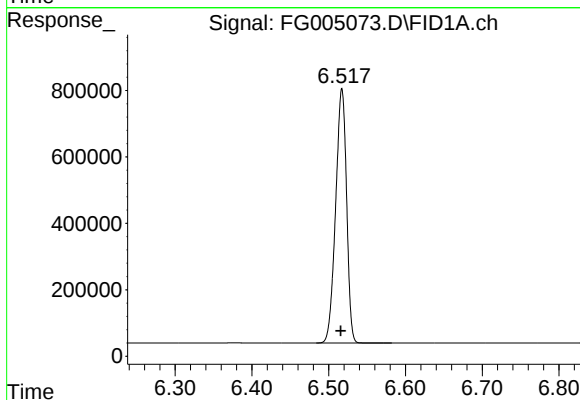


#3 N-DODECANE

R.T.: 6.517 min
Delta R.T.: 0.001 min
Response: 7561844
Conc: 52.71 ug/ml

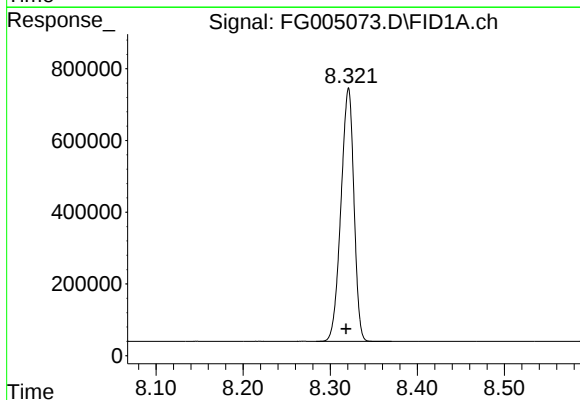


#4 N-TETRADECANE

R.T.: 8.321 min
Delta R.T.: 0.003 min
Response: 7304993
Conc: 50.90 ug/ml

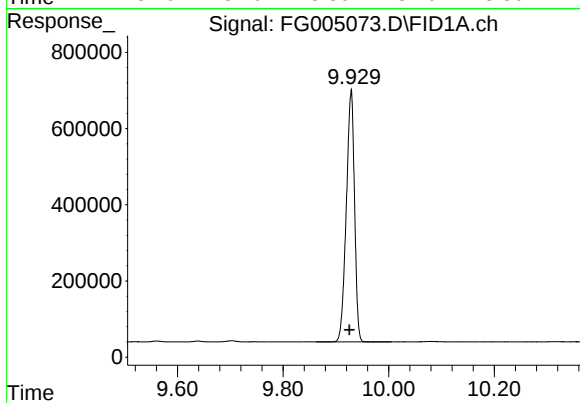


#5 N-HEXADECANE

R.T.: 9.929 min
Delta R.T.: 0.003 min
Response: 7130788
Conc: 49.37 ug/ml

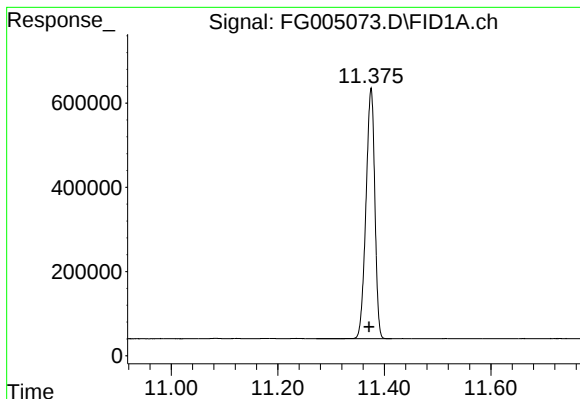


#6 N-OCTADECANE

R.T.: 11.375 min
Delta R.T.: 0.004 min
Response: 6843199
Conc: 48.00 ug/ml

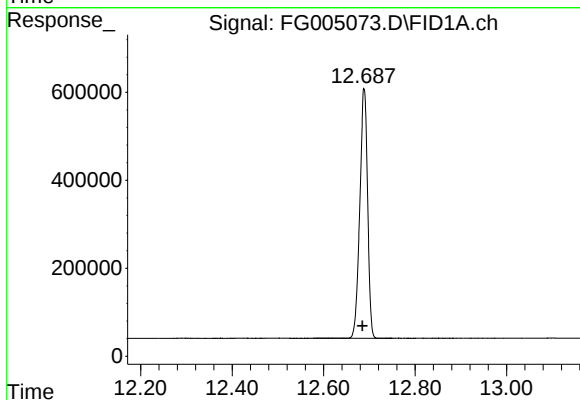


#7 N-EICOSANE

R.T.: 12.689 min
Delta R.T.: 0.004 min
Response: 6692143
Conc: 47.22 ug/ml

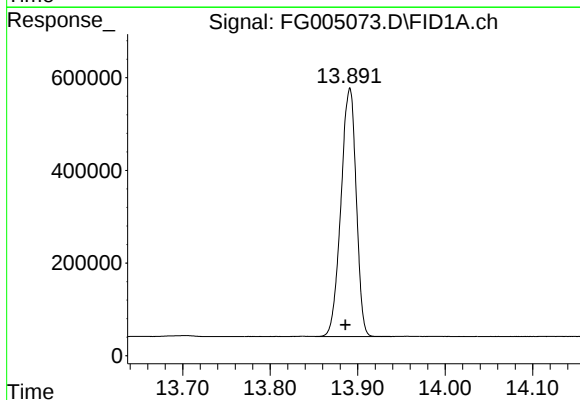


#8 N-DOCOSANE

R.T.: 13.891 min
Delta R.T.: 0.005 min
Response: 6501147
Conc: 46.91 ug/ml

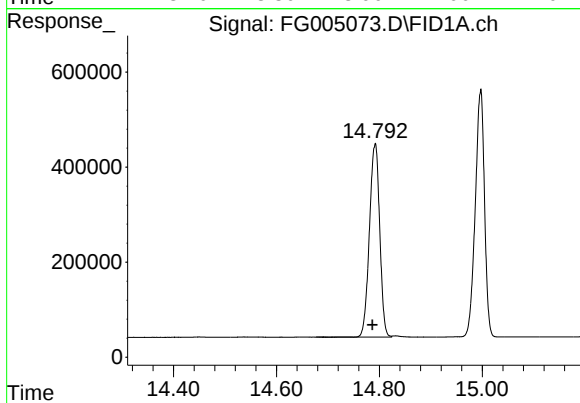


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.792 min
Delta R.T.: 0.006 min
Response: 5639586
Conc: 46.99 ug/ml

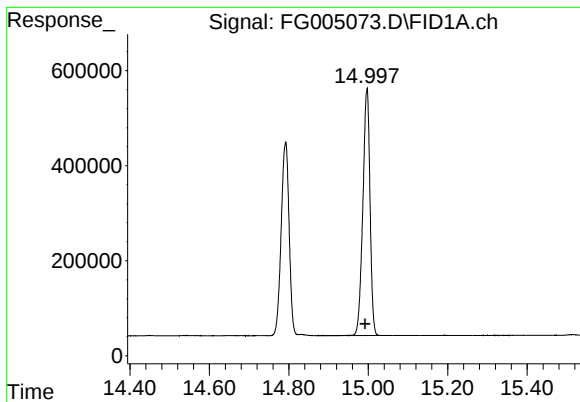


#10 N-TETRACOSANE

R.T.: 14.997 min
Delta R.T.: 0.005 min
Response: 6492341
Conc: 47.92 ug/ml

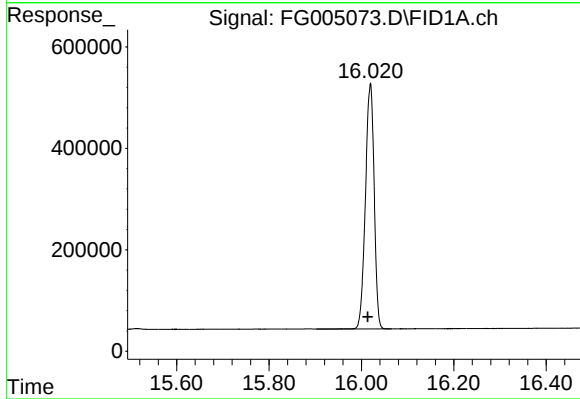

#11 N-HEXACOSANE

R.T.: 16.020 min
Delta R.T.: 0.006 min
Response: 6330743
Conc: 48.21 ug/ml

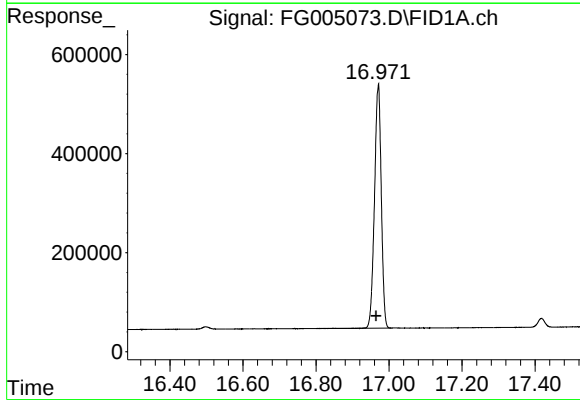

#12 N-OCTACOSANE

R.T.: 16.971 min
Delta R.T.: 0.006 min
Response: 6333578
Conc: 49.82 ug/ml