

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
 Data File : FG008152.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jun 2021 09:46
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 01:45:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.511	4048801	30.350 ug/ml
11) N-HEXACOSANE	16.011	90846	0.691 ug/ml
12) N-OCTACOSANE	16.967	5023124	38.755 ug/ml
13) N-TRIACONTANE	17.853	534987	4.191 ug/ml
14) N-DOTRIACONTANE	18.688	665754	5.357 ug/ml
15) N-TETRATRIACONTANE	19.472	533037	4.557 ug/ml
16) N-HEXATRIACONTANE	20.214	368114	3.324 ug/ml
17) N-OCTATRIACONTANE	20.976	261537	2.532 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
Data File : FG008152.D
Signal(s) : FID1A.ch
Acq On : 03 Jun 2021 09:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 01:45:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

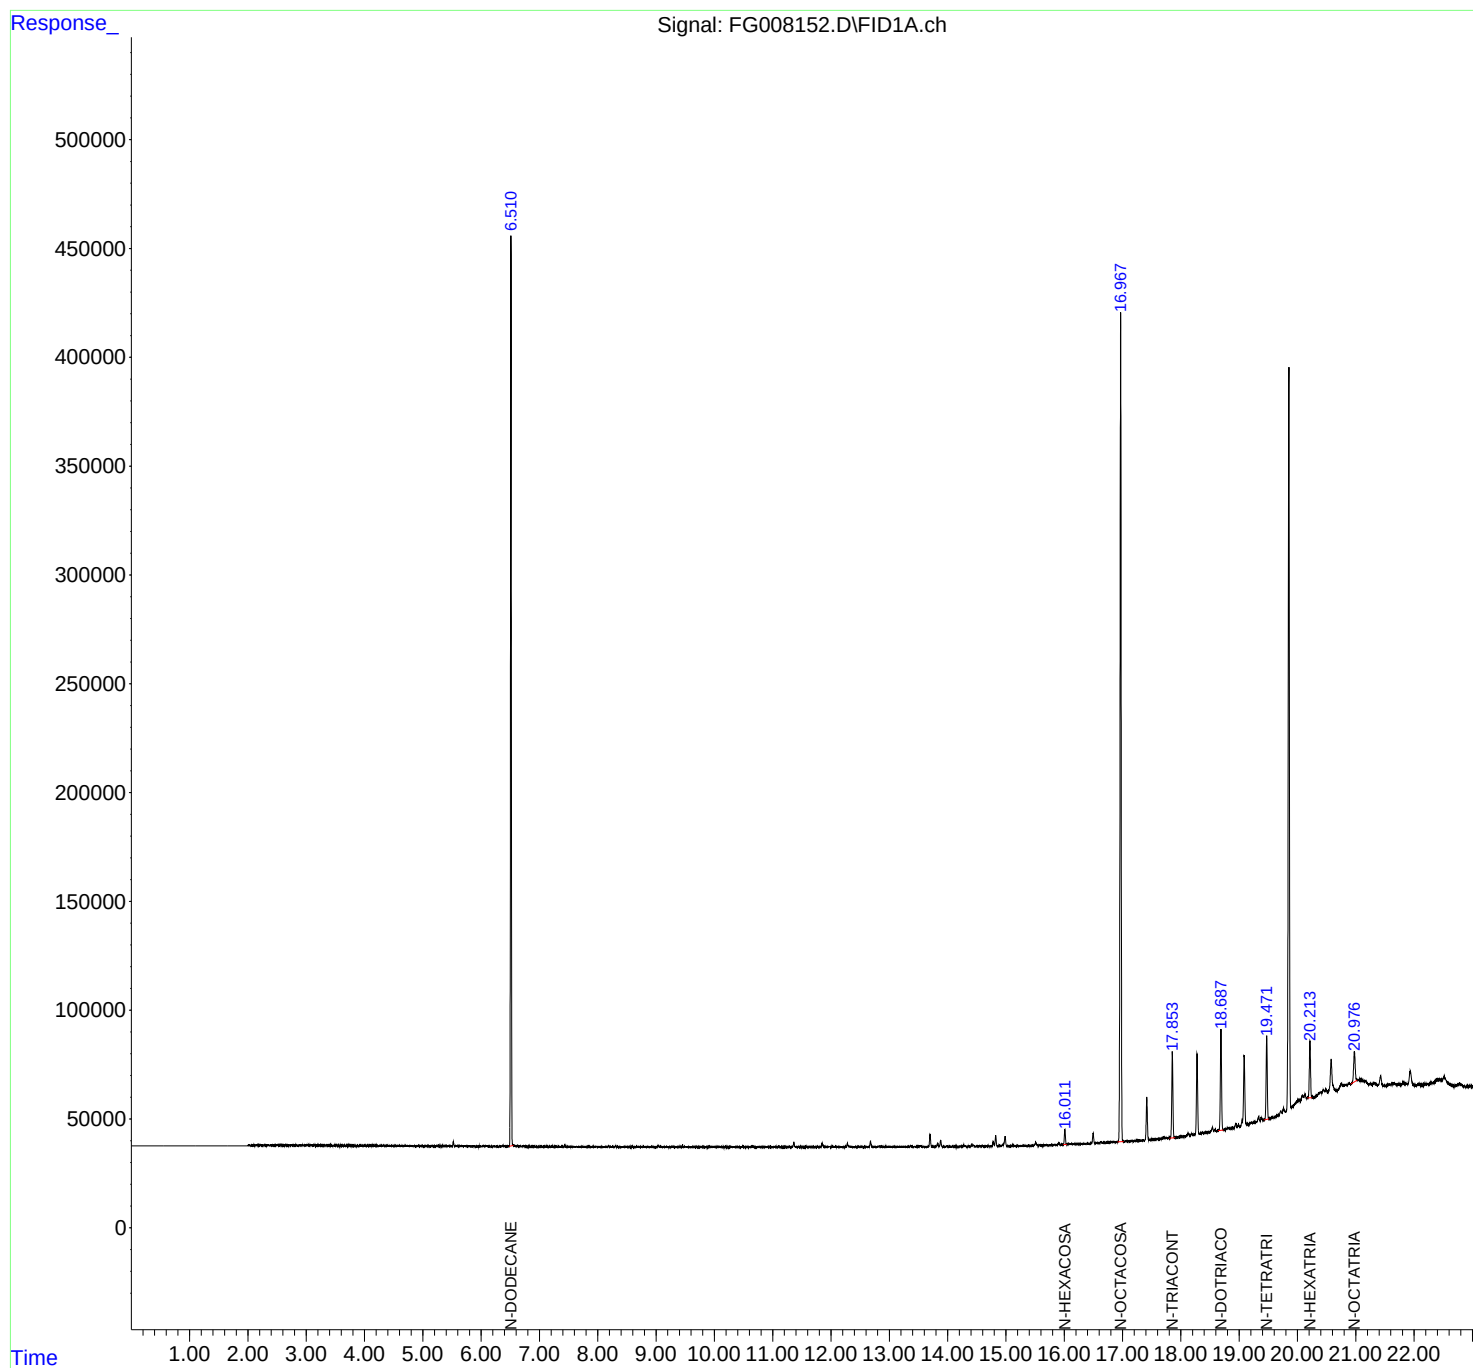


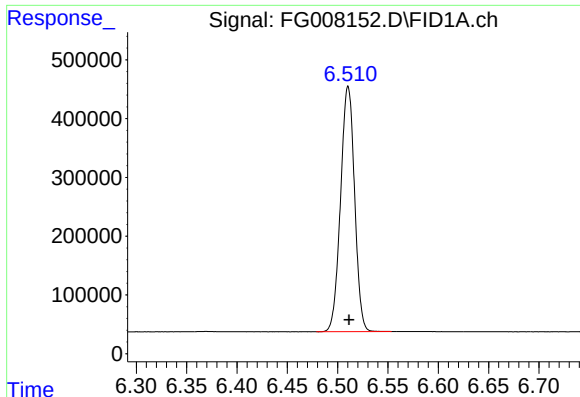

#3 N-DODECANE


R.T.: 6.511 min
Delta R.T.: 0.000 min
Response: 4048801
Conc: 30.35 ug/ml

Instrument :
FID_G
ClientSampleId :

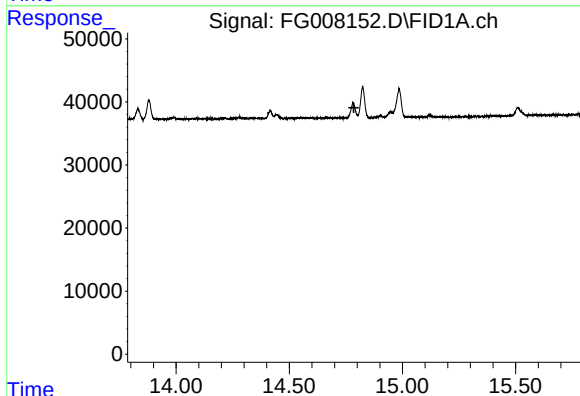


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

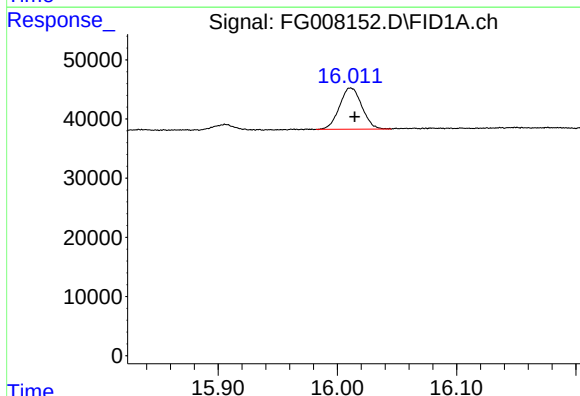


#11 N-HEXACOSANE

R.T.: 16.011 min
Delta R.T.: -0.003 min
Response: 90846
Conc: 0.69 ug/ml

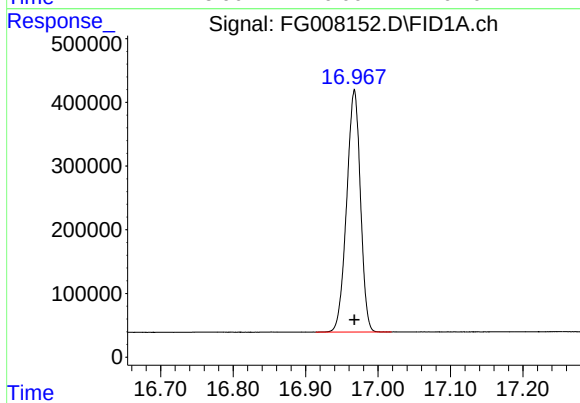

#12 N-OCTACOSANE


R.T.: 16.967 min
Delta R.T.: 0.000 min
Response: 5023124
Conc: 38.75 ug/ml

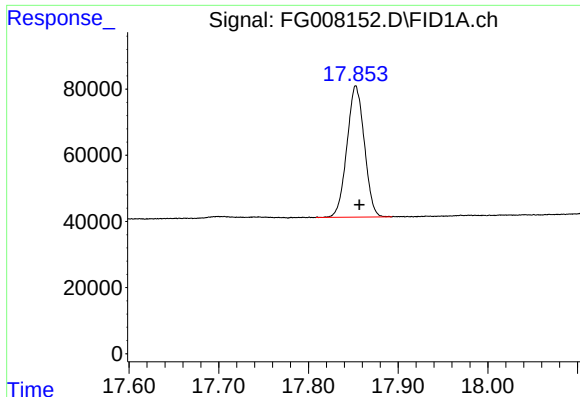

#13 N-TRIACONTANE


R.T.: 17.853 min
Delta R.T.: -0.004 min
Response: 534987
Conc: 4.19 ug/ml

Instrument :
FID_G
ClientSampleId :

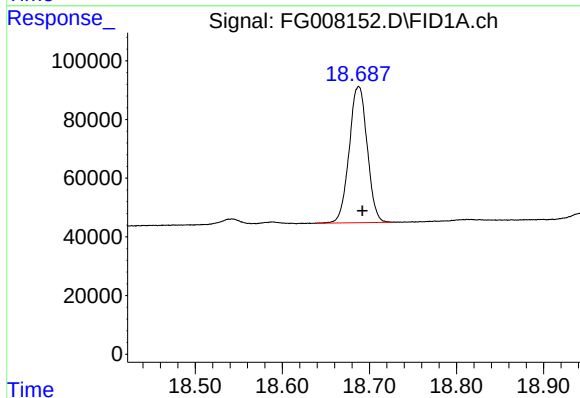


#14 N-DOTRIACONTANE

R.T.: 18.688 min
Delta R.T.: -0.004 min
Response: 665754
Conc: 5.36 ug/ml

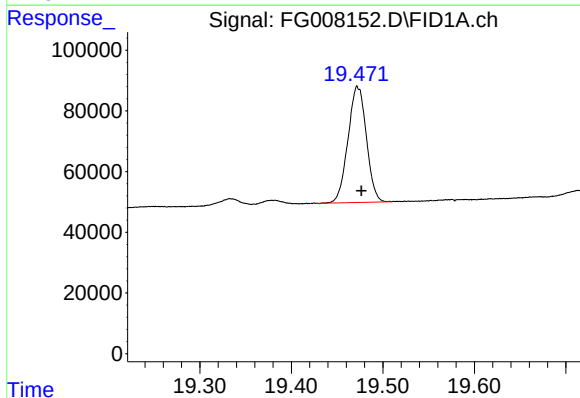


#15 N-TETRATRIACONTANE

R.T.: 19.472 min
Delta R.T.: -0.004 min
Response: 533037
Conc: 4.56 ug/ml

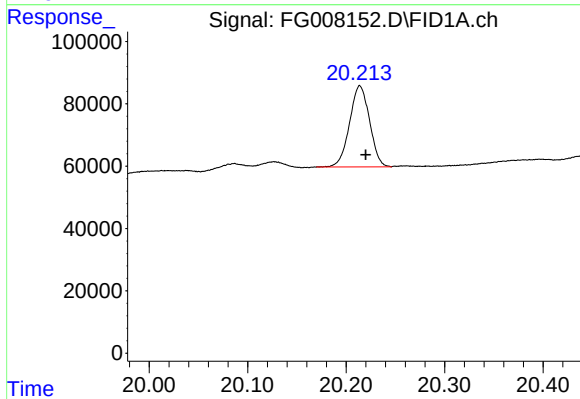

#16 N-HEXATRIACONTANE

R.T.: 20.214 min
Delta R.T.: -0.006 min
Response: 368114
Conc: 3.32 ug/ml

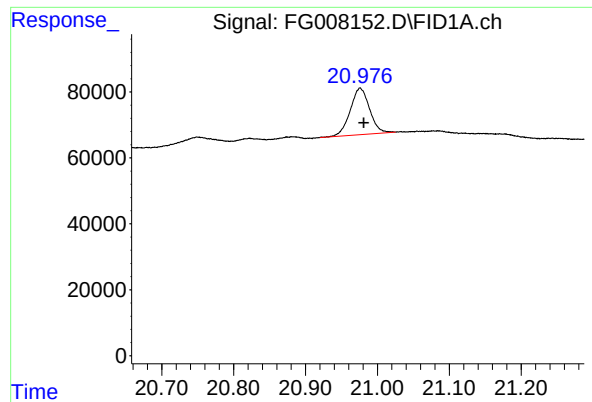

#17 N-OCTATRIACONTANE

R.T.: 20.976 min
Delta R.T.: -0.005 min
Response: 261537
Conc: 2.53 ug/ml

Instrument :
FID_G
ClientSampleId :