

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
 Data File : FG008153.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jun 2021 10:17
 Operator : DD\AJ
 Sample : M2580-15 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 01:45:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5)	N-HEXADECANE	9.918	94844	0.697 ug/ml
7)	N-EICOSANE	12.677	129842	0.949 ug/ml
8)	N-DOCOSANE	13.880	235307	1.734 ug/ml
10)	N-TETRACOSANE	14.985	673149	5.004 ug/ml
11)	N-HEXACOSANE	16.012	368132	2.801 ug/ml
12)	N-OCTACOSANE	16.964	297719	2.297 ug/ml
13)	N-TRIACONTANE	17.852	204542	1.602 ug/ml
14)	N-DOTRIACONTANE	18.688	153117	1.232 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
Data File : FG008153.D
Signal(s) : FID1A.ch
Acq On : 03 Jun 2021 10:17
Operator : DD\AJ
Sample : M2580-15 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 04 01:45:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

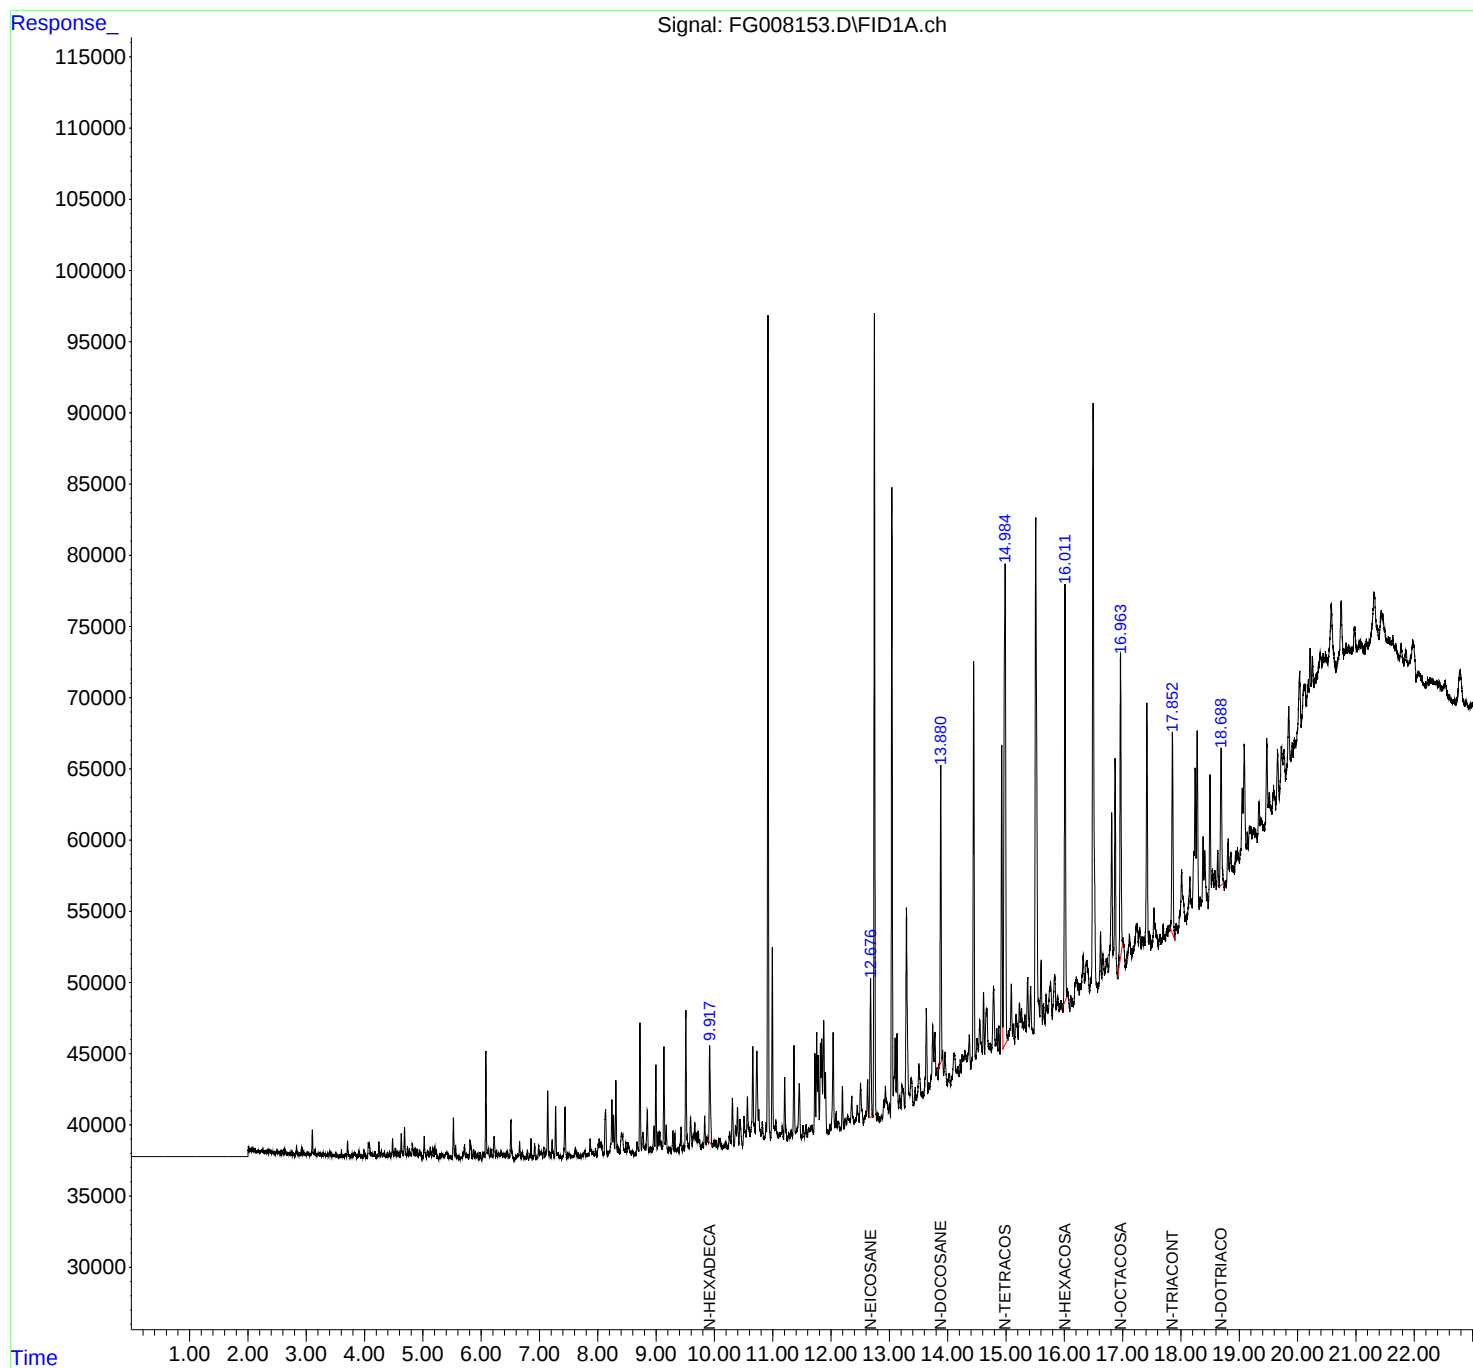


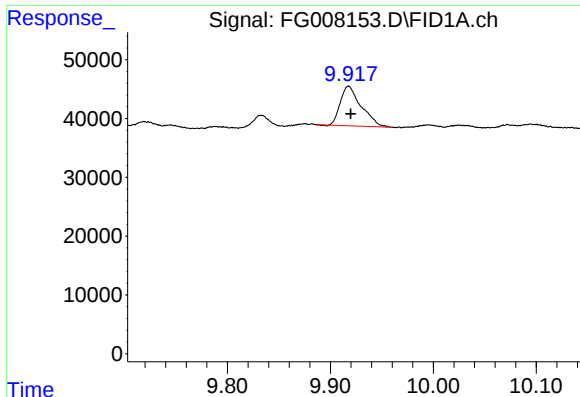

#5 N-HEXADECANE


R.T.: 9.918 min
Delta R.T.: -0.002 min
Response: 94844
Conc: 0.70 ug/ml

Instrument :
FID_G
ClientSampleId :

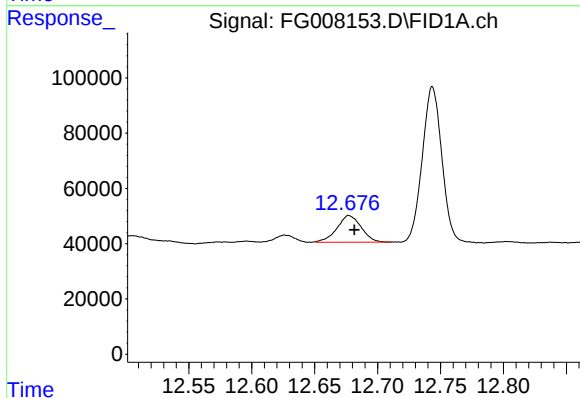


#7 N-EICOSANE

R.T.: 12.677 min
Delta R.T.: -0.004 min
Response: 129842
Conc: 0.95 ug/ml

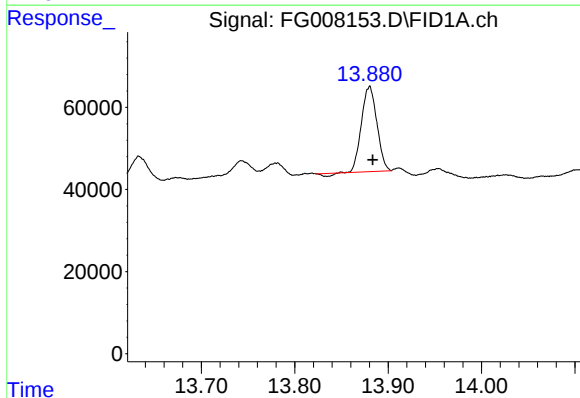


#8 N-DOCOSANE

R.T.: 13.880 min
Delta R.T.: -0.003 min
Response: 235307
Conc: 1.73 ug/ml

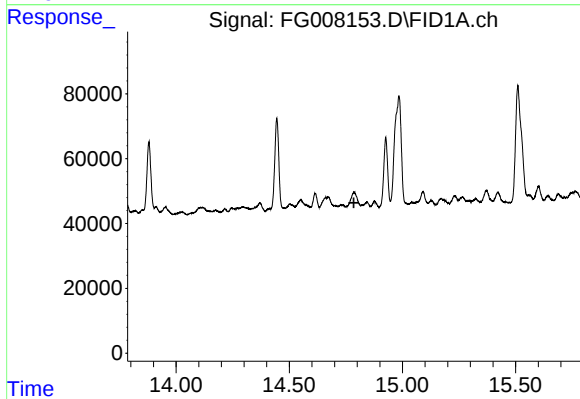

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.786 min
Response: 0
Conc: N.D.

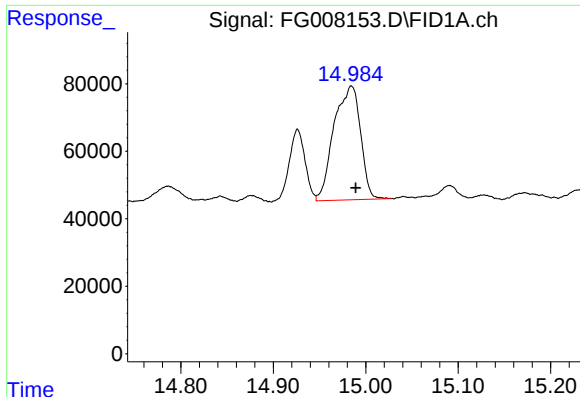

#10 N-TETRACOSANE


R.T.: 14.985 min
Delta R.T.: -0.005 min
Response: 673149
Conc: 5.00 ug/ml

Instrument :
FID_G
ClientSampleId :

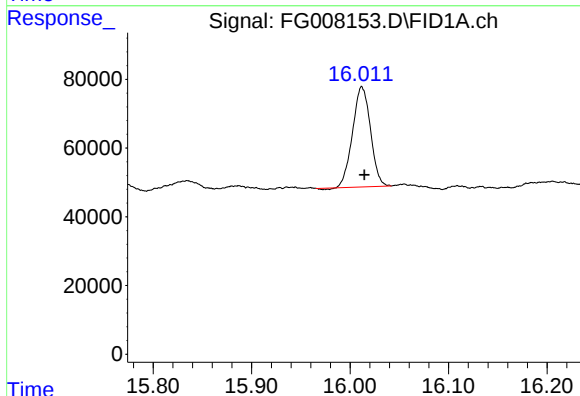


#11 N-HEXACOSANE

R.T.: 16.012 min
Delta R.T.: -0.003 min
Response: 368132
Conc: 2.80 ug/ml

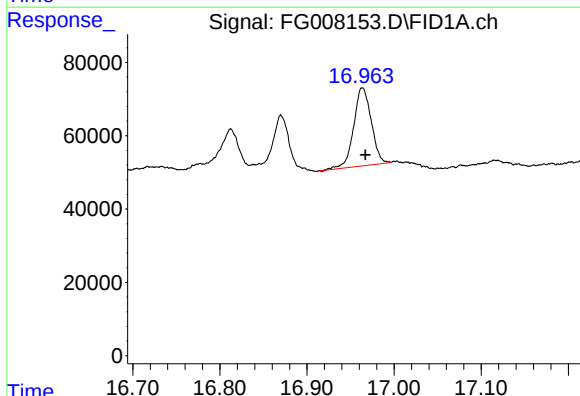


#12 N-OCTACOSANE

R.T.: 16.964 min
Delta R.T.: -0.004 min
Response: 297719
Conc: 2.30 ug/ml

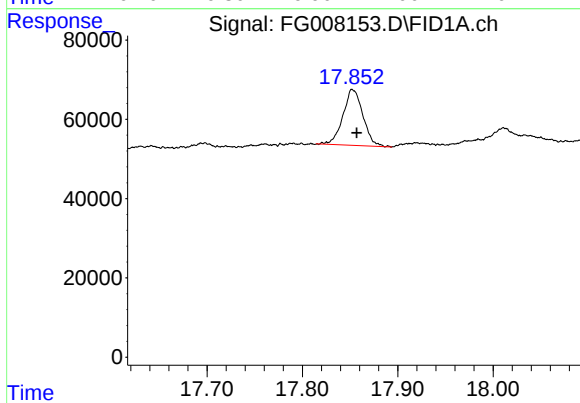

#13 N-TRIACONTANE

R.T.: 17.852 min
Delta R.T.: -0.004 min
Response: 204542
Conc: 1.60 ug/ml

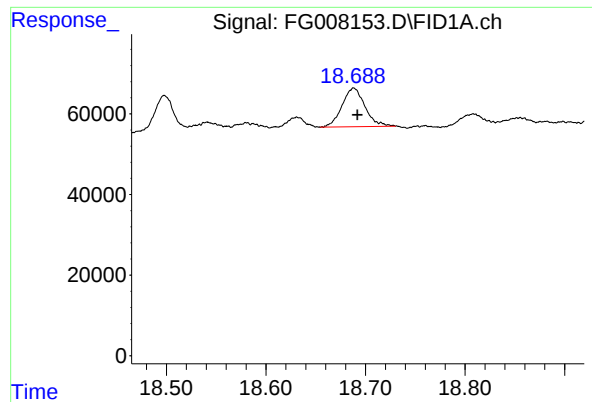

#14 N-DOTRIACONTANE

R.T.: 18.688 min
Delta R.T.: -0.004 min
Response: 153117
Conc: 1.23 ug/ml

Instrument :
FID_G
ClientSampleId :