

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
Data File : FG008154.D
Signal(s) : FID1A.ch
Acq On : 03 Jun 2021 10:48
Operator : DD\AJ
Sample : M2580-09 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 01:45:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	167673	1.413 ug/ml
Target Compounds			
7) N-EICOSANE	12.629f	97275	0.711 ug/ml
8) N-DOCOSANE	13.913	177329	1.306 ug/ml
10) N-TETRACOSANE	14.969	459629	3.417 ug/ml
12) N-OCTACOSANE	16.971	127493	0.984 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
Data File : FG008154.D
Signal(s) : FID1A.ch
Acq On : 03 Jun 2021 10:48
Operator : DD\AJ
Sample : M2580-09 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 01:45:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

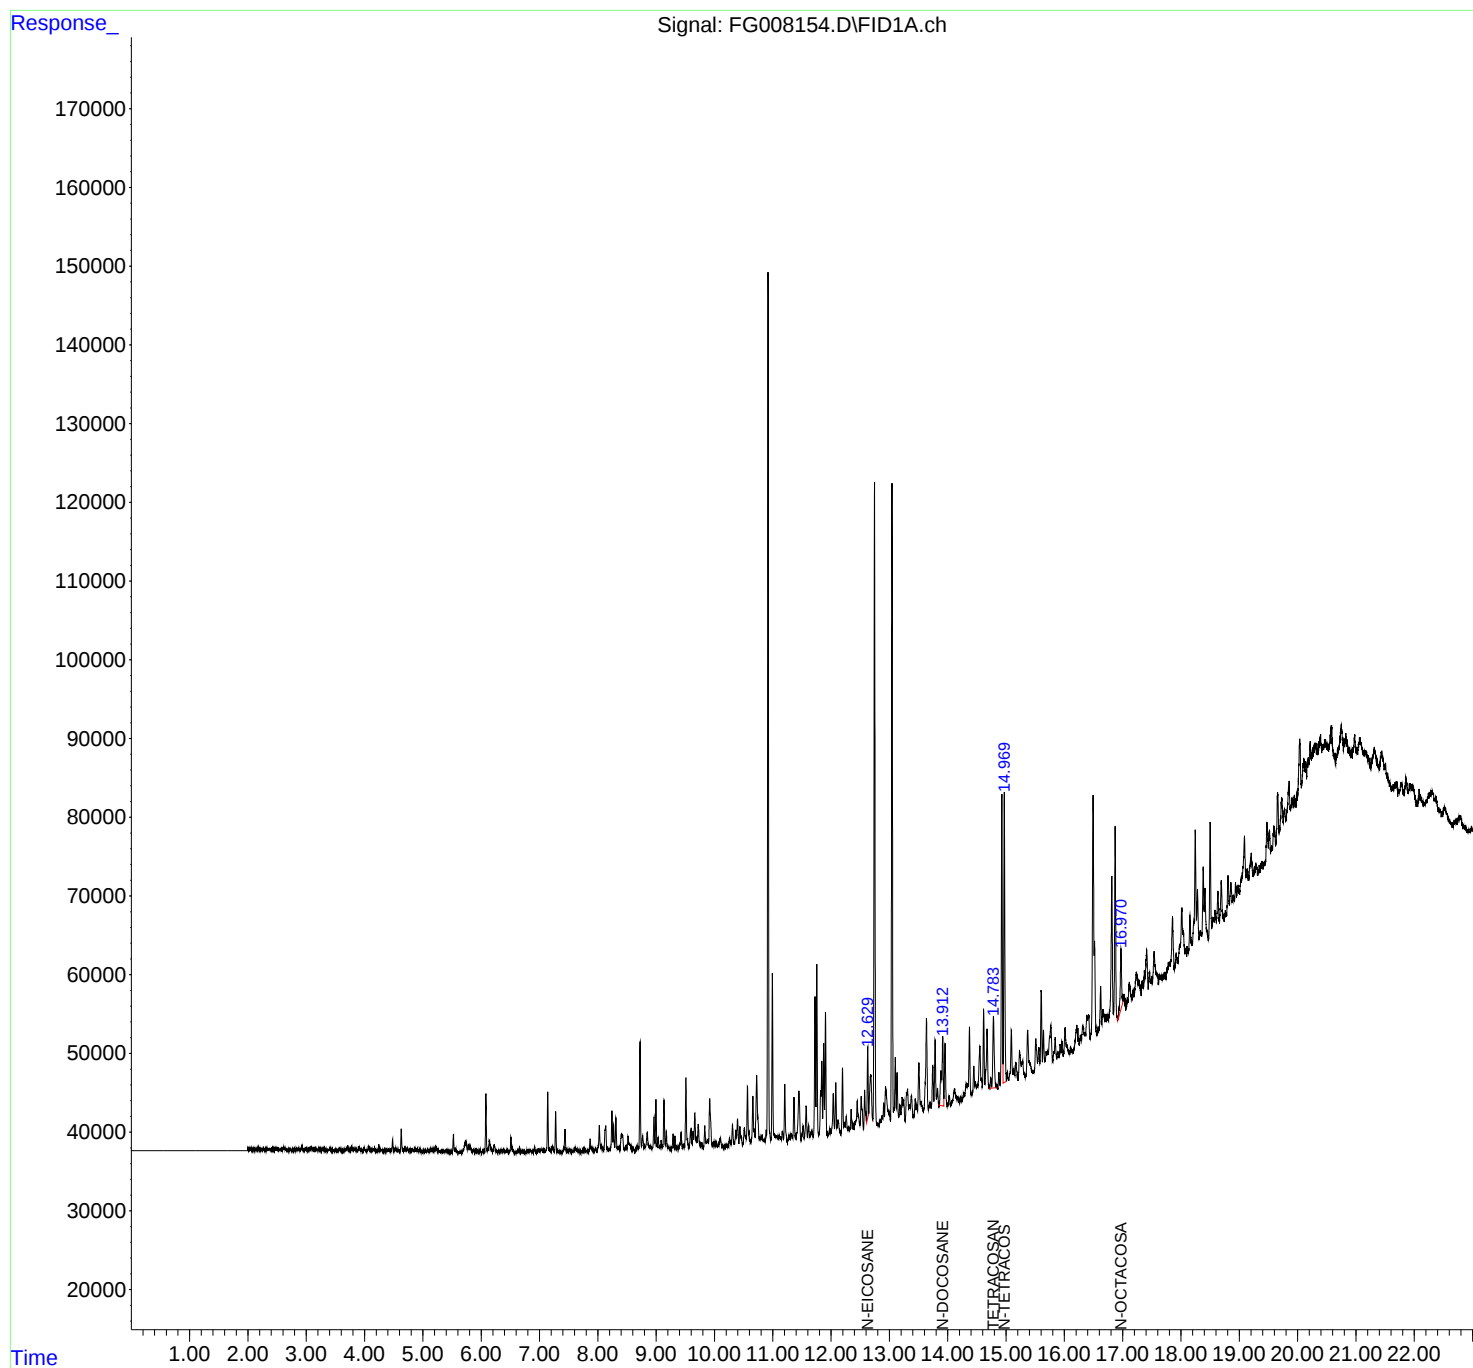


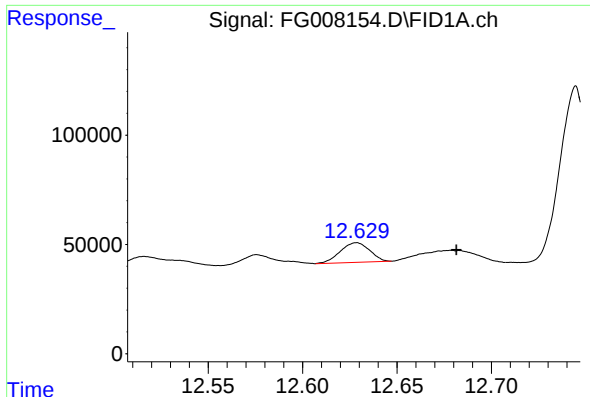

#7 N-EICOSANE


R.T.: 12.629 min
Delta R.T.: -0.053 min
Response: 97275
Conc: 0.71 ug/ml

Instrument :
FID_G
ClientSampleId :

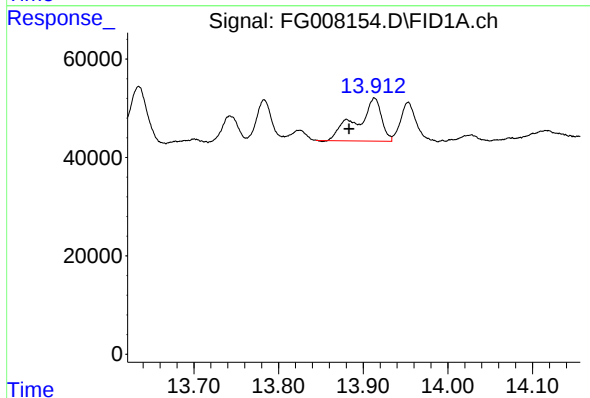


#8 N-DOCOSANE

R.T.: 13.913 min
Delta R.T.: 0.030 min
Response: 177329
Conc: 1.31 ug/ml

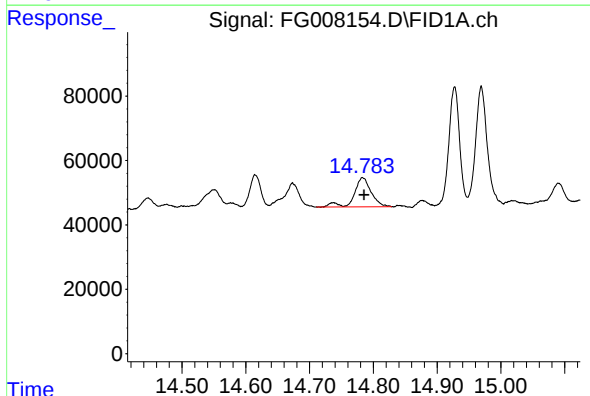


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.002 min
Response: 167673
Conc: 1.41 ug/ml

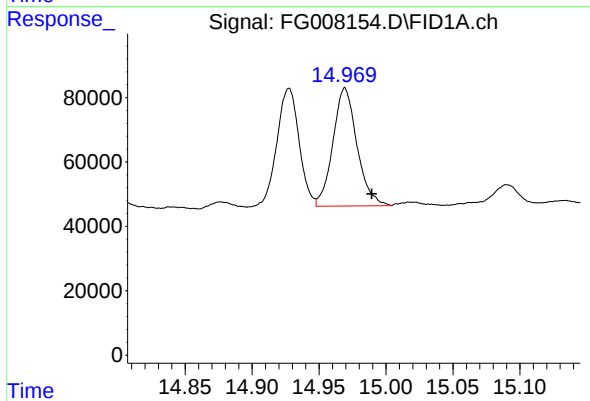

#10 N-TETRACOSANE

R.T.: 14.969 min
Delta R.T.: -0.020 min
Response: 459629
Conc: 3.42 ug/ml

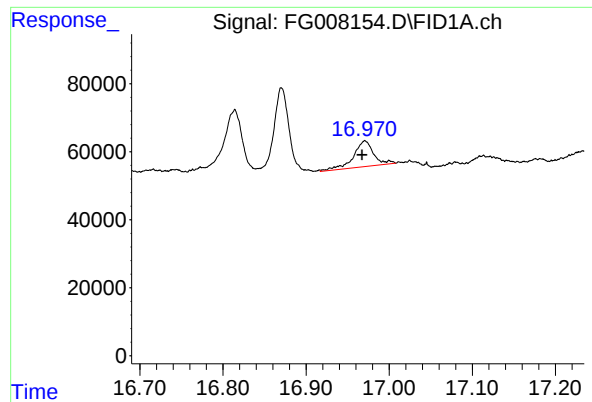

#12 N-OCTACOSANE

R.T.: 16.971 min
Delta R.T.: 0.004 min
Response: 127493
Conc: 0.98 ug/ml

Instrument :
FID_G
ClientSampleId :