

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
 Data File : FG008160.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jun 2021 14:09
 Operator : DD\AJ
 Sample : M2580-08 30X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 01:46:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.747f	393514	2.875 ug/ml
10) N-TETRACOSANE	14.973	205637	1.529 ug/ml
12) N-OCTACOSANE	16.970	83196	0.642 ug/ml
13) N-TRIACONTANE	17.858	274184	2.148 ug/ml
14) N-DOTRIACONTANE	18.694	201650	1.623 ug/ml
15) N-TETRATRIACONTANE	19.478	175433	1.500 ug/ml
16) N-HEXATRIACONTANE	20.219	246606	2.227 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060321\
Data File : FG008160.D
Signal(s) : FID1A.ch
Acq On : 03 Jun 2021 14:09
Operator : DD\AJ
Sample : M2580-08 30X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 04 01:46:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

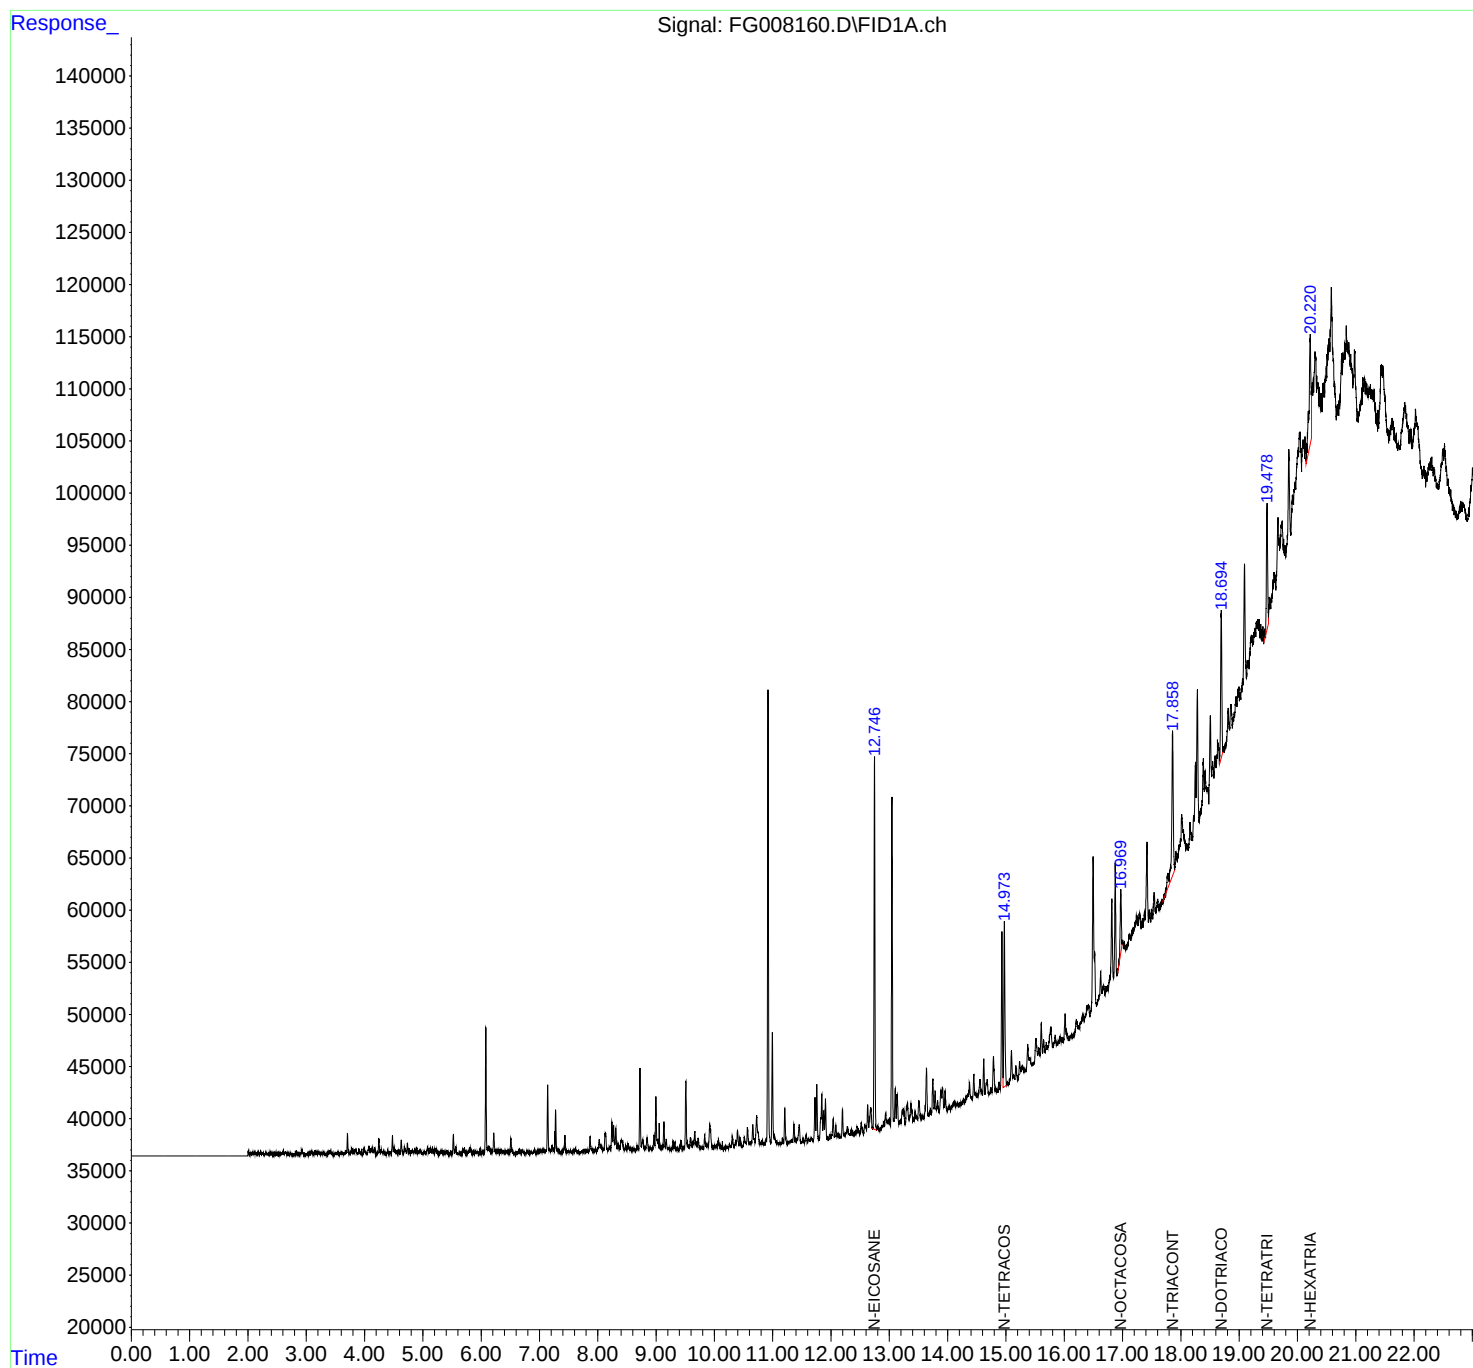


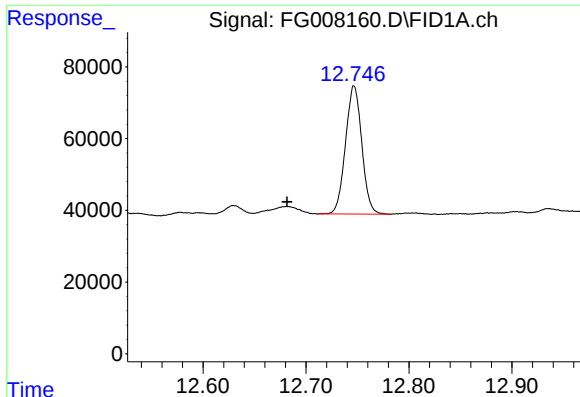

#7 N-EICOSANE


R.T.: 12.747 min
Delta R.T.: 0.065 min
Response: 393514
Conc: 2.88 ug/ml

Instrument :
FID_G
ClientSampleId :

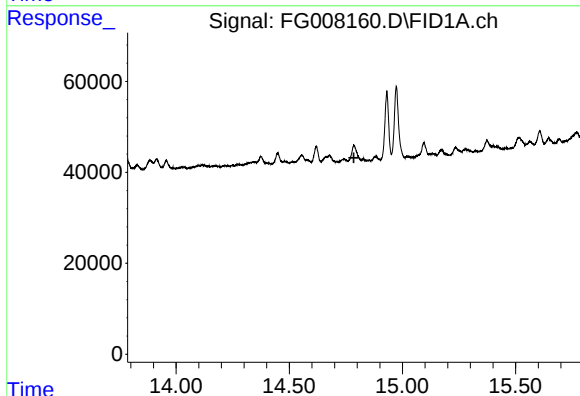


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

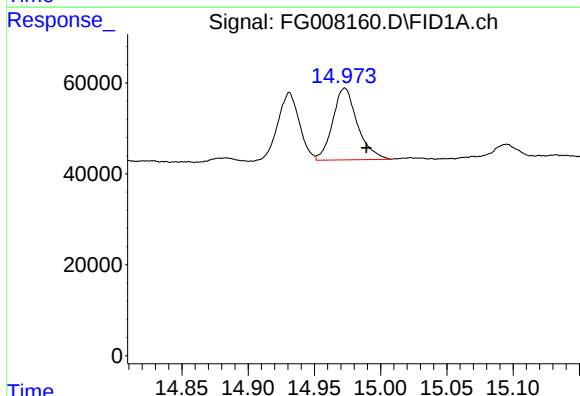


#10 N-TETRACOSANE

R.T.: 14.973 min
Delta R.T.: -0.016 min
Response: 205637
Conc: 1.53 ug/ml

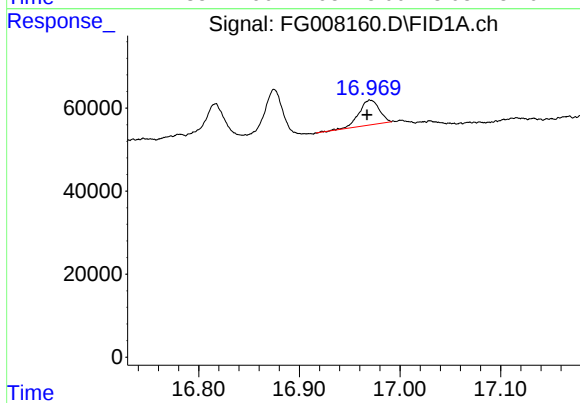

#12 N-OCTACOSANE


R.T.: 16.970 min
Delta R.T.: 0.003 min
Response: 83196
Conc: 0.64 ug/ml

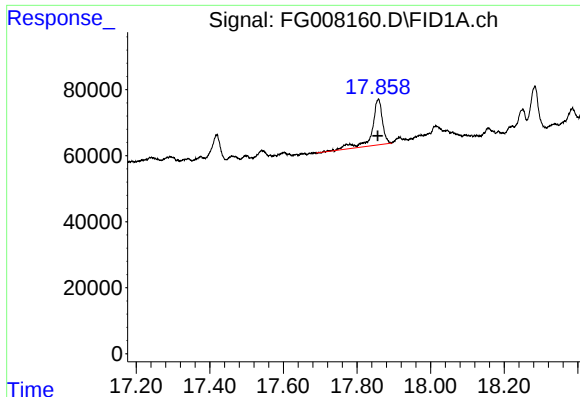

#13 N-TRIACONTANE


R.T.: 17.858 min
Delta R.T.: 0.001 min
Response: 274184
Conc: 2.15 ug/ml

Instrument :
FID_G
ClientSampleId :

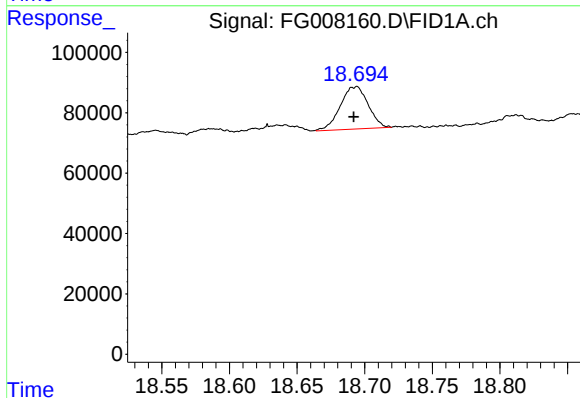


#14 N-DOTRIACONTANE

R.T.: 18.694 min
Delta R.T.: 0.002 min
Response: 201650
Conc: 1.62 ug/ml

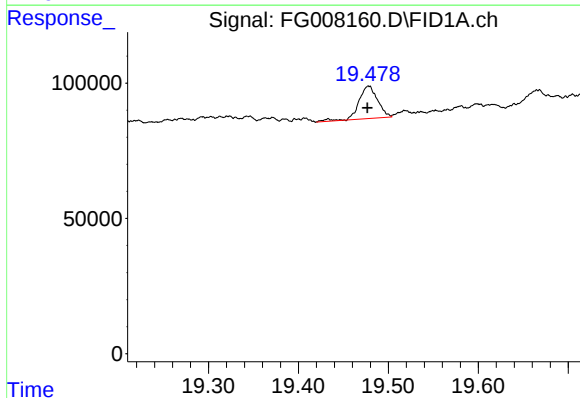

#15 N-TETRATRIACONTANE

R.T.: 19.478 min
Delta R.T.: 0.001 min
Response: 175433
Conc: 1.50 ug/ml

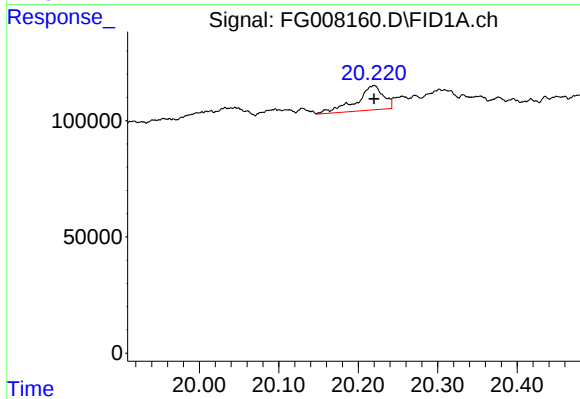

#16 N-HEXATRIACONTANE

R.T.: 20.219 min
Delta R.T.: 0.000 min
Response: 246606
Conc: 2.23 ug/ml