

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060421\
Data File : FG008168.D
Signal(s) : FID1A.ch
Acq On : 04 Jun 2021 10:55
Operator : DD\AJ
Sample : M2589-02 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:47:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.741f	243357	1.778 ug/ml
10) N-TETRACOSANE	14.968	154854	1.151 ug/ml
13) N-TRIACONTANE	17.859	183679	1.439 ug/ml
15) N-TETRATRIACONTANE	19.516	94687	0.809 ug/ml
16) N-HEXATRIACONTANE	20.221	76320	0.689 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060421\
Data File : FG008168.D
Signal(s) : FID1A.ch
Acq On : 04 Jun 2021 10:55
Operator : DD\AJ
Sample : M2589-02 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:47:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

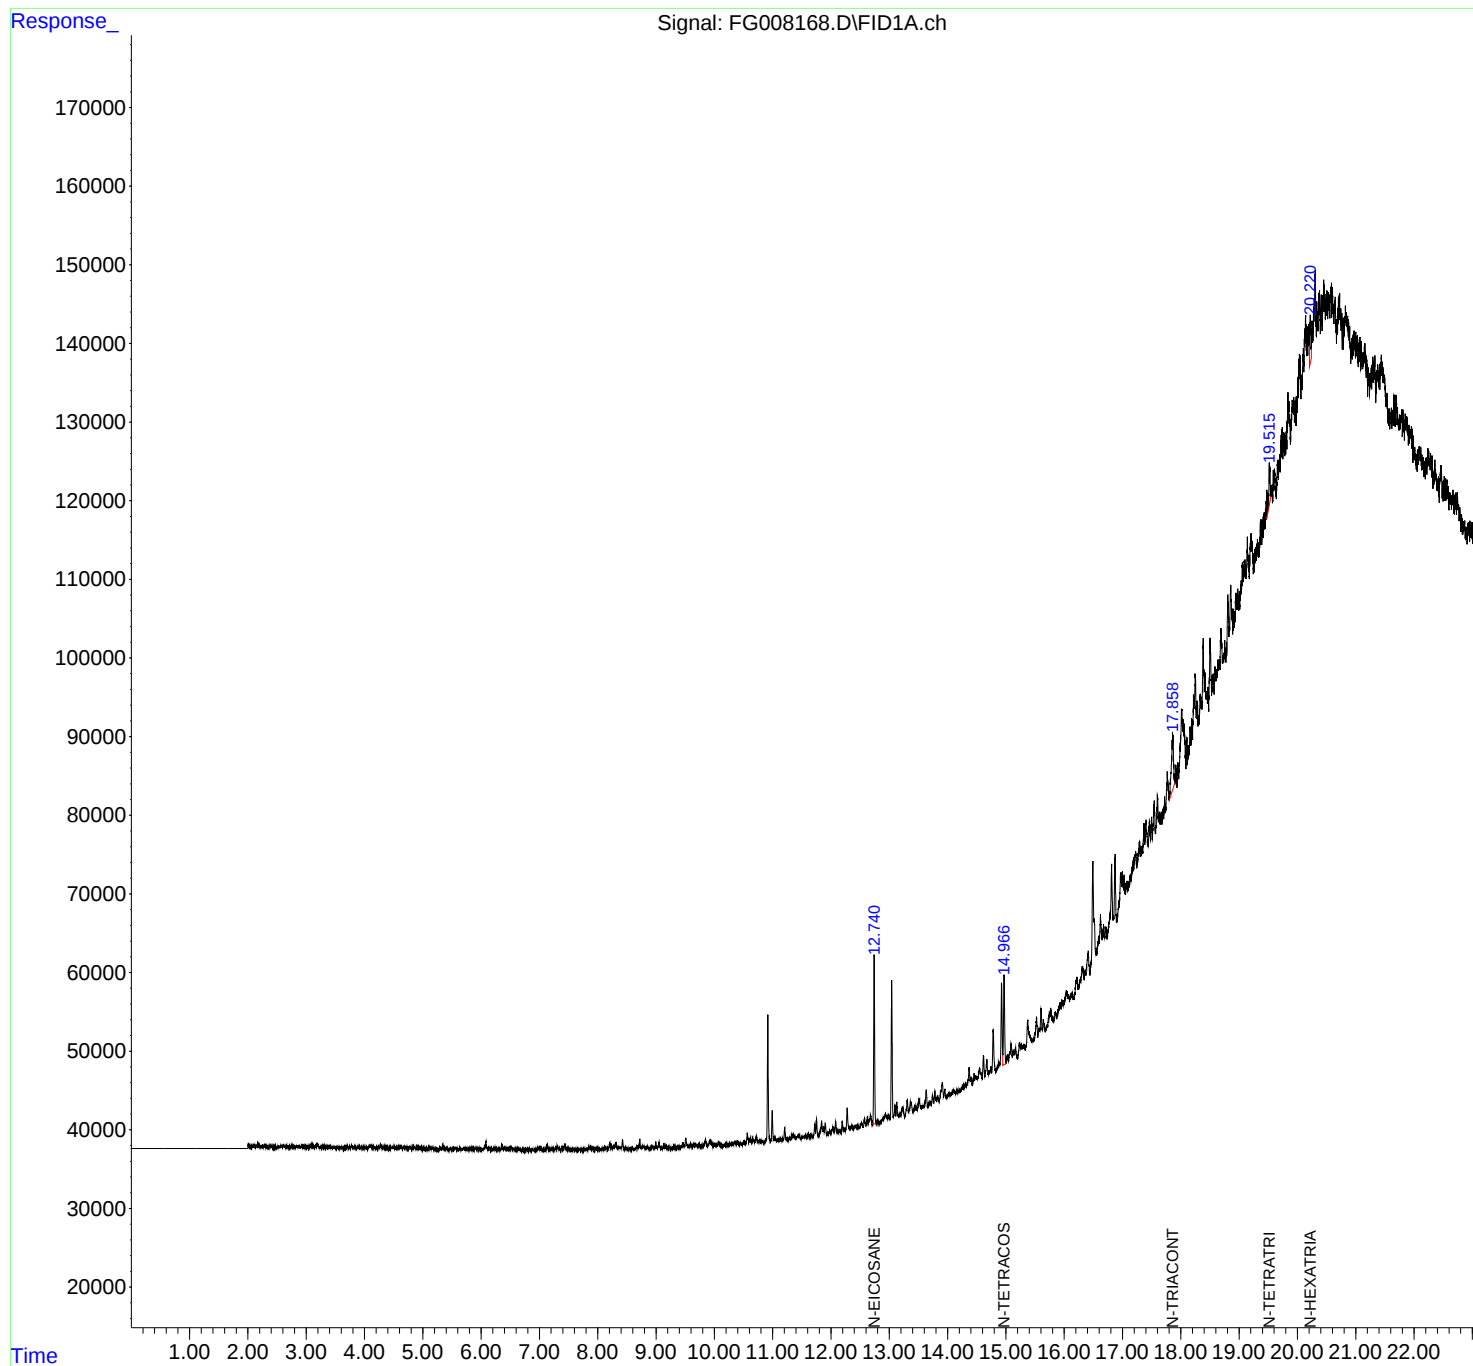


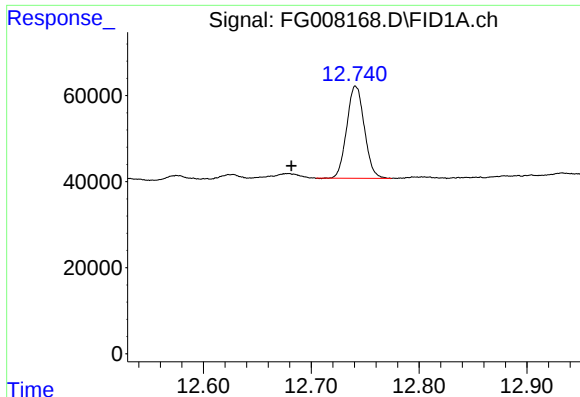

#7 N-EICOSANE


R.T.: 12.741 min
Delta R.T.: 0.060 min
Response: 243357
Conc: 1.78 ug/ml

Instrument :
FID_G
ClientSampleId :

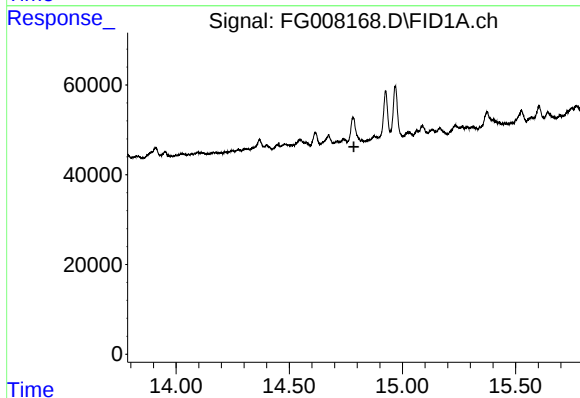


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

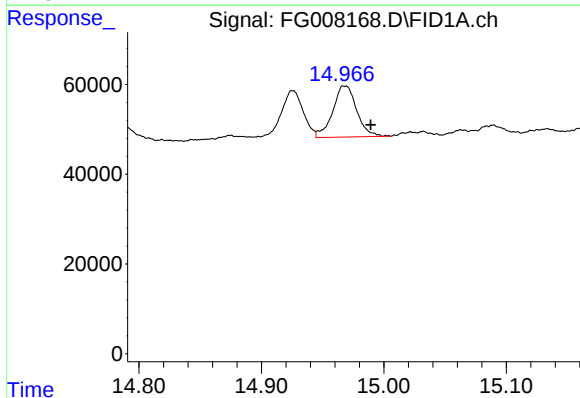


#10 N-TETRACOSANE

R.T.: 14.968 min
Delta R.T.: -0.021 min
Response: 154854
Conc: 1.15 ug/ml

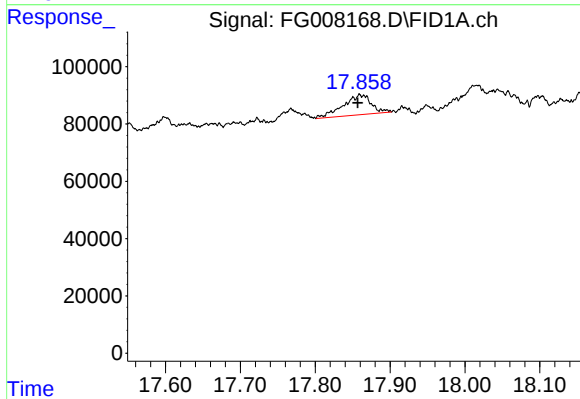

#13 N-TRIACONTANE


R.T.: 17.859 min
Delta R.T.: 0.002 min
Response: 183679
Conc: 1.44 ug/ml

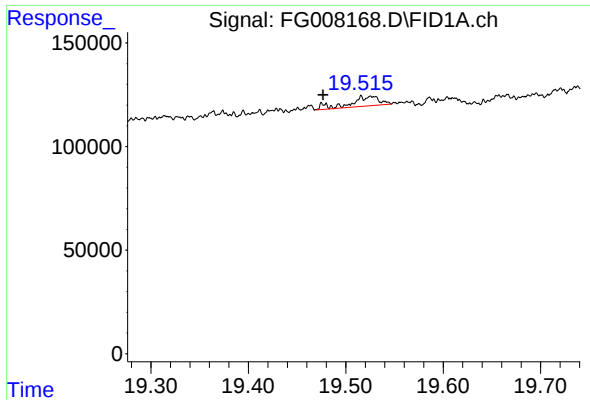

#15 N-TETRATRIACONTANE

R.T.: 19.516 min
Delta R.T.: 0.039 min
Response: 94687
Conc: 0.81 ug/ml

Instrument :
FID_G
ClientSampleId :

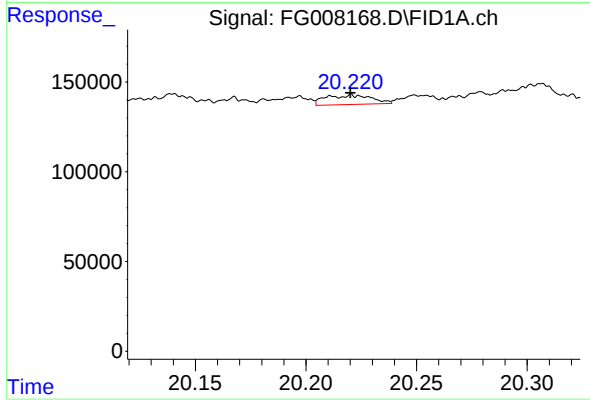

#16 N-HEXATRIACONTANE

R.T.: 20.221 min
Delta R.T.: 0.000 min
Response: 76320
Conc: 0.69 ug/ml