

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060421\
 Data File : FG008175.D
 Signal(s) : FID1A.ch
 Acq On : 04 Jun 2021 15:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:48:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.787	2056197	17.326 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.691	707209	5.691 ug/ml
16) N-HEXATRIACONTANE	20.220	253291	2.287 ug/ml
18) N-TETRACONTANE	21.969	124697	1.162 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060421\
Data File : FG008175.D
Signal(s) : FID1A.ch
Acq On : 04 Jun 2021 15:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 05 00:48:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

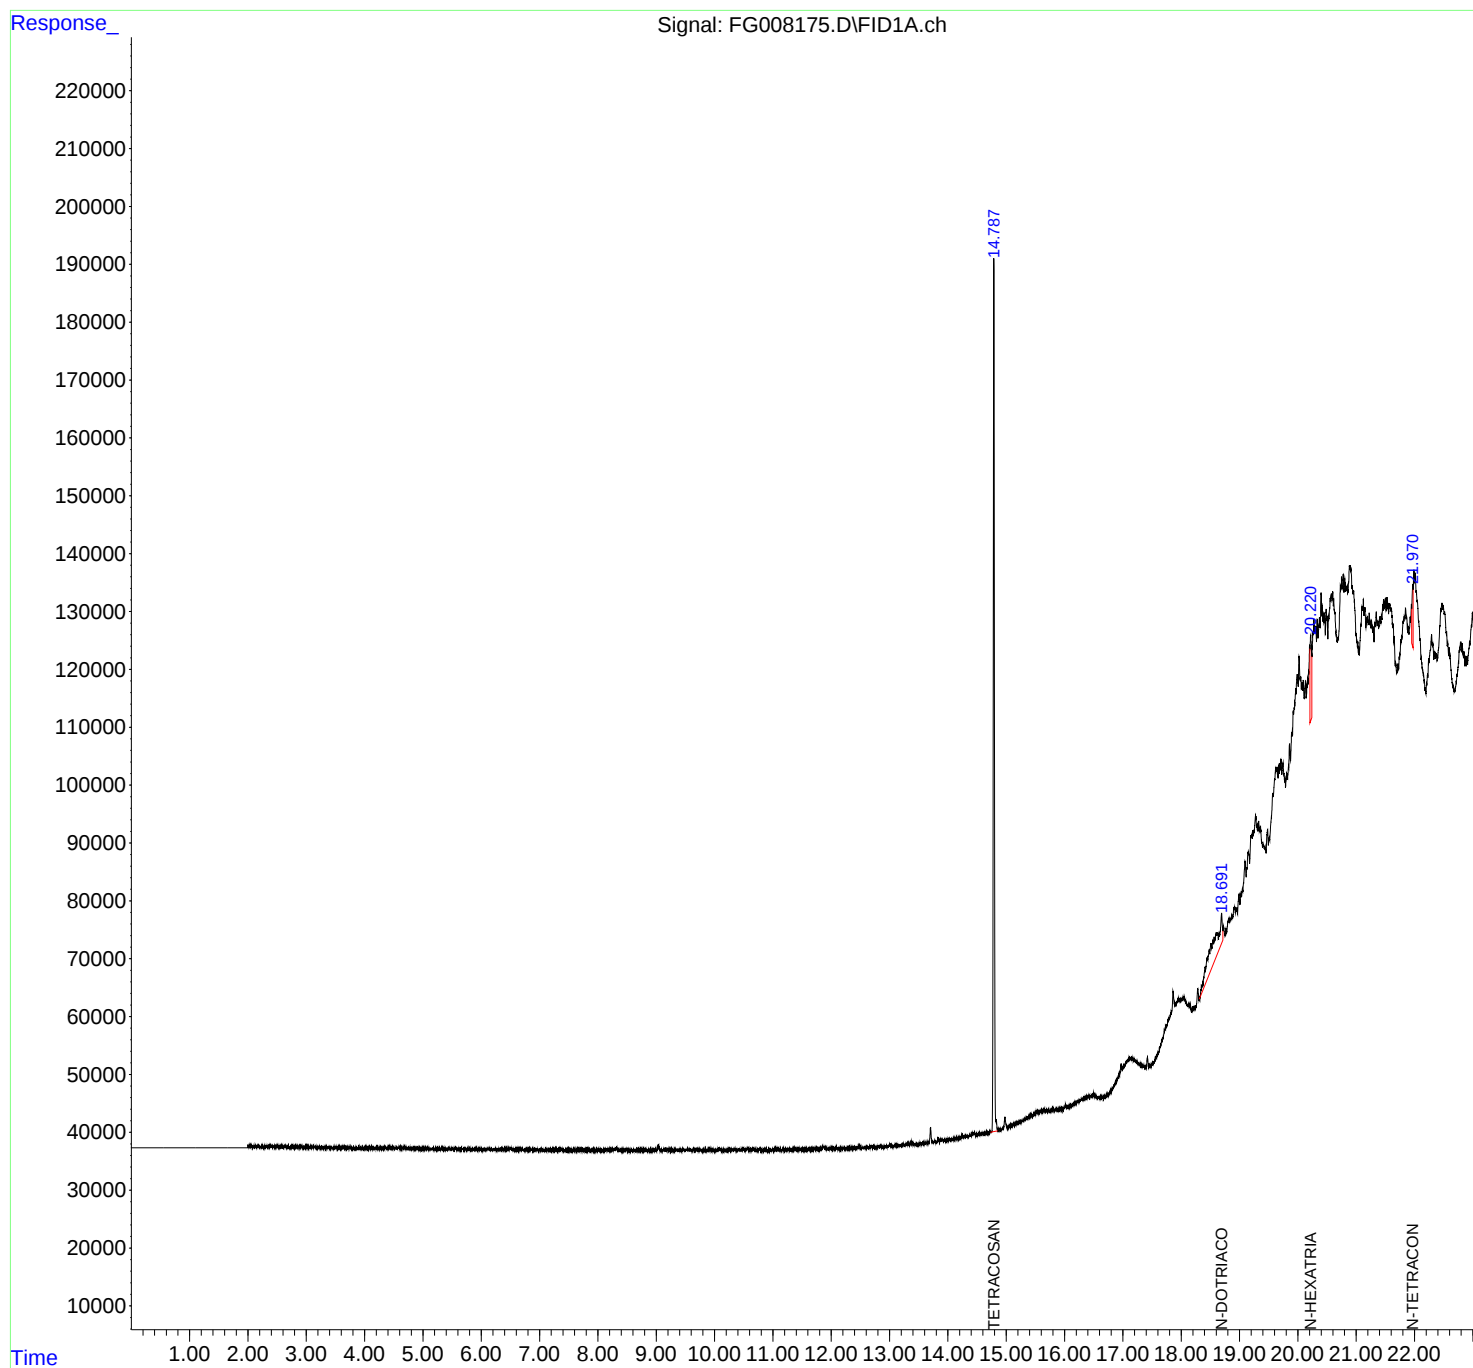


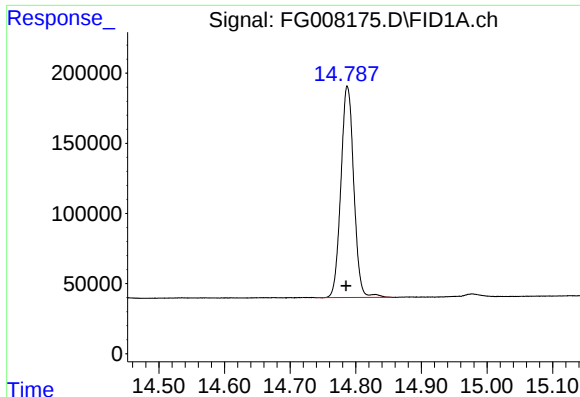

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.787 min
Delta R.T.: 0.002 min
Response: 2056197
Conc: 17.33 ug/ml

Instrument :
FID_G
ClientSampleId :

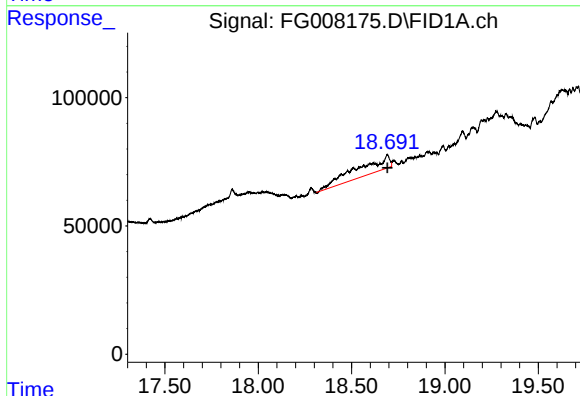


#14 N-DOTRIACONTANE

R.T.: 18.691 min
Delta R.T.: 0.000 min
Response: 707209
Conc: 5.69 ug/ml

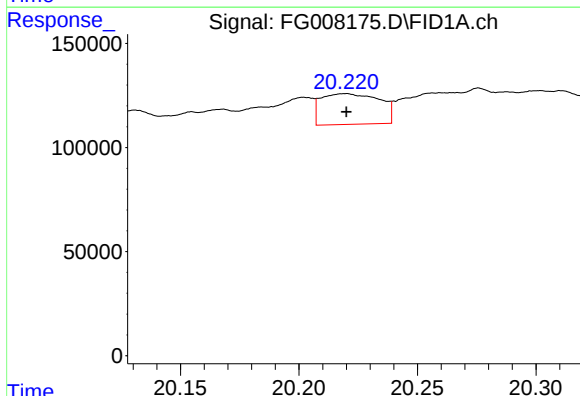

#16 N-HEXATRIACONTANE

R.T.: 20.220 min
Delta R.T.: 0.000 min
Response: 253291
Conc: 2.29 ug/ml

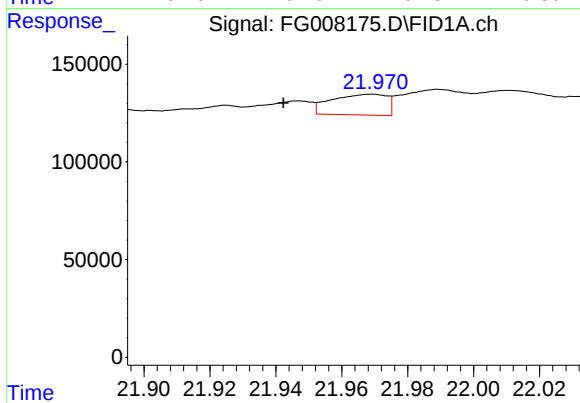

#18 N-TETRACONTANE

R.T.: 21.969 min
Delta R.T.: 0.027 min
Response: 124697
Conc: 1.16 ug/ml