

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060421\
Data File : FG008178.D
Signal(s) : FID1A.ch
Acq On : 04 Jun 2021 16:41
Operator : DD\AJ
Sample : M2589-03 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:49:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.748f	224540	1.641 ug/ml
10)	N-TETRACOSANE	14.974	130598	0.971 ug/ml
13)	N-TRIACONTANE	17.861	95710	0.750 ug/ml
14)	N-DOTRIACONTANE	18.694	112876	0.908 ug/ml
15)	N-TETRATRIACONTANE	19.480	47655	0.407 ug/ml
16)	N-HEXATRIACONTANE	20.219	109385	0.988 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060421\
Data File : FG008178.D
Signal(s) : FID1A.ch
Acq On : 04 Jun 2021 16:41
Operator : DD\AJ
Sample : M2589-03 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:49:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

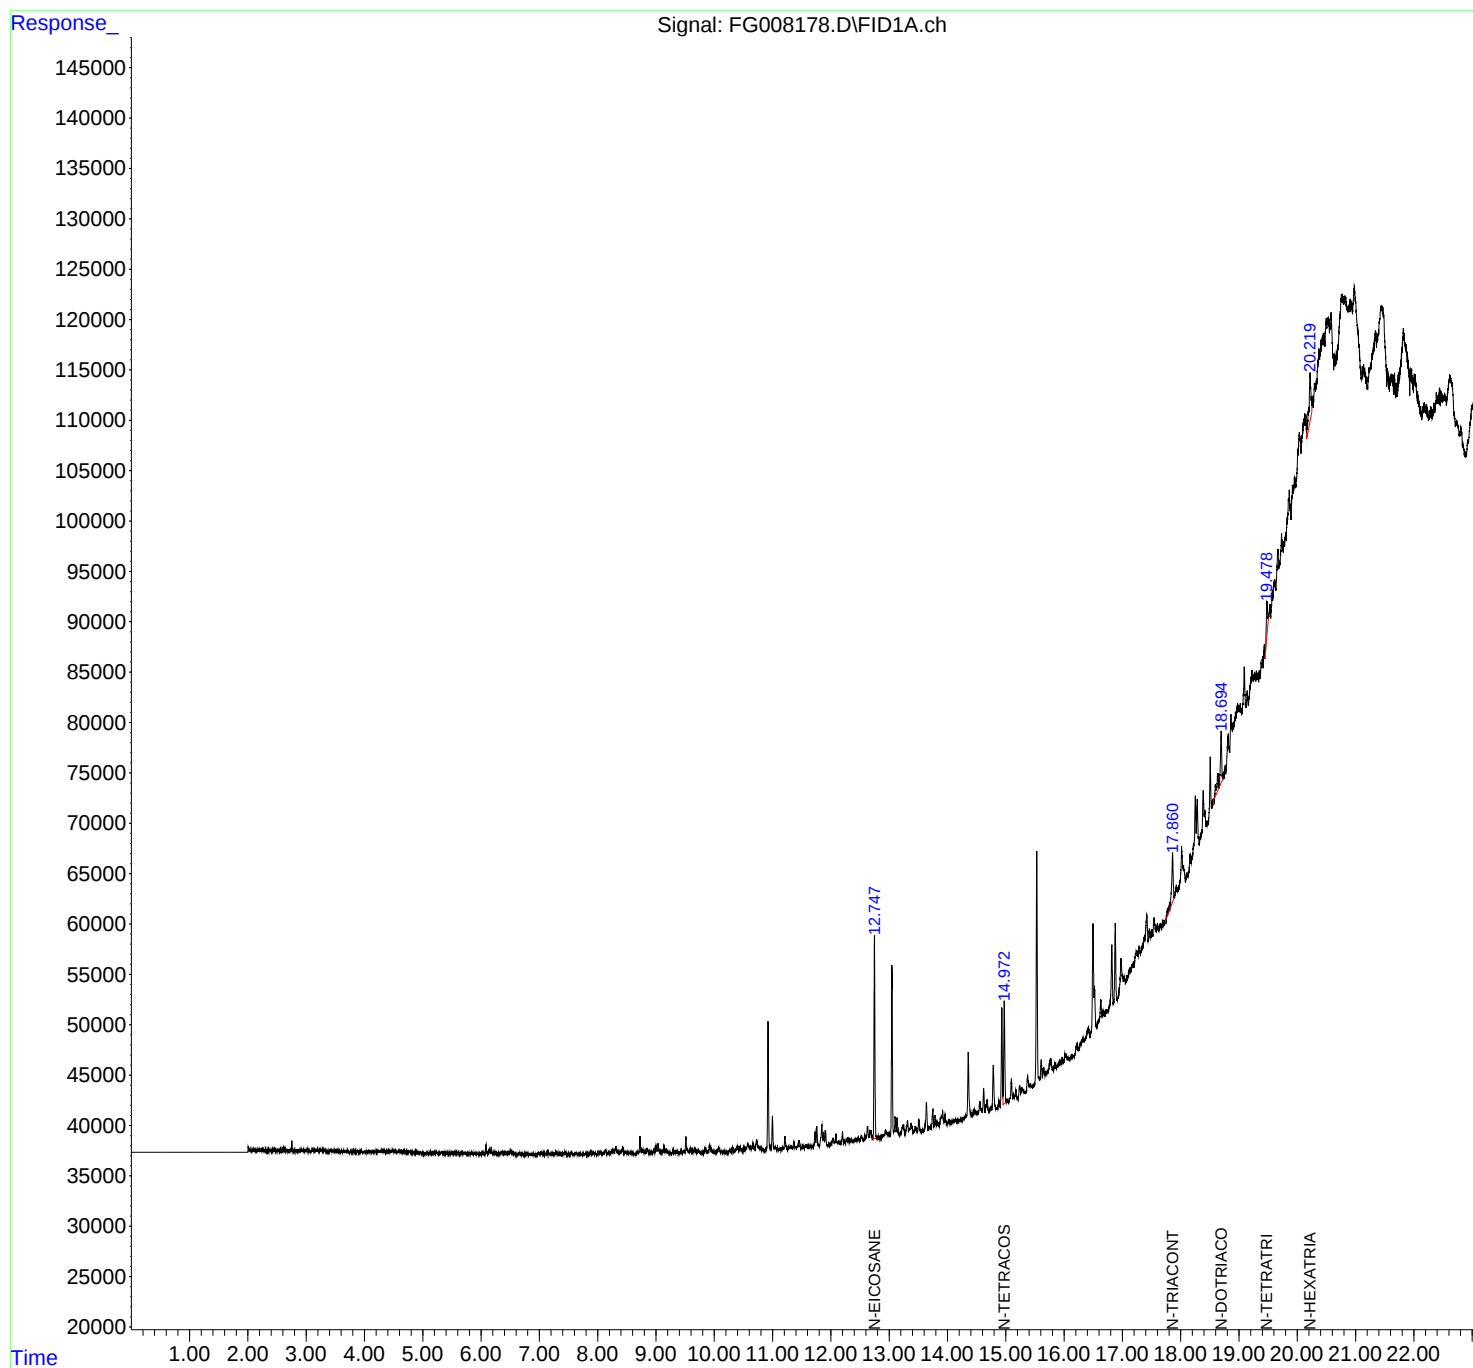


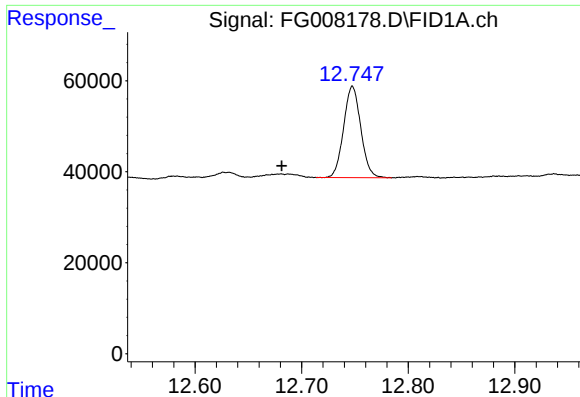

#7 N-EICOSANE


R.T.: 12.748 min
Delta R.T.: 0.066 min
Response: 224540
Conc: 1.64 ug/ml

Instrument :
FID_G
ClientSampleId :

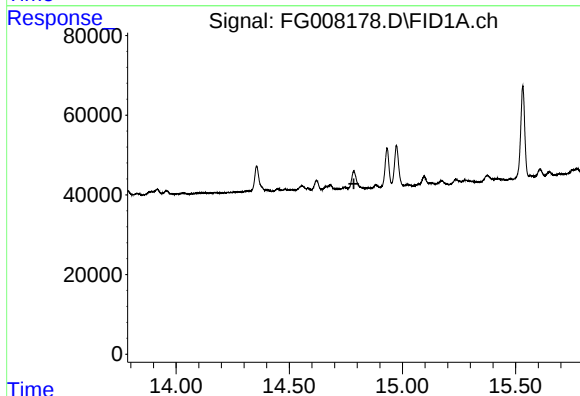


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.786 min
Response: 0
Conc: N.D.

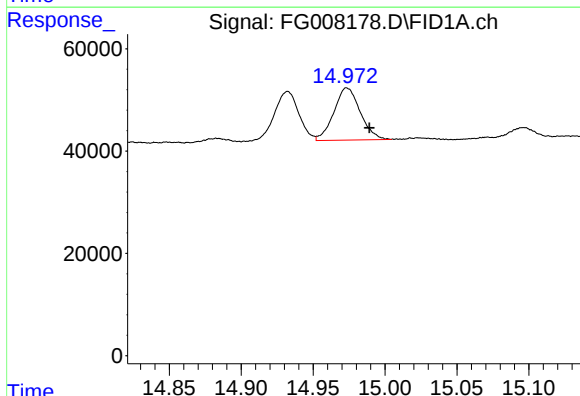


#10 N-TETRACOSANE

R.T.: 14.974 min
Delta R.T.: -0.016 min
Response: 130598
Conc: 0.97 ug/ml

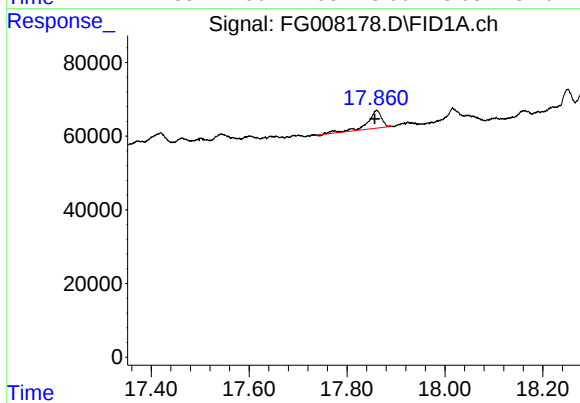

#13 N-TRIACONTANE


R.T.: 17.861 min
Delta R.T.: 0.004 min
Response: 95710
Conc: 0.75 ug/ml

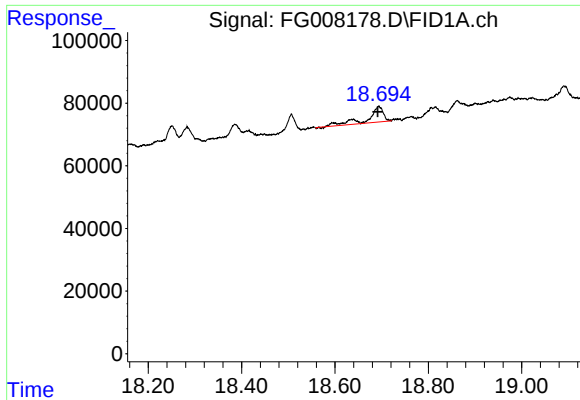

#14 N-DOTRIACONTANE


R.T.: 18.694 min
Delta R.T.: 0.002 min
Response: 112876
Conc: 0.91 ug/ml

Instrument :
FID_G
ClientSampleId :

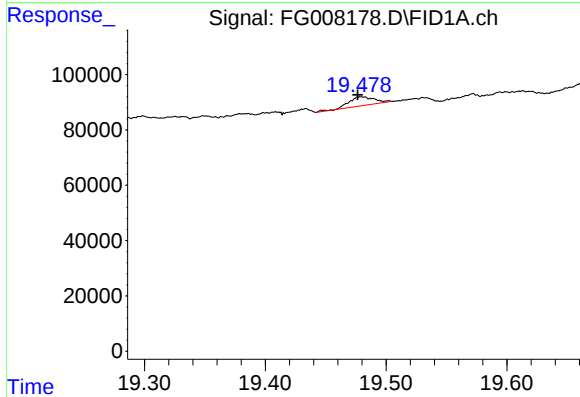

#15 N-TETRATRIACONTANE

R.T.: 19.480 min
Delta R.T.: 0.003 min
Response: 47655
Conc: 0.41 ug/ml

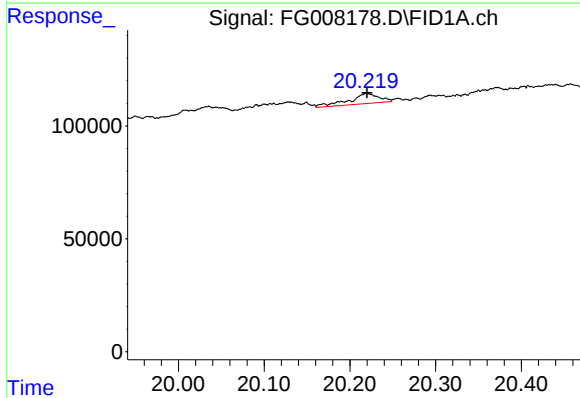

#16 N-HEXATRIACONTANE

R.T.: 20.219 min
Delta R.T.: 0.000 min
Response: 109385
Conc: 0.99 ug/ml