

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG060425\  
Data File : FG015912.D  
Signal(s) : FID1A.ch  
Acq On : 04 Jun 2025 12:48  
Operator : YP\AJ  
Sample : PB168274BL  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
PB168274BL

Integration File: Sample.e  
Quant Time: Jun 05 05:09:46 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052225.M  
Quant Title :  
QLast Update : Thu May 22 06:20:25 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.981 | 1910787  | 15.590 ug/ml |
| Target Compounds              |        |          |              |
| 11) N-HEXACOSANE              | 16.222 | 8862     | 0.065 ug/ml  |
| 12) N-OCTACOSANE              | 17.172 | 91231    | 0.677 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG060425\  
Data File : FG015912.D  
Signal(s) : FID1A.ch  
Acq On : 04 Jun 2025 12:48  
Operator : YP\AJ  
Sample : PB168274BL  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
PB168274BL

Integration File: Sample.e  
Quant Time: Jun 05 05:09:46 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG052225.M  
Quant Title :  
QLast Update : Thu May 22 06:20:25 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

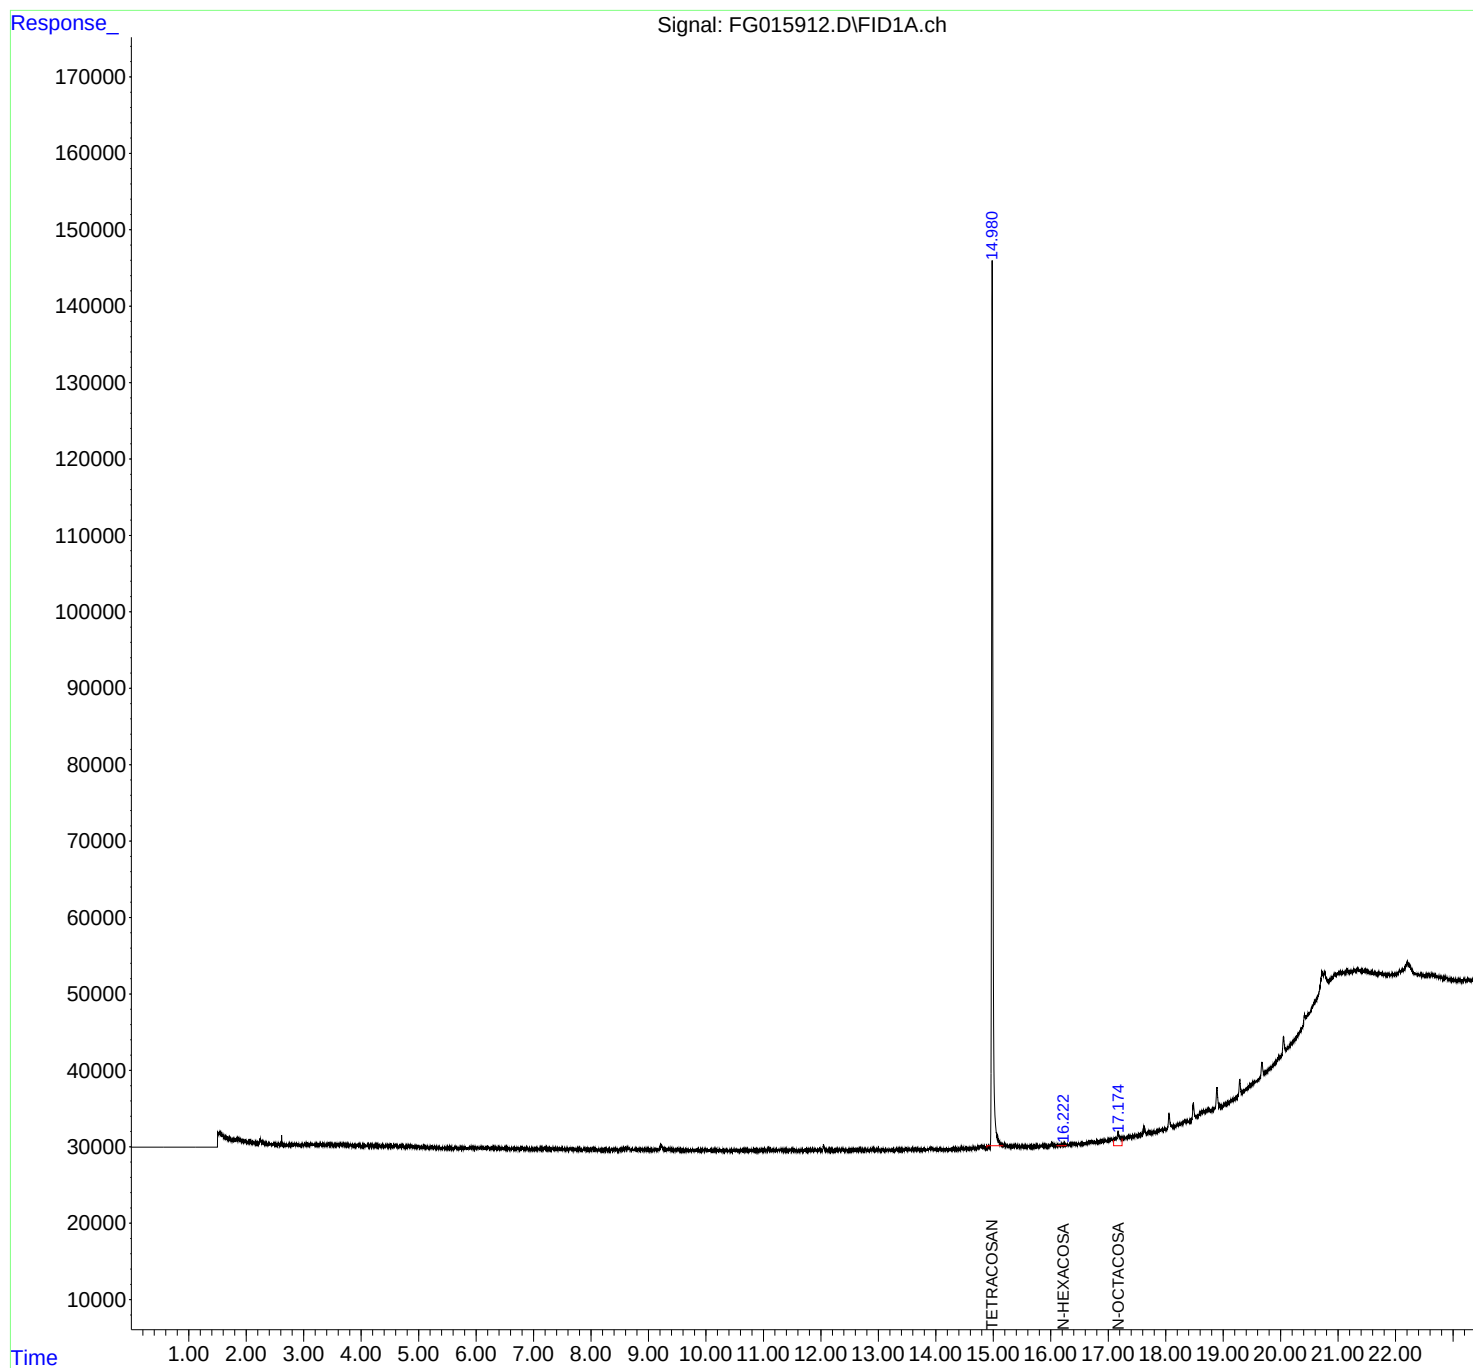


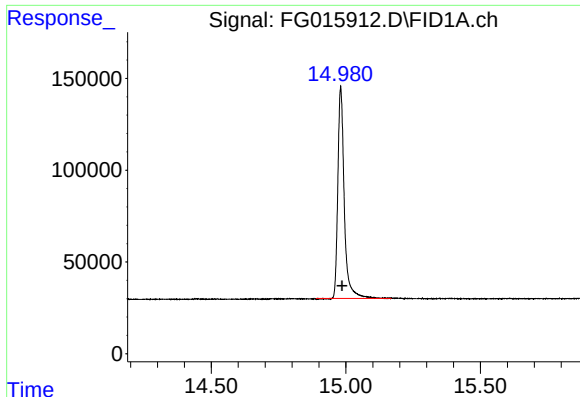

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.981 min  
Delta R.T.: -0.005 min  
Response: 1910787  
Conc: 15.59 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
PB168274BL

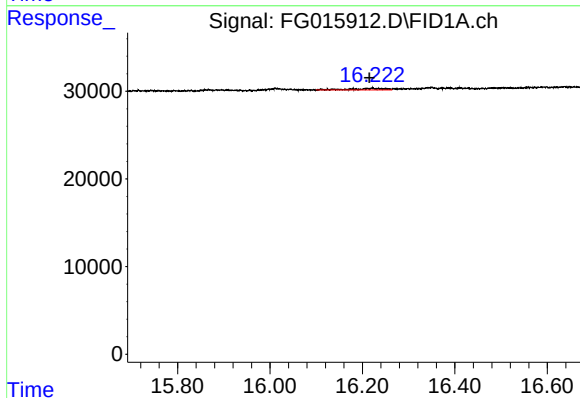

#11 N-HEXACOSANE

R.T.: 16.222 min  
Delta R.T.: 0.007 min  
Response: 8862  
Conc: 0.07 ug/ml

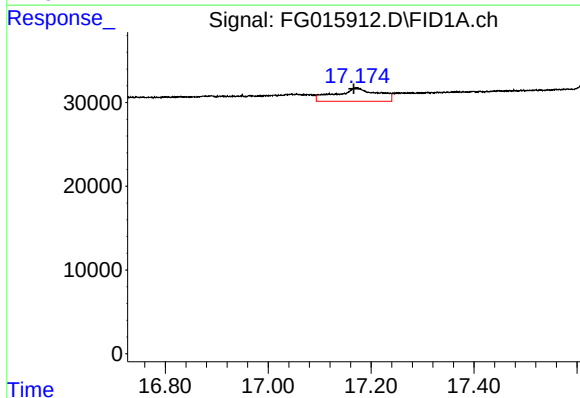

#12 N-OCTACOSANE

R.T.: 17.172 min  
Delta R.T.: 0.006 min  
Response: 91231  
Conc: 0.68 ug/ml