

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060425\
 Data File : FG015924.D
 Signal(s) : FID1A.ch
 Acq On : 04 Jun 2025 19:16
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Jun 05 05:12:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052225.M
 Quant Title :
 QLast Update : Thu May 22 06:20:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.986	5769617	47.075 ug/ml
Target Compounds			
2) N-DECANE	4.486	6104301	51.952 ug/ml
3) N-DODECANE	6.669	6274174	51.694 ug/ml
4) N-TETRADECANE	8.506	6426661	50.330 ug/ml
5) N-HEXADECANE	10.119	6488013	48.698 ug/ml
6) N-OCTADECANE	11.568	6633650	48.068 ug/ml
7) N-EICOSANE	12.882	6706560	47.471 ug/ml
8) N-DOCOSANE	14.085	6511288	47.401 ug/ml
10) N-TETRACOSANE	15.191	6567275	47.772 ug/ml
11) N-HEXACOSANE	16.215	6554402	48.241 ug/ml
12) N-OCTACOSANE	17.168	6597278	48.932 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060425\
Data File : FG015924.D
Signal(s) : FID1A.ch
Acq On : 04 Jun 2025 19:16
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Jun 05 05:12:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052225.M
Quant Title :
QLast Update : Thu May 22 06:20:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

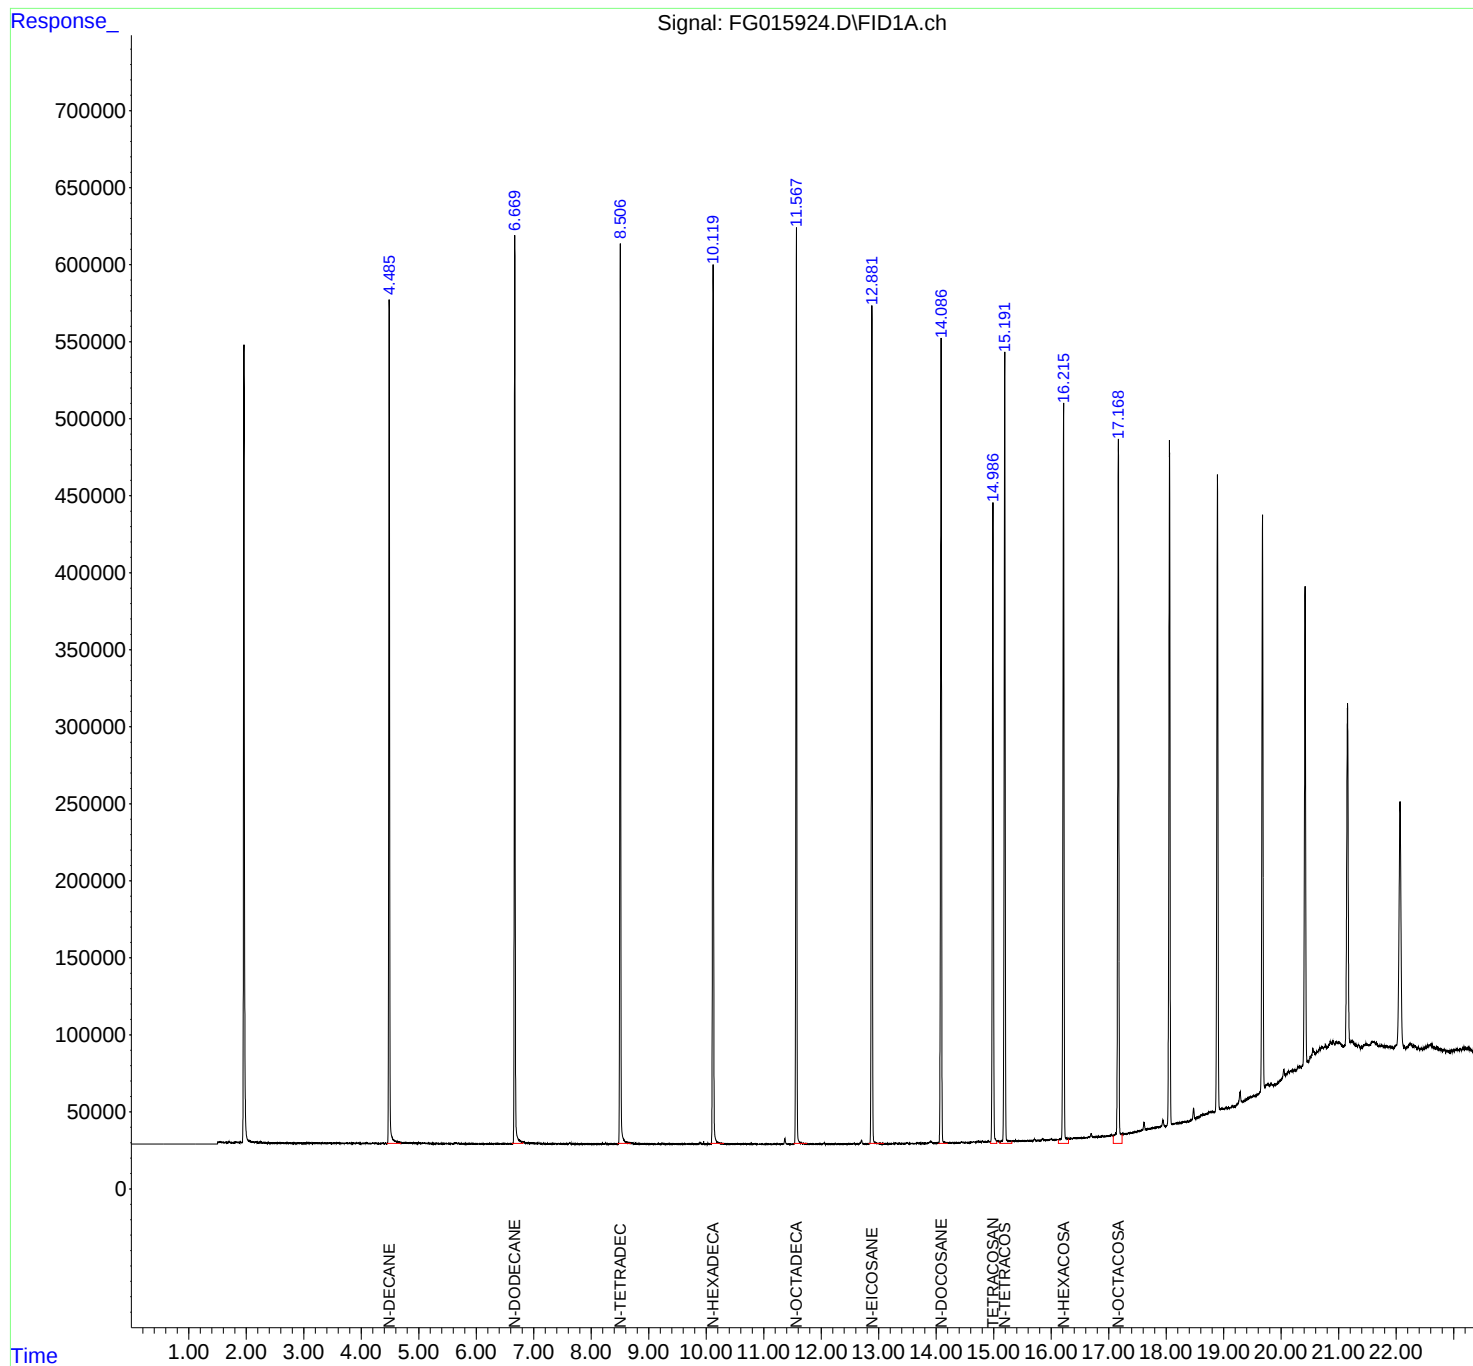


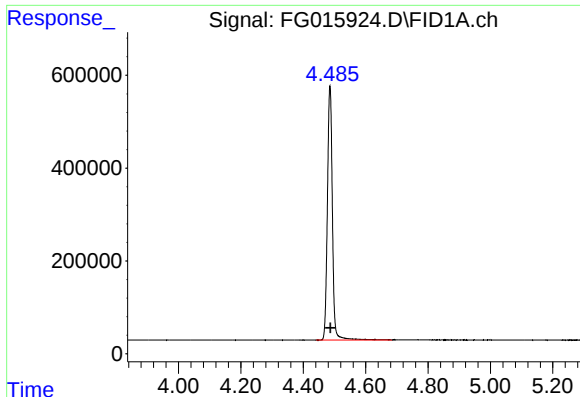

#2 N-DECANE


R.T.: 4.486 min
Delta R.T.: -0.002 min
Response: 6104301
Conc: 51.95 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

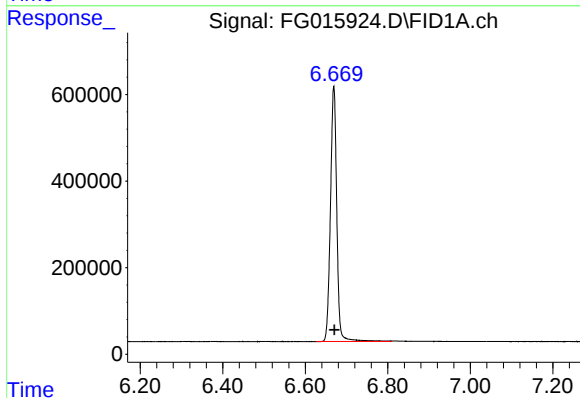


#3 N-DODECANE

R.T.: 6.669 min
Delta R.T.: -0.001 min
Response: 6274174
Conc: 51.69 ug/ml

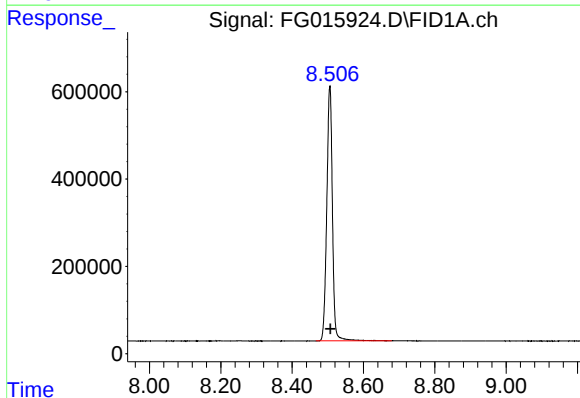


#4 N-TETRADECANE

R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 6426661
Conc: 50.33 ug/ml

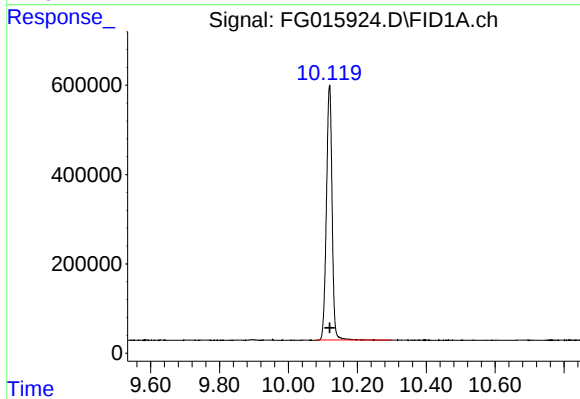

#5 N-HEXADECANE


R.T.: 10.119 min
Delta R.T.: 0.000 min
Response: 6488013
Conc: 48.70 ug/ml

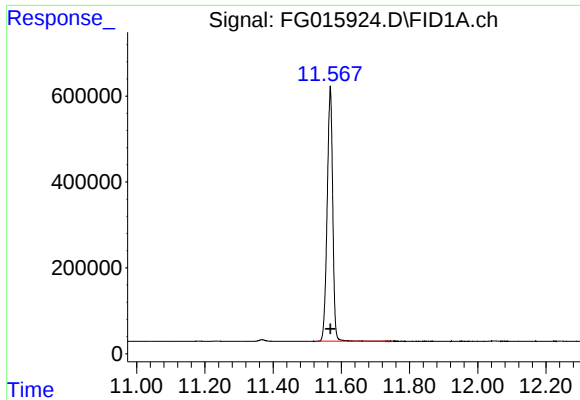

#6 N-OCTADECANE


R.T.: 11.568 min
Delta R.T.: 0.000 min
Response: 6633650
Conc: 48.07 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

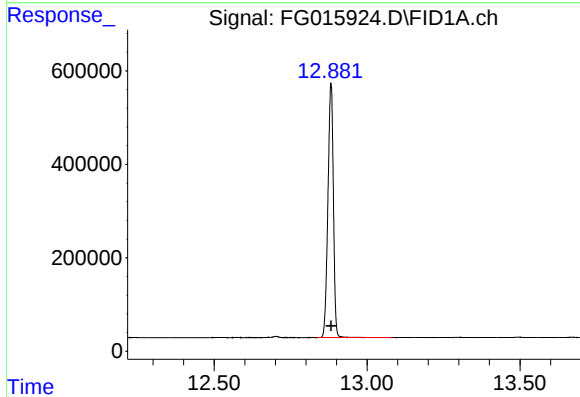


#7 N-EICOSANE

R.T.: 12.882 min
Delta R.T.: 0.000 min
Response: 6706560
Conc: 47.47 ug/ml

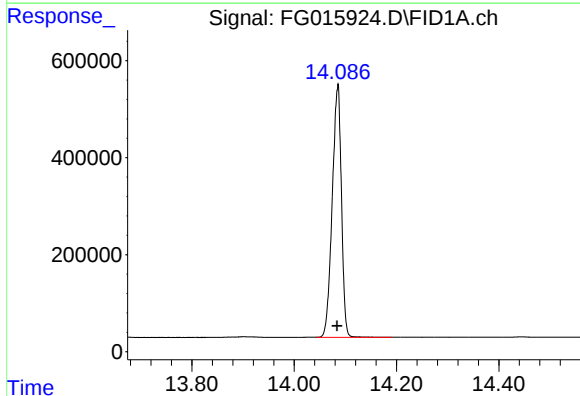


#8 N-DOCOSANE

R.T.: 14.085 min
Delta R.T.: 0.001 min
Response: 6511288
Conc: 47.40 ug/ml

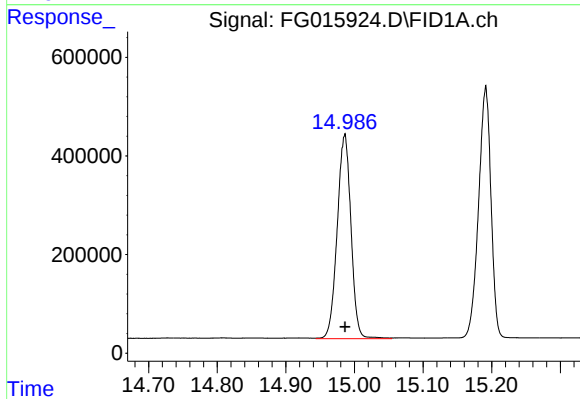

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.986 min
Delta R.T.: 0.000 min
Response: 5769617
Conc: 47.08 ug/ml

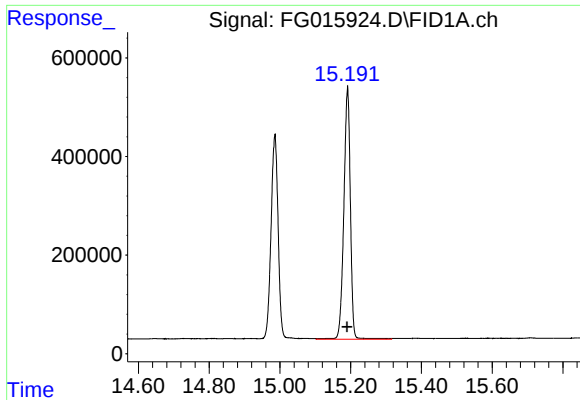

#10 N-TETRACOSANE


R.T.: 15.191 min
Delta R.T.: 0.000 min
Response: 6567275
Conc: 47.77 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

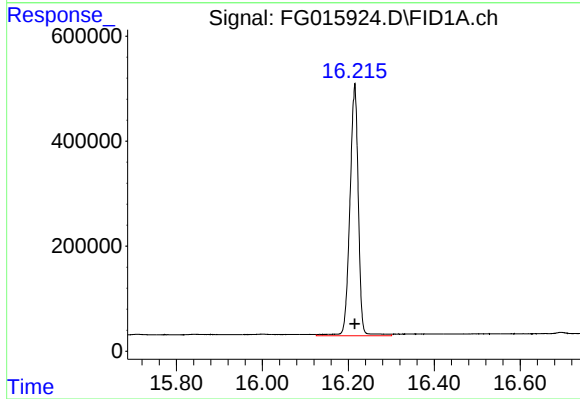

#11 N-HEXACOSANE

R.T.: 16.215 min
Delta R.T.: 0.000 min
Response: 6554402
Conc: 48.24 ug/ml

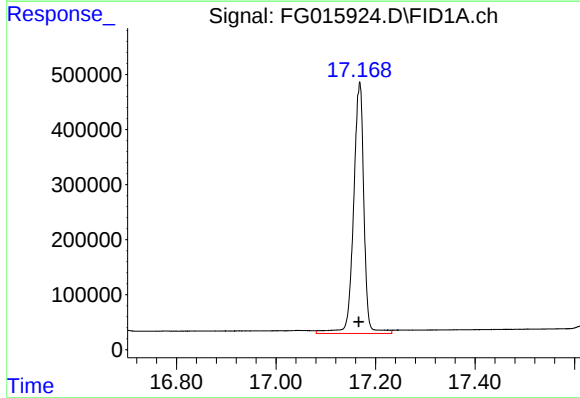

#12 N-OCTACOSANE

R.T.: 17.168 min
Delta R.T.: 0.001 min
Response: 6597278
Conc: 48.93 ug/ml