

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060619\
Data File : FG005114.D
Signal(s) : FID1A.ch
Acq On : 06 Jun 2019 08:22
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 07 00:37:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.978	101022	0.746 ug/ml
12)	N-OCTACOSANE	16.964	26995	0.212 ug/ml
13)	N-TRIACONTANE	17.849	58695	0.467 ug/ml
14)	N-DOTRIACONTANE	18.687	91694	0.765 ug/ml
15)	N-TETRATRIACONTANE	19.473	54518	0.484 ug/ml
16)	N-HEXATRIACONTANE	20.239	538144	5.073 ug/ml
17)	N-OCTATRIACONTANE	20.979	37663	0.389 ug/ml
18)	N-TETRACONTANE	21.963	381149	3.913 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060619\
Data File : FG005114.D
Signal(s) : FID1A.ch
Acq On : 06 Jun 2019 08:22
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 07 00:37:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG050919.M
Quant Title :
QLast Update : Thu May 09 14:52:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

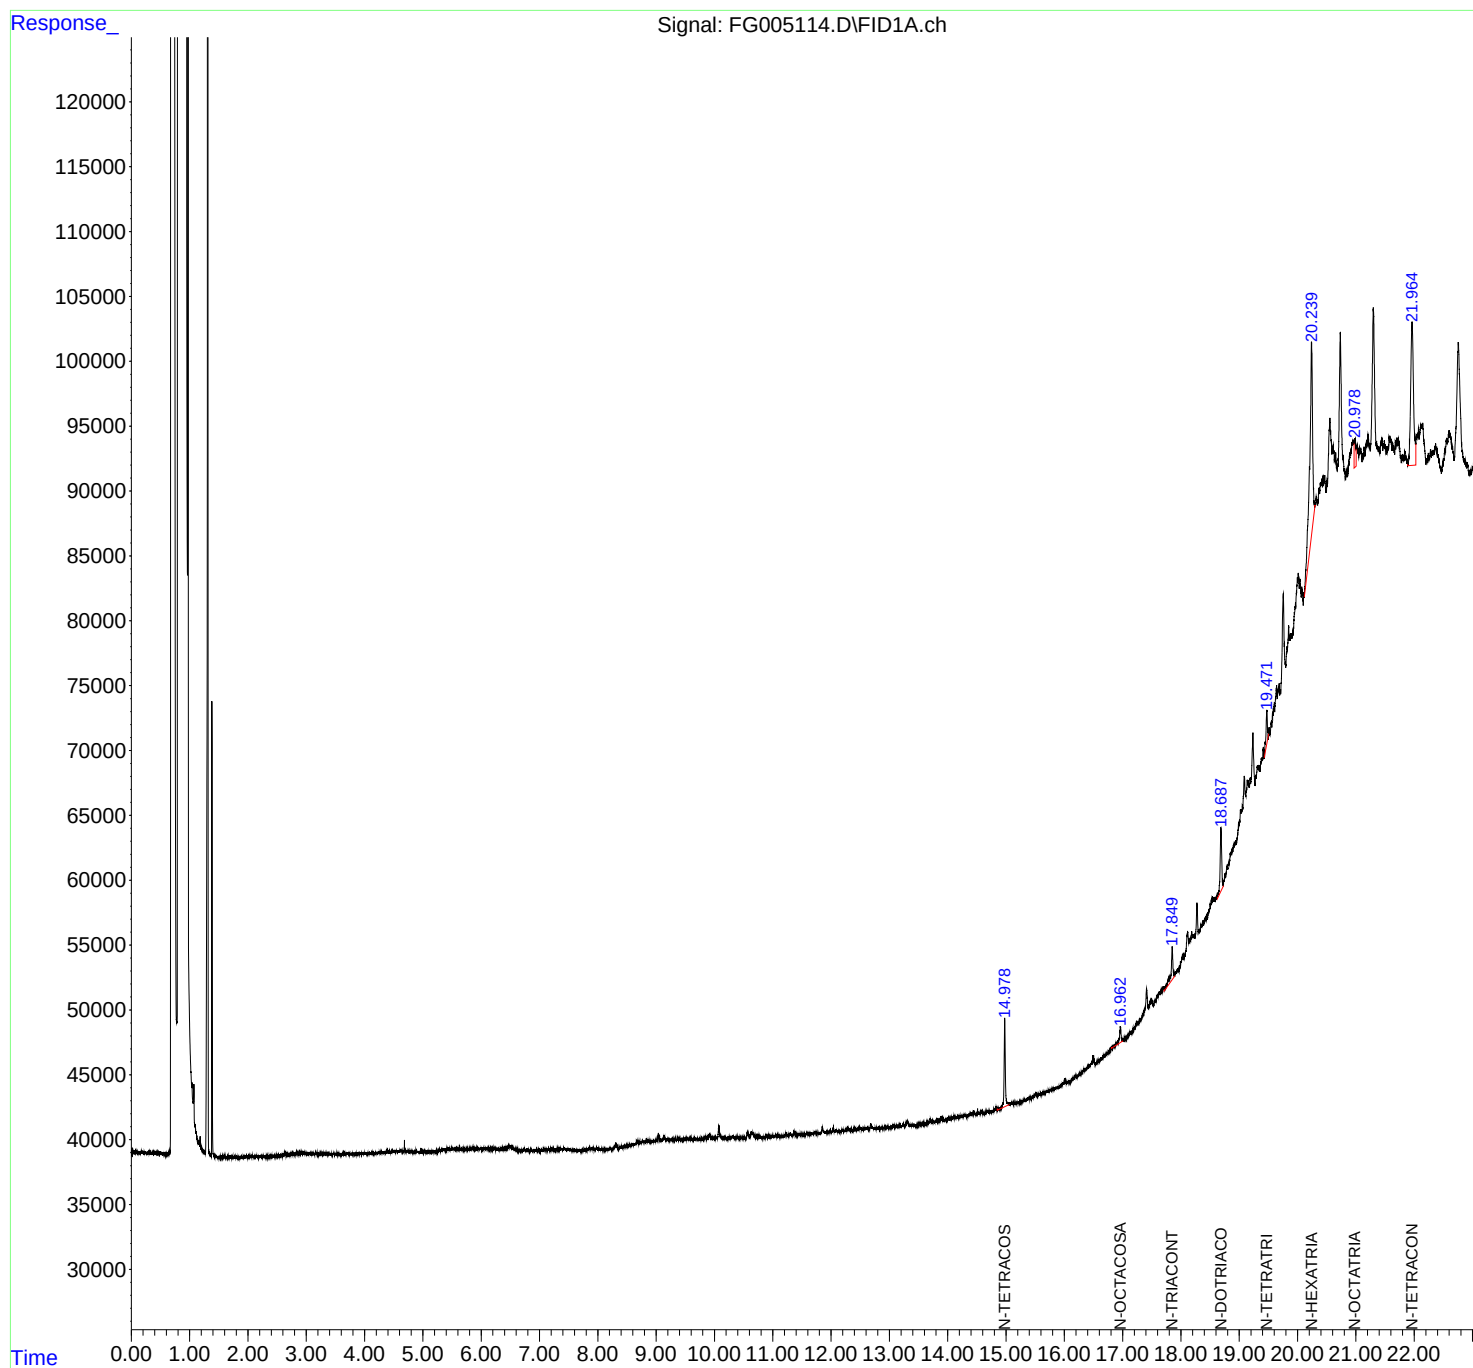

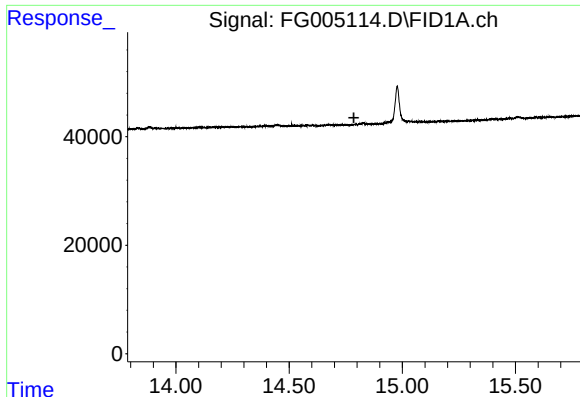


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.786 min
Response: 0
Conc: N.D.

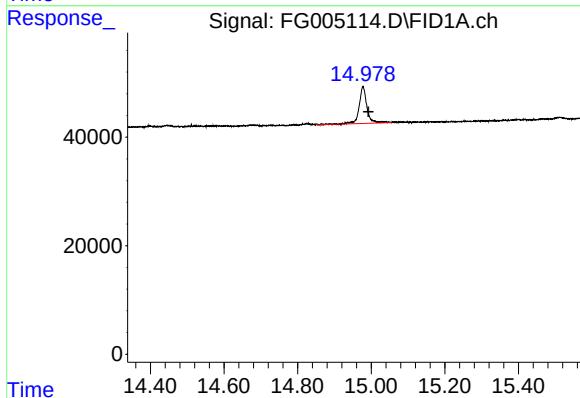


#10 N-TETRACOSANE

R.T.: 14.978 min
Delta R.T.: -0.015 min
Response: 101022
Conc: 0.75 ug/ml

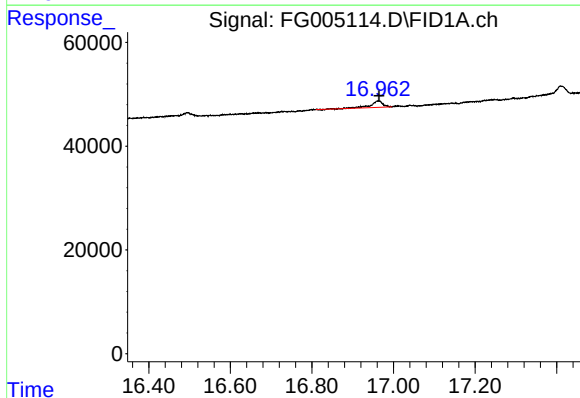


#12 N-OCTACOSANE

R.T.: 16.964 min
Delta R.T.: 0.000 min
Response: 26995
Conc: 0.21 ug/ml

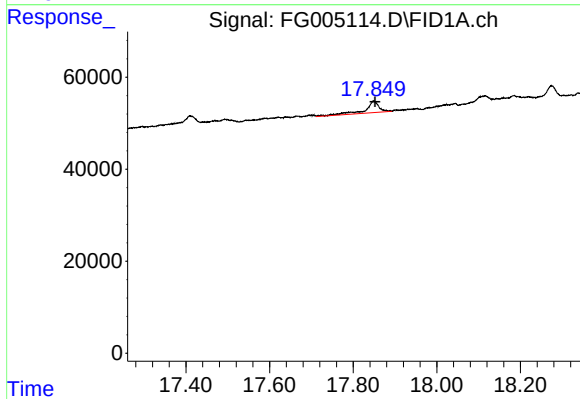


#13 N-TRIACONTANE

R.T.: 17.849 min
Delta R.T.: -0.004 min
Response: 58695
Conc: 0.47 ug/ml

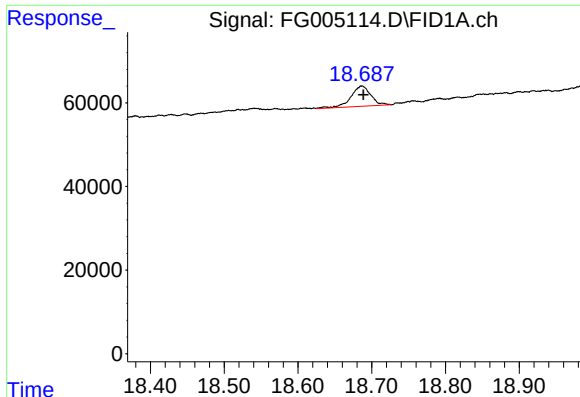


#14 N-DOTRIACONTANE

R.T.: 18.687 min
Delta R.T.: -0.002 min
Response: 91694
Conc: 0.77 ug/ml

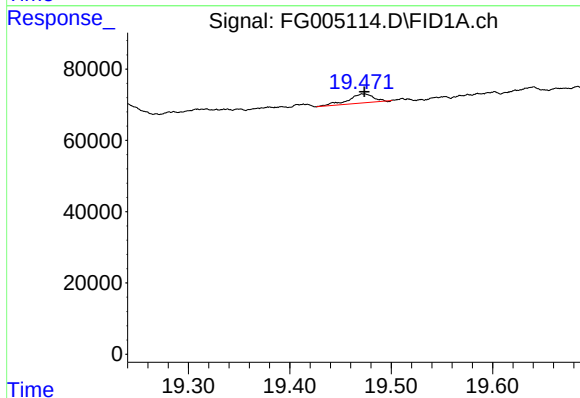


#15 N-TETRATRIACONTANE

R.T.: 19.473 min
Delta R.T.: 0.000 min
Response: 54518
Conc: 0.48 ug/ml

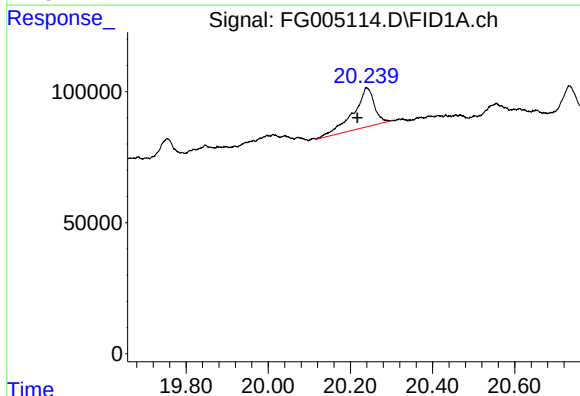


#16 N-HEXATRIACONTANE

R.T.: 20.239 min
Delta R.T.: 0.022 min
Response: 538144
Conc: 5.07 ug/ml

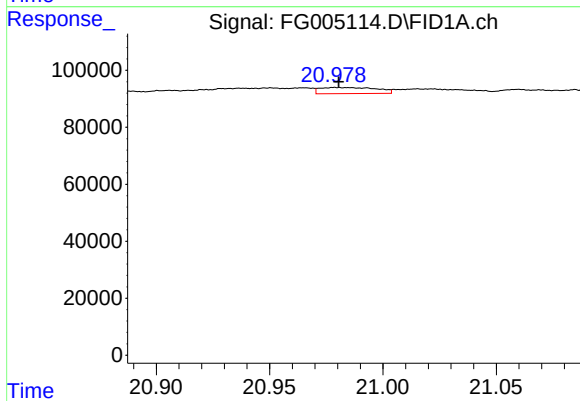

#17 N-OCTATRIACONTANE

R.T.: 20.979 min
Delta R.T.: -0.001 min
Response: 37663
Conc: 0.39 ug/ml

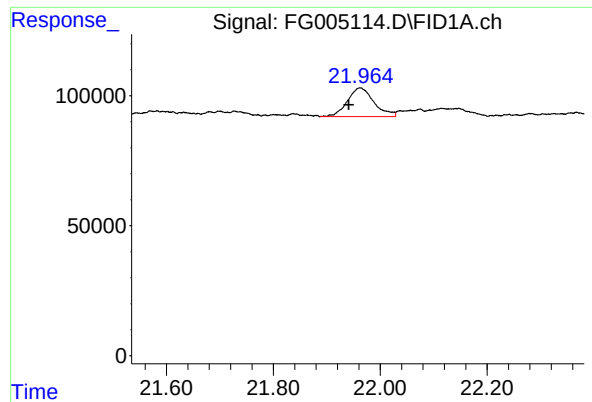

#18 N-TETRACONTANE

R.T.: 21.963 min
Delta R.T.: 0.022 min
Response: 381149
Conc: 3.91 ug/ml