

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
 Data File : FG008192.D
 Signal(s) : FID1A.ch
 Acq On : 06 Jun 2021 13:56
 Operator : DD\AJ
 Sample : M2603-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 04:53:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.787	2369909	19.970 ug/ml
Target Compounds			
7) N-EICOSANE	12.633	85452	0.624 ug/ml
8) N-DOCOSANE	13.881	152373	1.123 ug/ml
10) N-TETRACOSANE	14.977	1237726	9.201 ug/ml
11) N-HEXACOSANE	16.016	47507	0.361 ug/ml
12) N-OCTACOSANE	16.984	487956	3.765 ug/ml
13) N-TRIACONTANE	17.861	227730	1.784 ug/ml
14) N-DOTRIACONTANE	18.688	293894	2.365 ug/ml
15) N-TETRATRIACONTANE	19.481	118724	1.015 ug/ml
16) N-HEXATRIACONTANE	20.195	752405	6.794 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
Data File : FG008192.D
Signal(s) : FID1A.ch
Acq On : 06 Jun 2021 13:56
Operator : DD\AJ
Sample : M2603-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 04:53:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

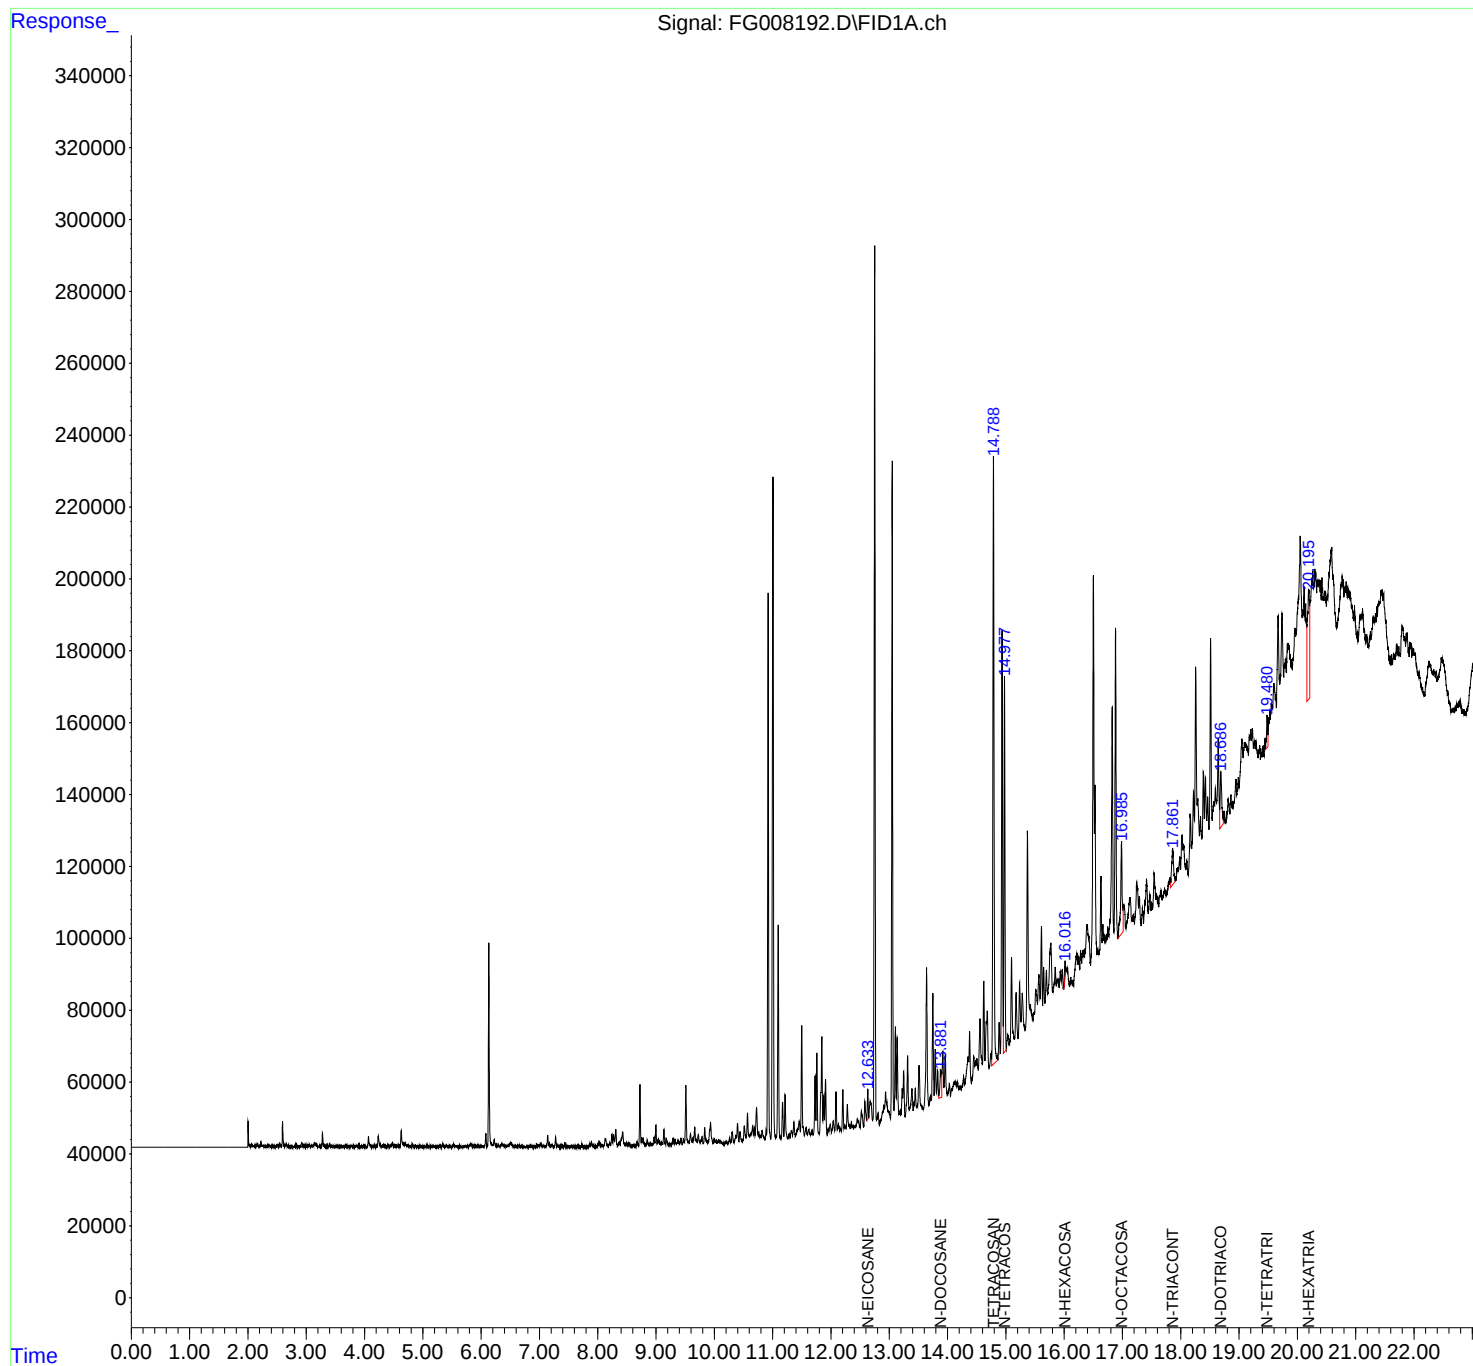


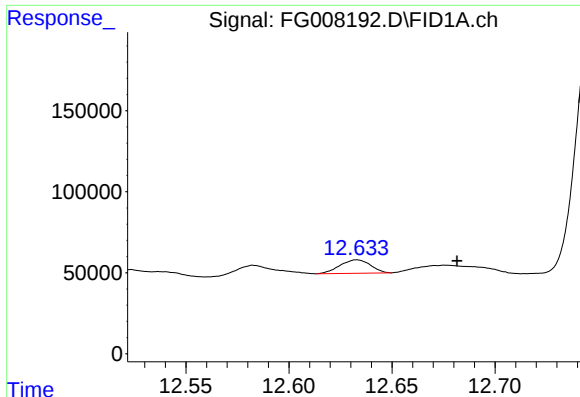

#7 N-EICOSANE


R.T.: 12.633 min
Delta R.T.: -0.048 min
Response: 85452
Conc: 0.62 ug/ml

Instrument :
FID_G
ClientSampleId :

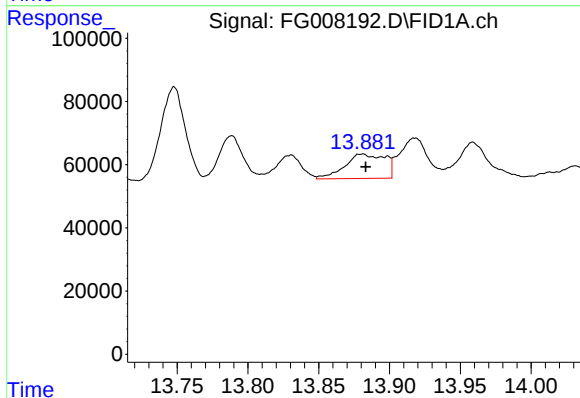


#8 N-DOCOSANE

R.T.: 13.881 min
Delta R.T.: -0.003 min
Response: 152373
Conc: 1.12 ug/ml

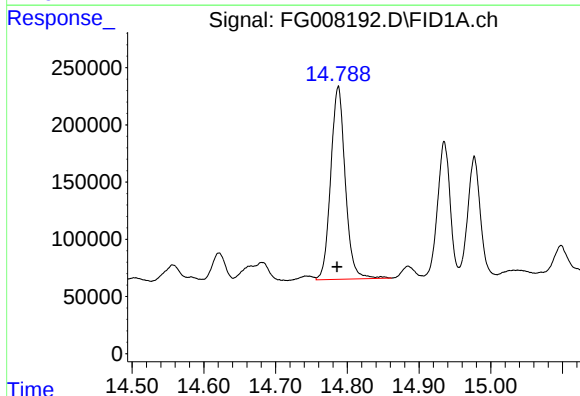


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.787 min
Delta R.T.: 0.002 min
Response: 2369909
Conc: 19.97 ug/ml

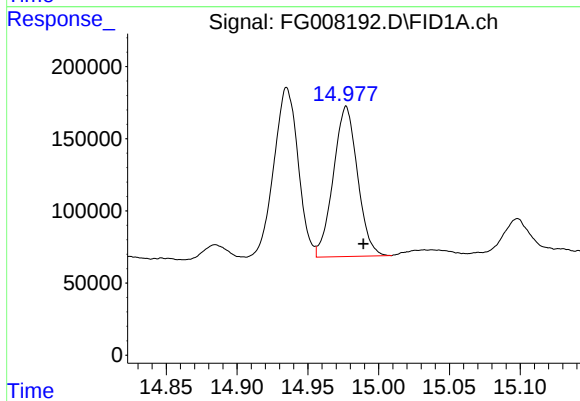

#10 N-TETRACOSANE


R.T.: 14.977 min
Delta R.T.: -0.012 min
Response: 1237726
Conc: 9.20 ug/ml

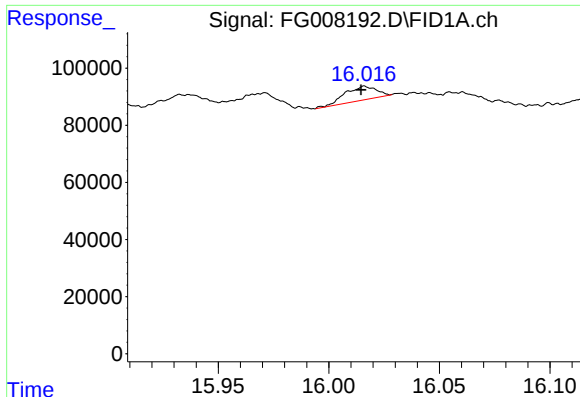

#11 N-HEXACOSANE


R.T.: 16.016 min
Delta R.T.: 0.002 min
Response: 47507
Conc: 0.36 ug/ml

Instrument :
FID_G
ClientSampleId :

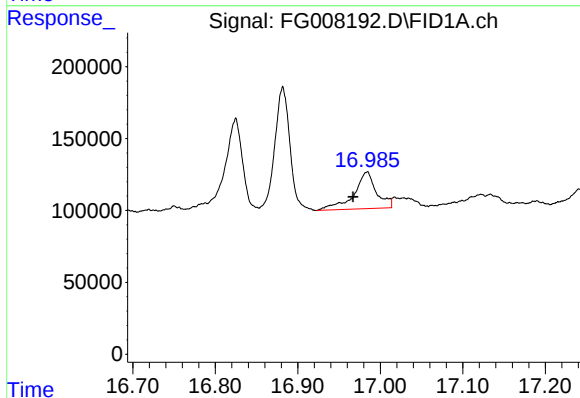


#12 N-OCTACOSANE

R.T.: 16.984 min
Delta R.T.: 0.017 min
Response: 487956
Conc: 3.76 ug/ml

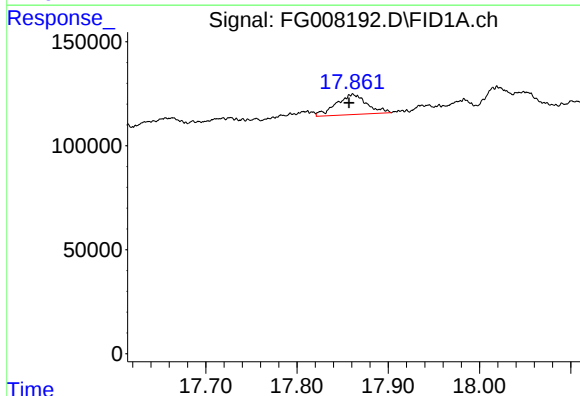


#13 N-TRIACONTANE

R.T.: 17.861 min
Delta R.T.: 0.004 min
Response: 227730
Conc: 1.78 ug/ml

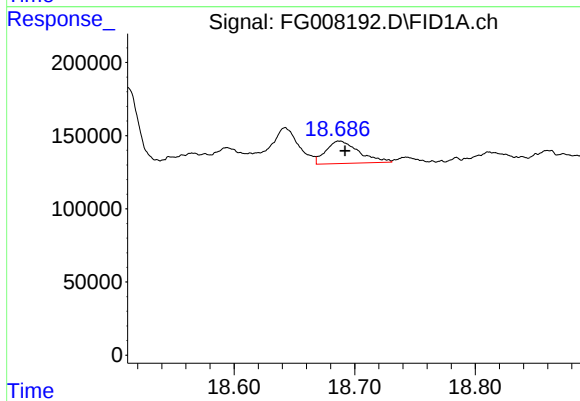

#14 N-DOTRIACONTANE


R.T.: 18.688 min
Delta R.T.: -0.004 min
Response: 293894
Conc: 2.37 ug/ml

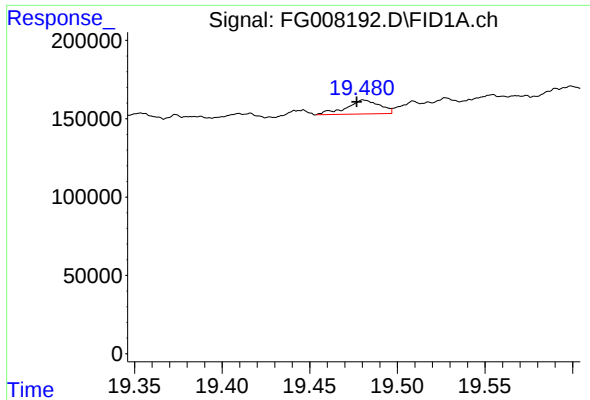

#15 N-TETRATRIACONTANE

R.T.: 19.481 min
Delta R.T.: 0.004 min
Response: 118724
Conc: 1.01 ug/ml

Instrument :
FID_G
ClientSampleId :

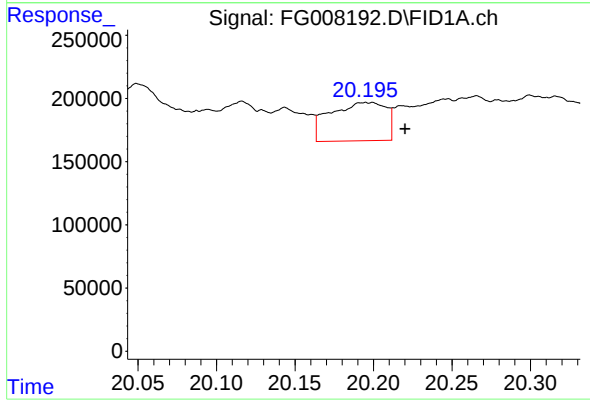

#16 N-HEXATRIACONTANE

R.T.: 20.195 min
Delta R.T.: -0.025 min
Response: 752405
Conc: 6.79 ug/ml