

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
 Data File : FG008193.D
 Signal(s) : FID1A.ch
 Acq On : 06 Jun 2021 14:28
 Operator : DD\AJ
 Sample : M2603-25
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 04:53:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	1257943	10.600 ug/ml
Target Compounds			
4) N-TETRADECANE	8.371f	116844	0.857 ug/ml
7) N-EICOSANE	12.747f	175794	1.284 ug/ml
10) N-TETRACOSANE	14.975	171005	1.271 ug/ml
11) N-HEXACOSANE	16.013	90267	0.687 ug/ml
12) N-OCTACOSANE	16.967	172396	1.330 ug/ml
13) N-TRIACONTANE	17.859	94396	0.739 ug/ml
14) N-DOTRIACONTANE	18.690	189214	1.523 ug/ml
16) N-HEXATRIACONTANE	20.226	290831	2.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
Data File : FG008193.D
Signal(s) : FID1A.ch
Acq On : 06 Jun 2021 14:28
Operator : DD\AJ
Sample : M2603-25
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 04:53:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

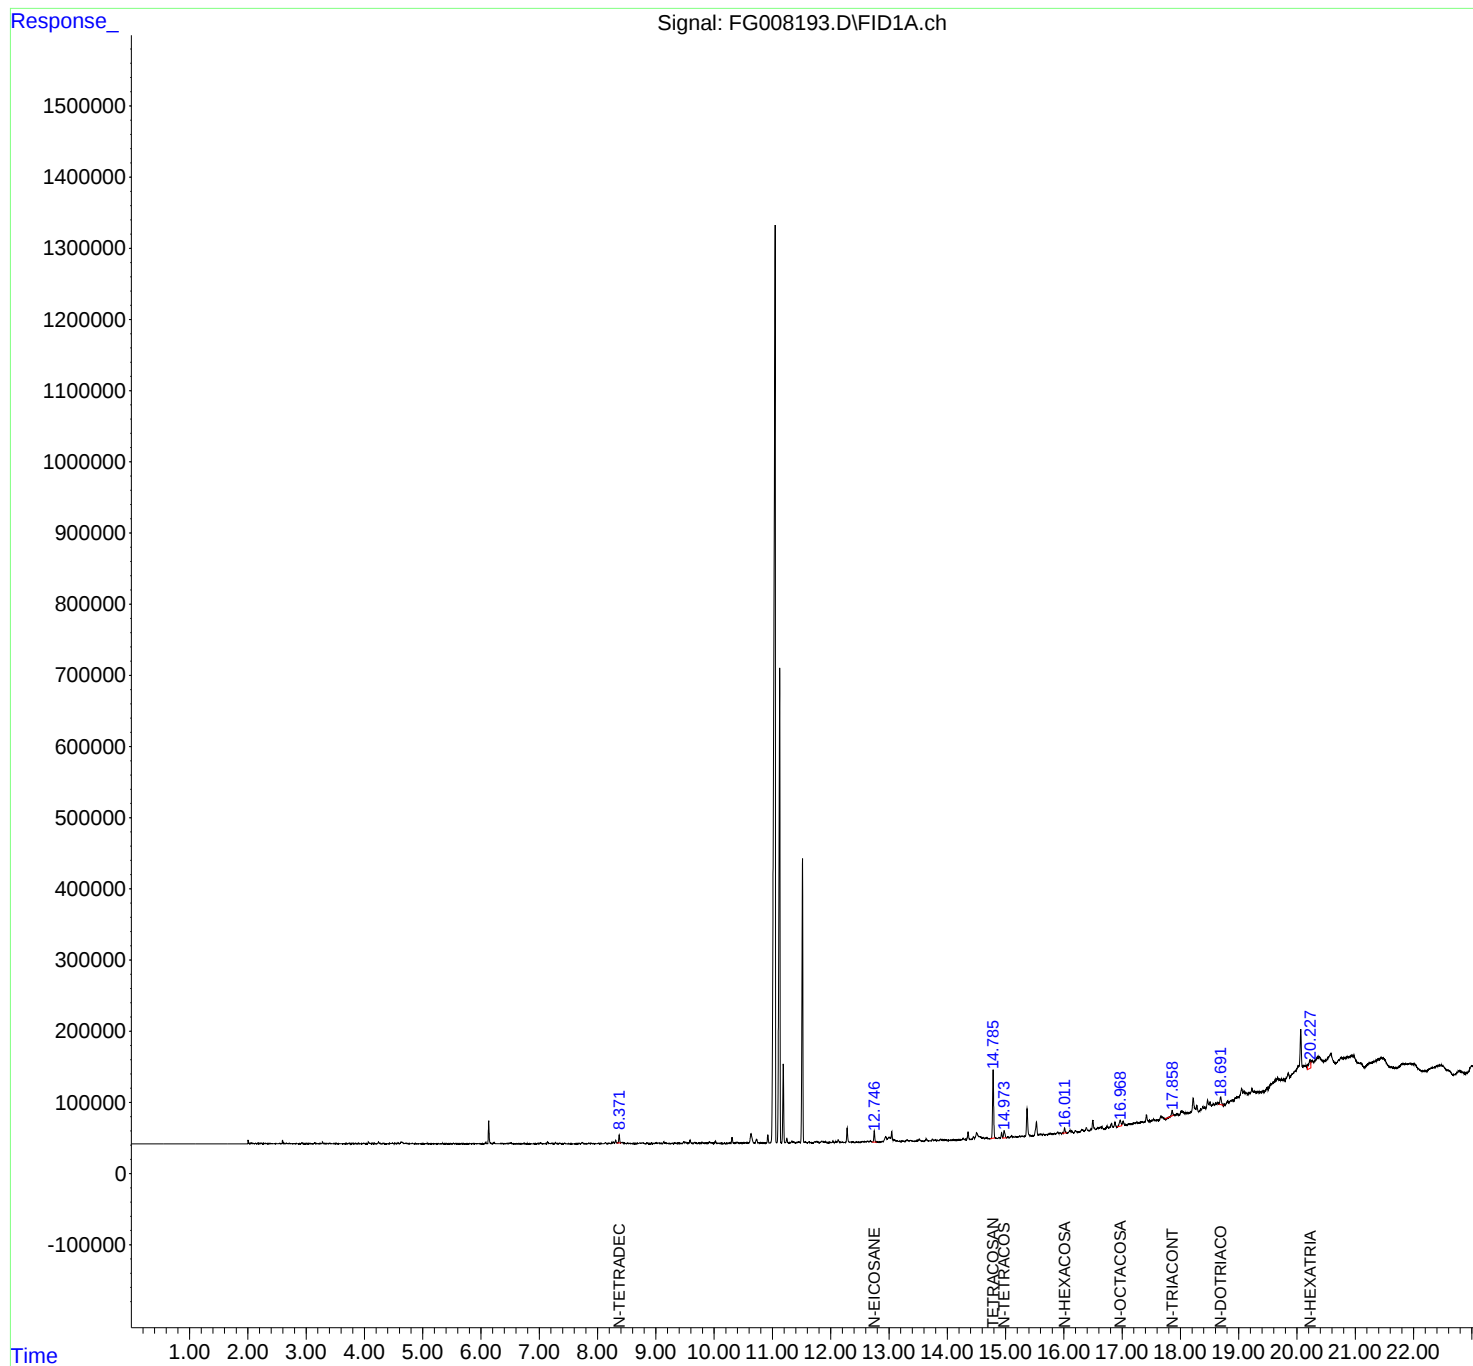


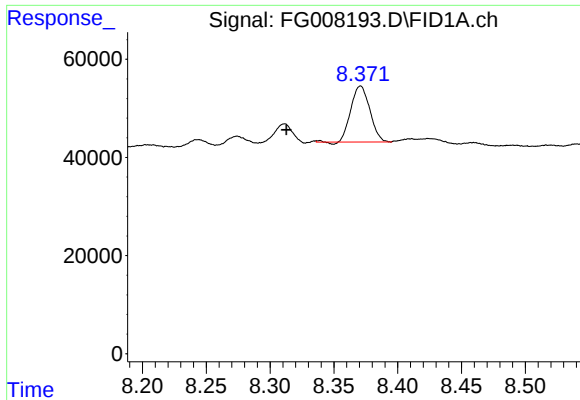

#4 N-TETRADECANE


R.T.: 8.371 min
Delta R.T.: 0.058 min
Response: 116844
Conc: 0.86 ug/ml

Instrument :
FID_G
ClientSampleId :

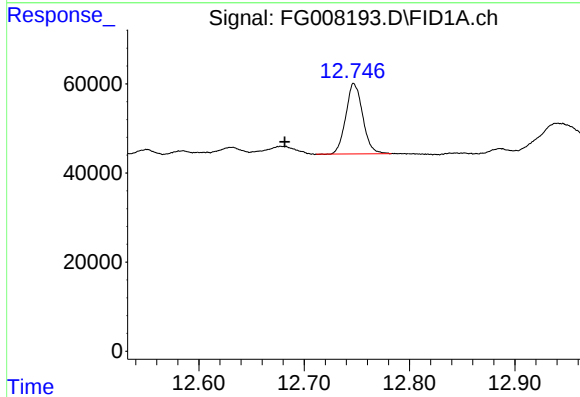


#7 N-EICOSANE

R.T.: 12.747 min
Delta R.T.: 0.066 min
Response: 175794
Conc: 1.28 ug/ml

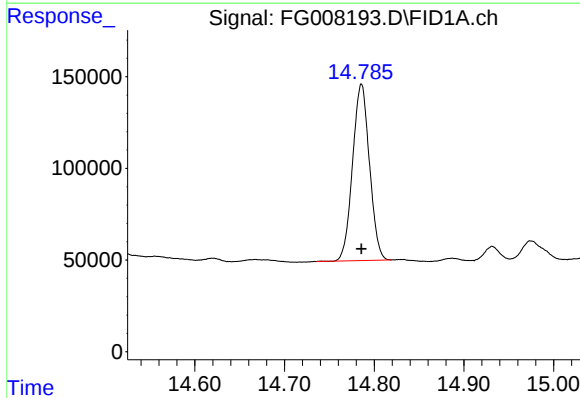


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.786 min
Delta R.T.: 0.000 min
Response: 1257943
Conc: 10.60 ug/ml

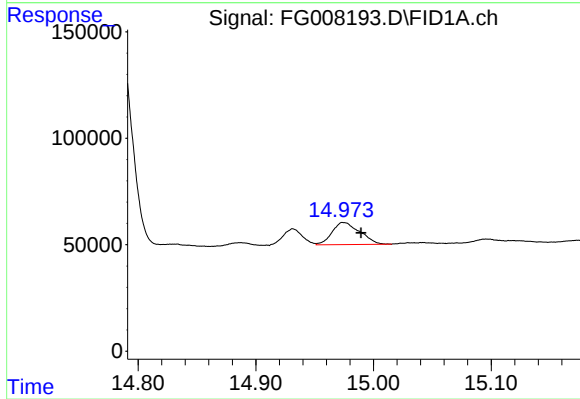

#10 N-TETRACOSANE


R.T.: 14.975 min
Delta R.T.: -0.015 min
Response: 171005
Conc: 1.27 ug/ml

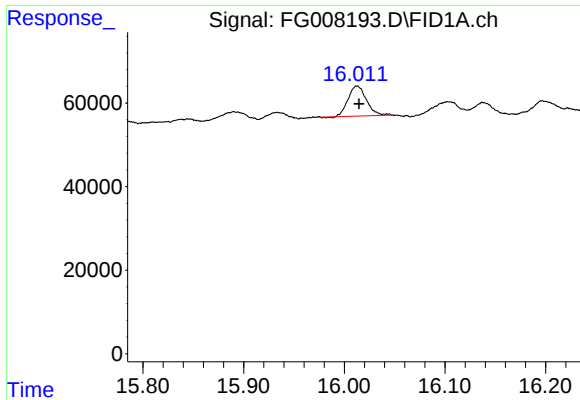

#11 N-HEXACOSANE


R.T.: 16.013 min
Delta R.T.: -0.002 min
Response: 90267
Conc: 0.69 ug/ml

Instrument :
FID_G
ClientSampleId :

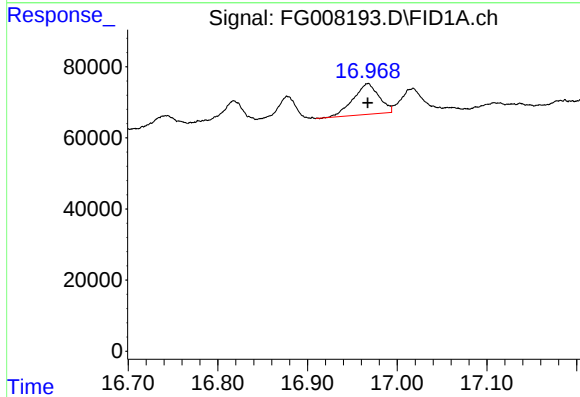


#12 N-OCTACOSANE

R.T.: 16.967 min
Delta R.T.: 0.000 min
Response: 172396
Conc: 1.33 ug/ml

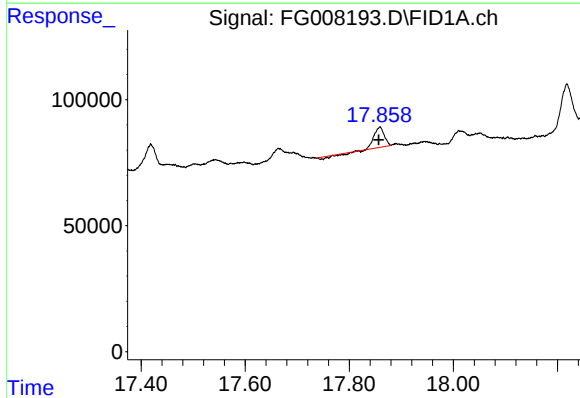


#13 N-TRIACONTANE

R.T.: 17.859 min
Delta R.T.: 0.002 min
Response: 94396
Conc: 0.74 ug/ml

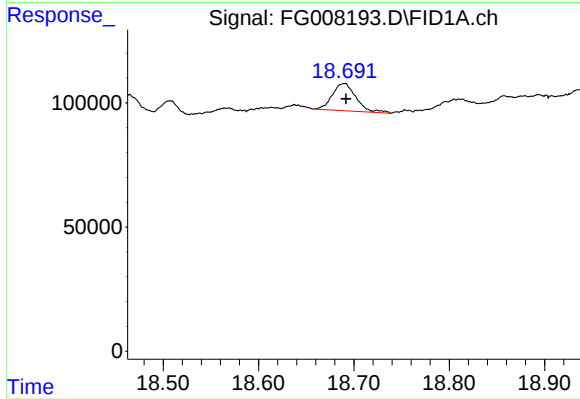

#14 N-DOTRIACONTANE

R.T.: 18.690 min
Delta R.T.: -0.002 min
Response: 189214
Conc: 1.52 ug/ml

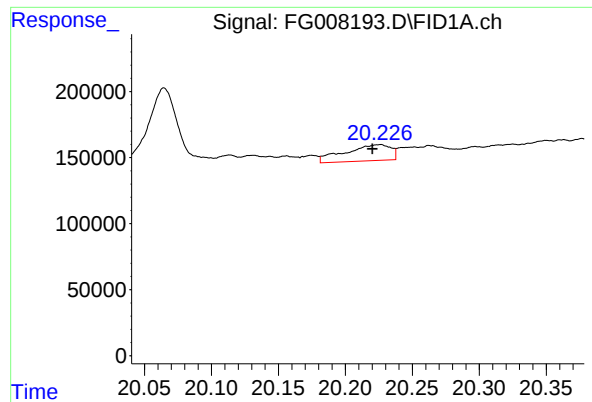

#16 N-HEXATRIACONTANE

R.T.: 20.226 min
Delta R.T.: 0.006 min
Response: 290831
Conc: 2.63 ug/ml

Instrument :
FID_G
ClientSampleId :