

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
Data File : FG008195.D
Signal(s) : FID1A.ch
Acq On : 06 Jun 2021 15:31
Operator : DD\AJ
Sample : M2613-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 04:53:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	2000456	16.857 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.213	503299	4.544 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
Data File : FG008195.D
Signal(s) : FID1A.ch
Acq On : 06 Jun 2021 15:31
Operator : DD\AJ
Sample : M2613-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 04:53:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

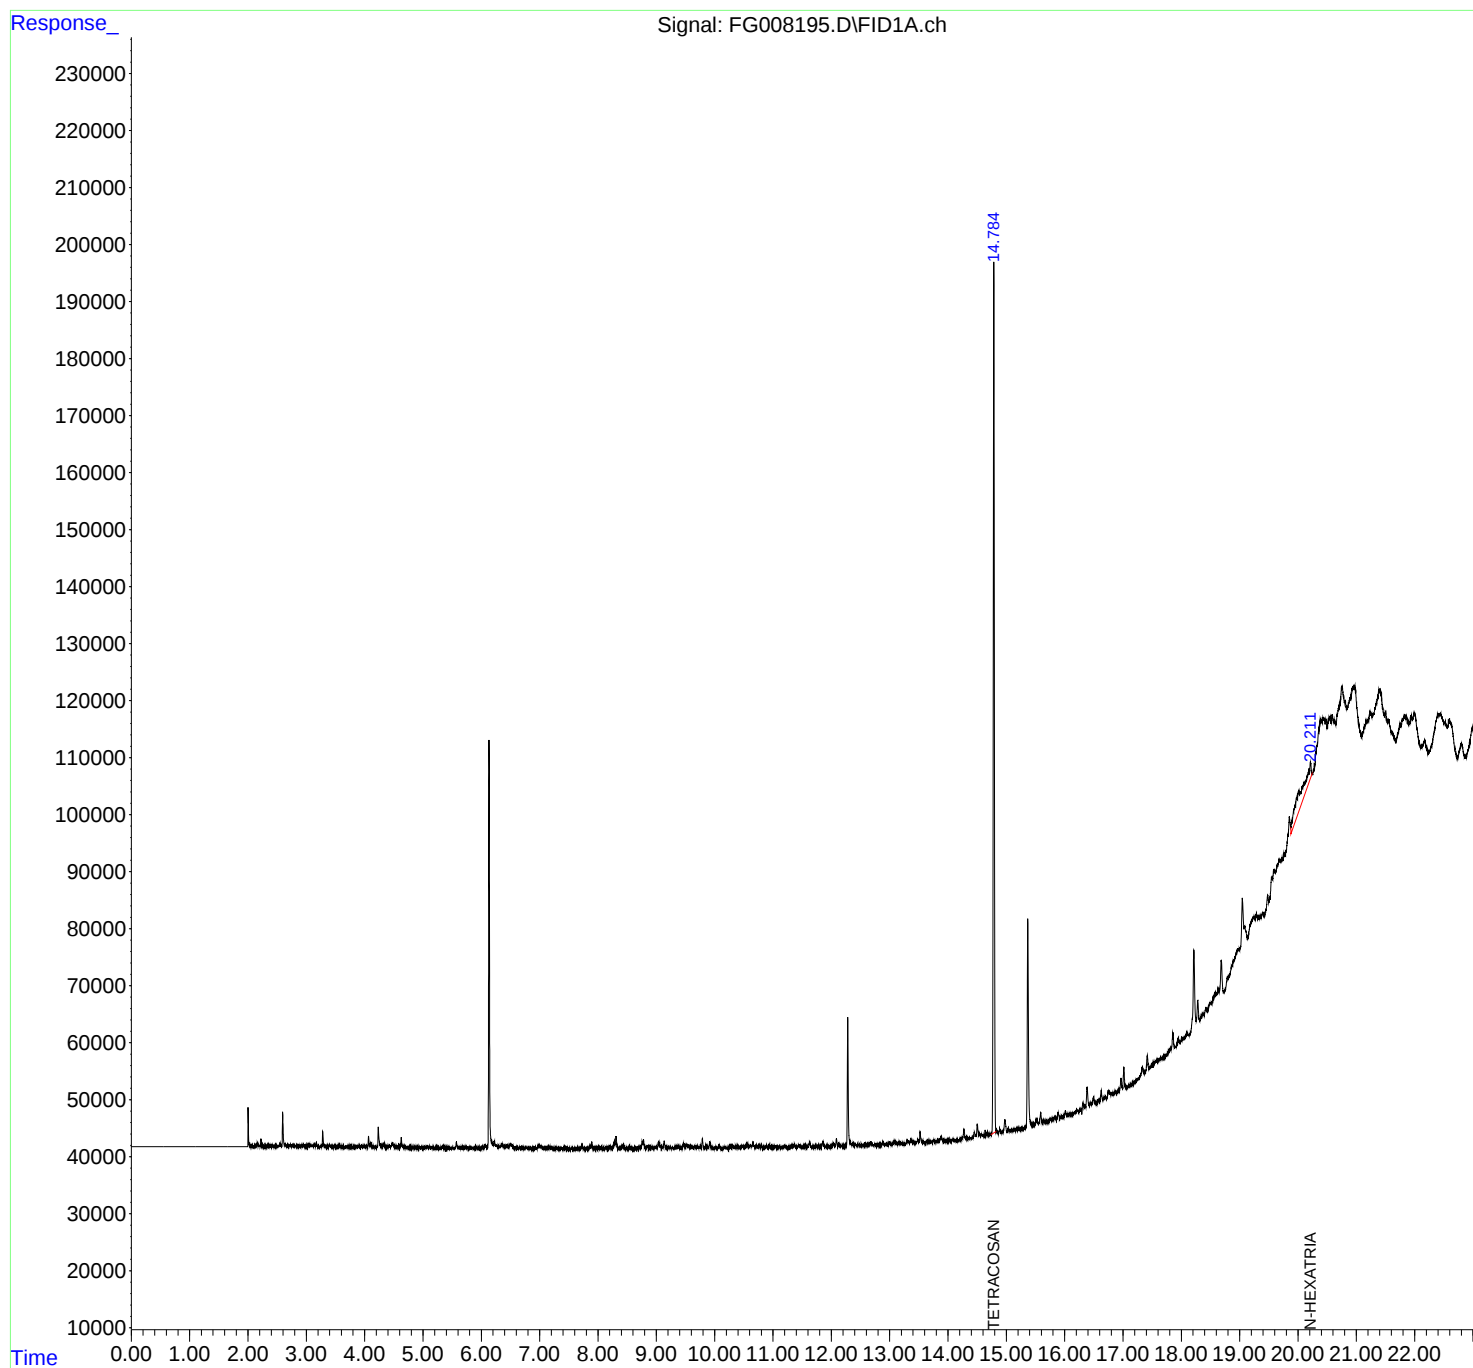


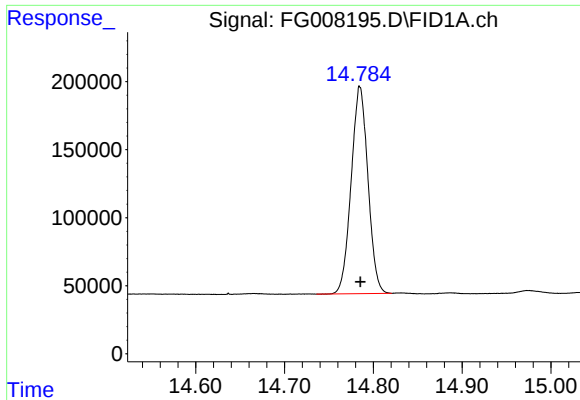

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 2000456
Conc: 16.86 ug/ml

Instrument :
FID_G
ClientSampleId :

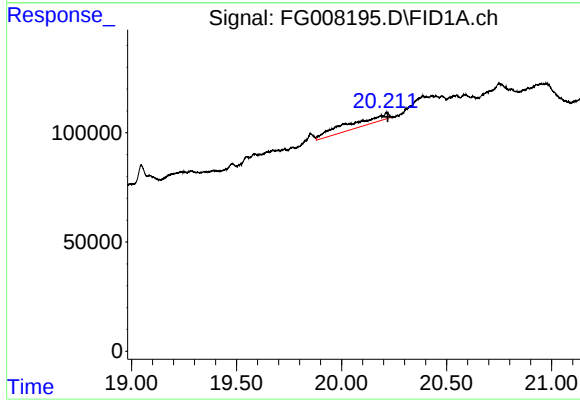

#16 N-HEXATRIACONTANE

R.T.: 20.213 min
Delta R.T.: -0.007 min
Response: 503299
Conc: 4.54 ug/ml