

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
 Data File : FG008212.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jun 2021 01:31
 Operator : DD\AJ
 Sample : M2603-17 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 04:56:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.782	271479	2.288 ug/ml
Target Compounds			
7) N-EICOSANE	12.627f	72752	0.532 ug/ml
10) N-TETRACOSANE	14.969	146048	1.086 ug/ml
13) N-TRIACONTANE	17.856	107508	0.842 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060621\
Data File : FG008212.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2021 01:31
Operator : DD\AJ
Sample : M2603-17 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 04:56:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

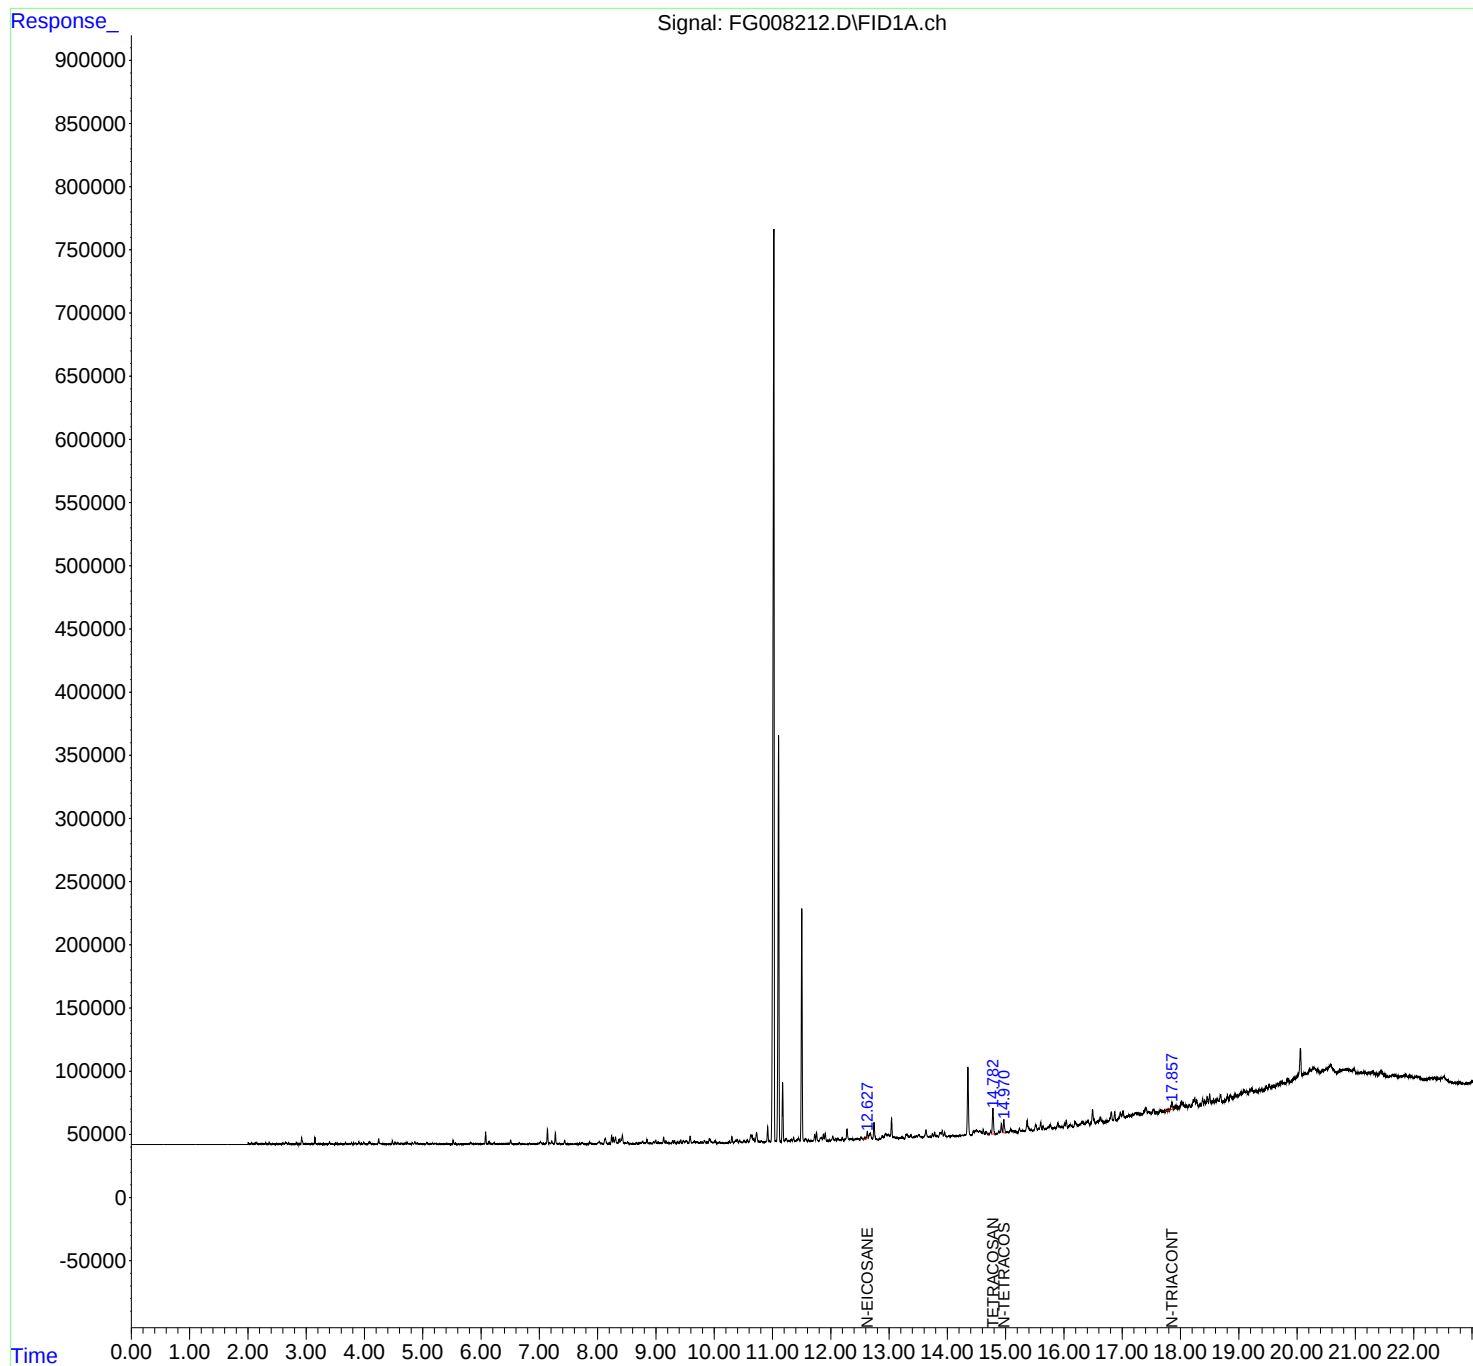


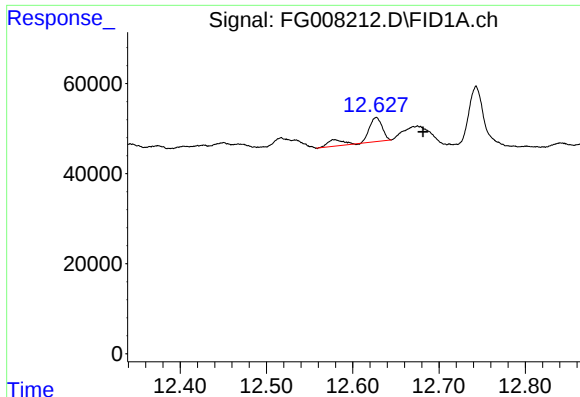

#7 N-EICOSANE


R.T.: 12.627 min
Delta R.T.: -0.054 min
Response: 72752
Conc: 0.53 ug/ml

Instrument :
FID_G
ClientSampleId :

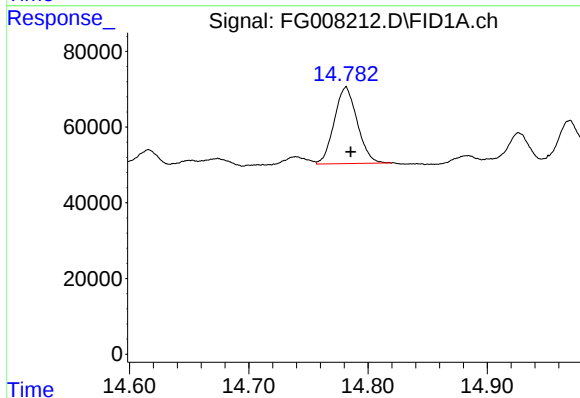


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.782 min
Delta R.T.: -0.004 min
Response: 271479
Conc: 2.29 ug/ml

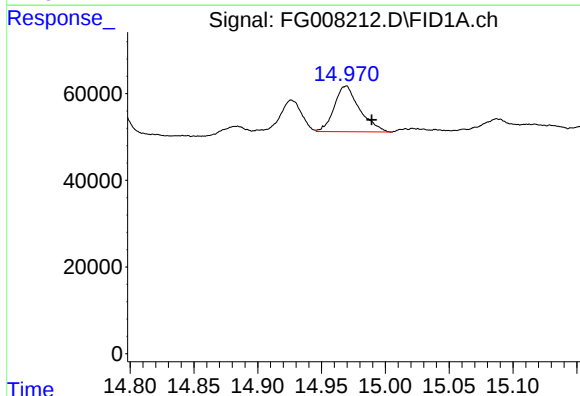

#10 N-TETRACOSANE

R.T.: 14.969 min
Delta R.T.: -0.020 min
Response: 146048
Conc: 1.09 ug/ml

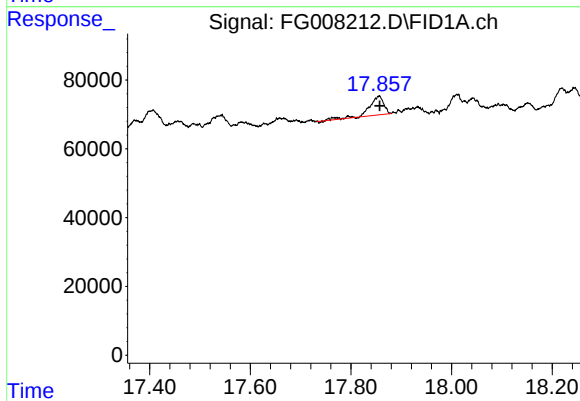

#13 N-TRIACONTANE

R.T.: 17.856 min
Delta R.T.: 0.000 min
Response: 107508
Conc: 0.84 ug/ml