

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060719\
Data File : FG005130.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2019 17:52
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 10 08:28:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:27:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

12)	N-OCTACOSANE	16.955	32805	0.225 ug/ml
13)	N-TRIACONTANE	17.843	64275	0.452 ug/ml
14)	N-DOTRIACONTANE	18.681	81218	0.592 ug/ml
15)	N-TETRATRIACONTANE	19.463	26895	0.205 ug/ml
16)	N-HEXATRIACONTANE	20.238	66788	0.542 ug/ml
18)	N-TETRACONTANE	21.956	82636	0.756 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG060719\
Data File : FG005130.D
Signal(s) : FID1A.ch
Acq On : 07 Jun 2019 17:52
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 10 08:28:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:27:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

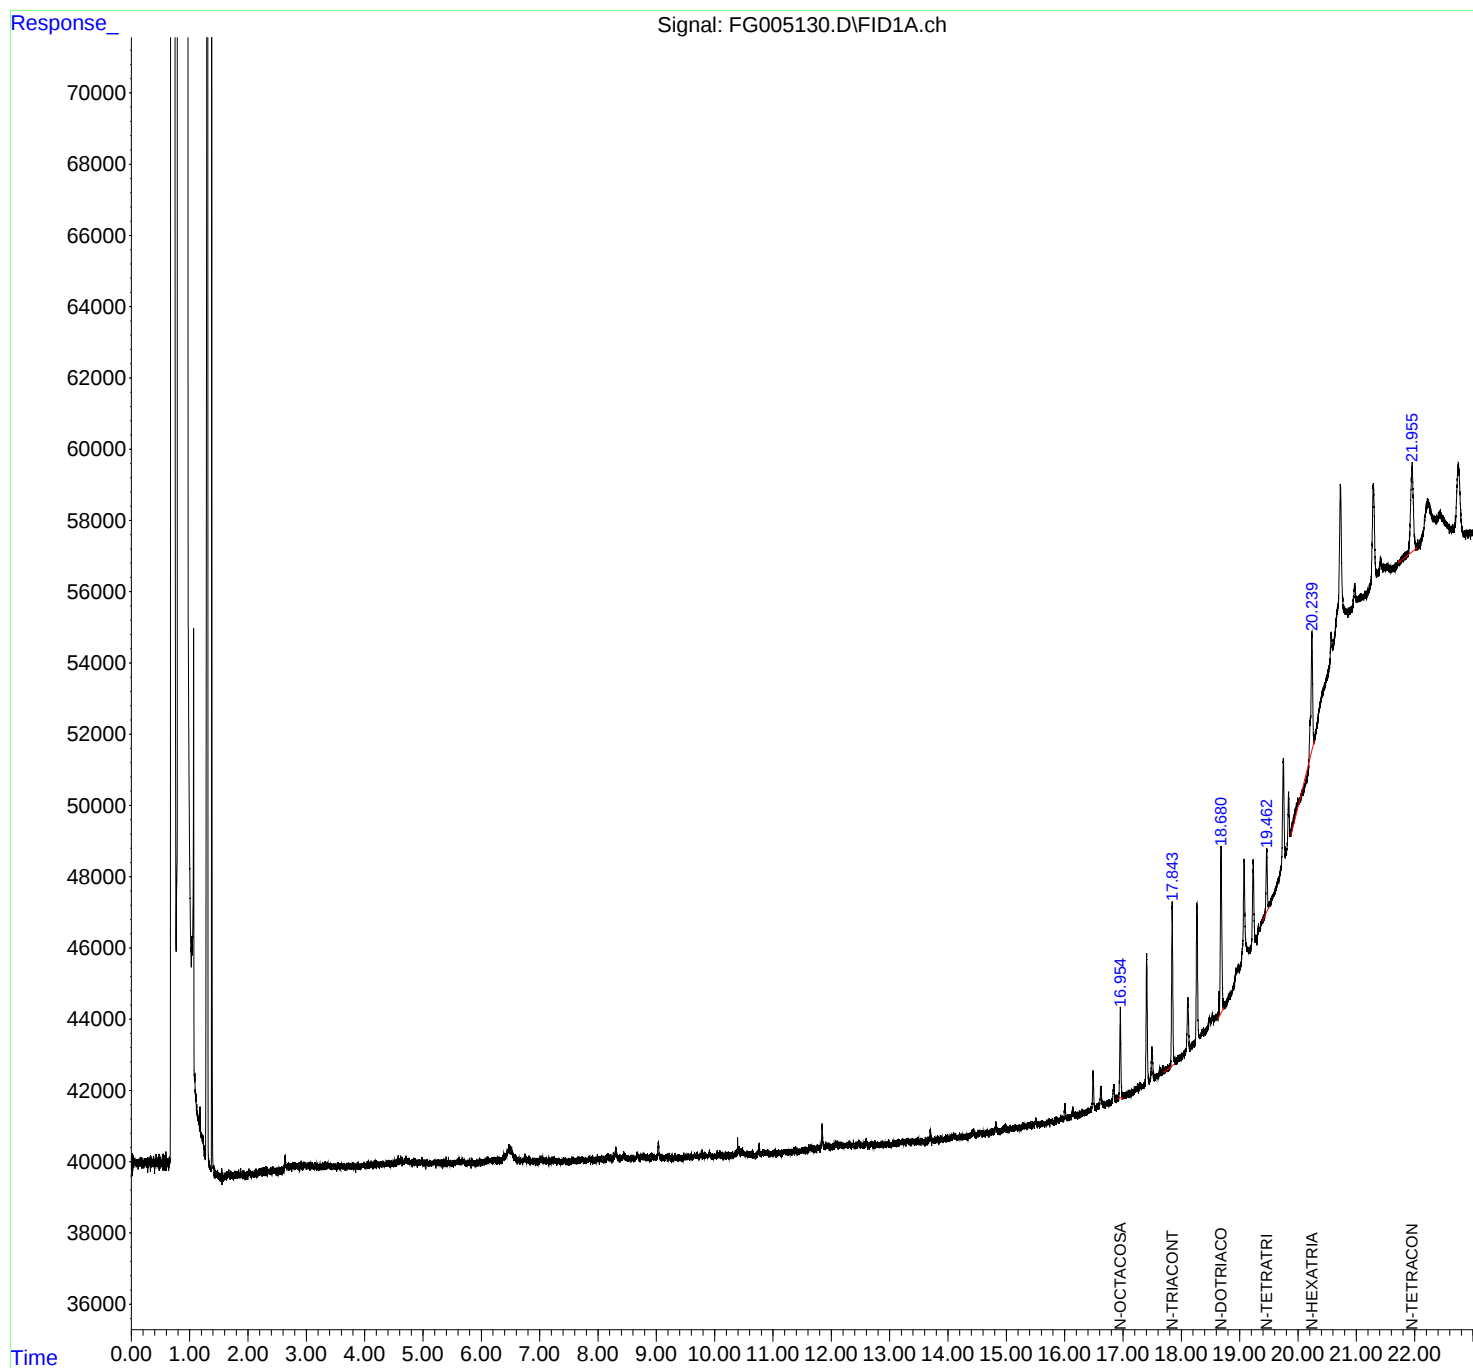


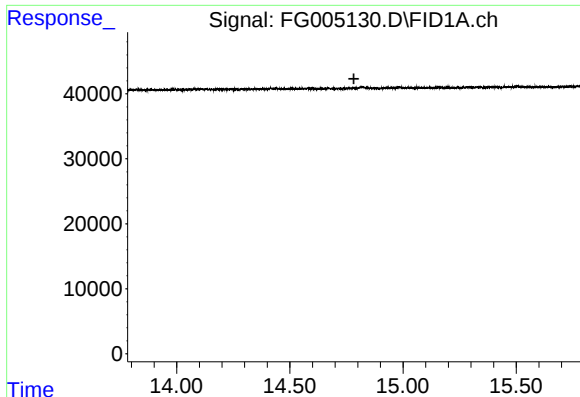

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.783 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

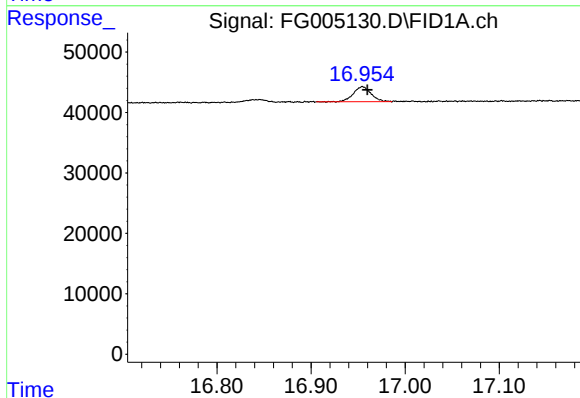


#12 N-OCTACOSANE

R.T.: 16.955 min
Delta R.T.: -0.005 min
Response: 32805
Conc: 0.22 ug/ml

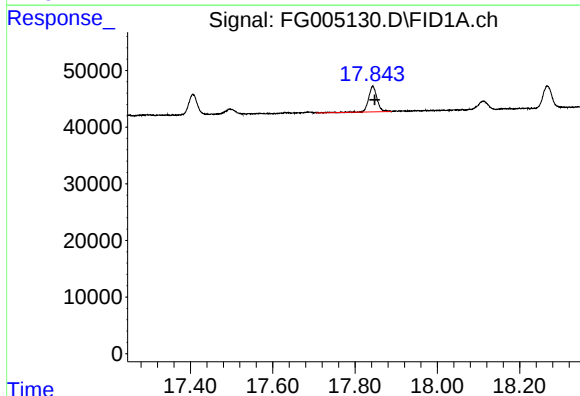


#13 N-TRIACONTANE

R.T.: 17.843 min
Delta R.T.: -0.005 min
Response: 64275
Conc: 0.45 ug/ml

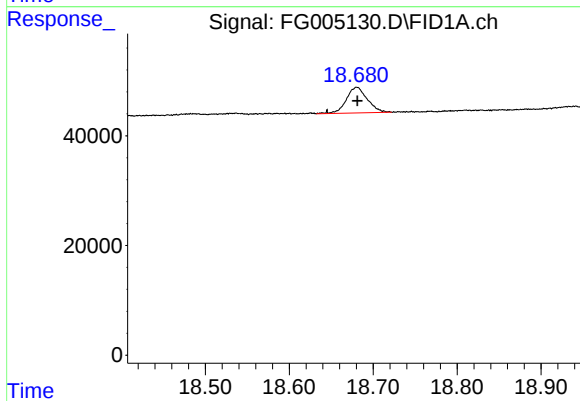

#14 N-DOTRIACONTANE


R.T.: 18.681 min
Delta R.T.: 0.000 min
Response: 81218
Conc: 0.59 ug/ml

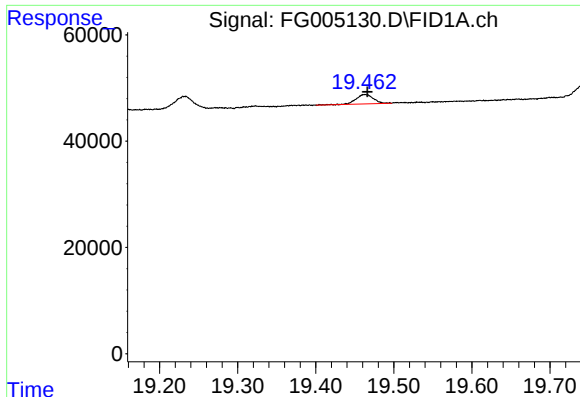

#15 N-TETRATRIACONTANE


R.T.: 19.463 min
Delta R.T.: -0.004 min
Response: 26895
Conc: 0.20 ug/ml

Instrument :
FID_G
ClientSampleId :

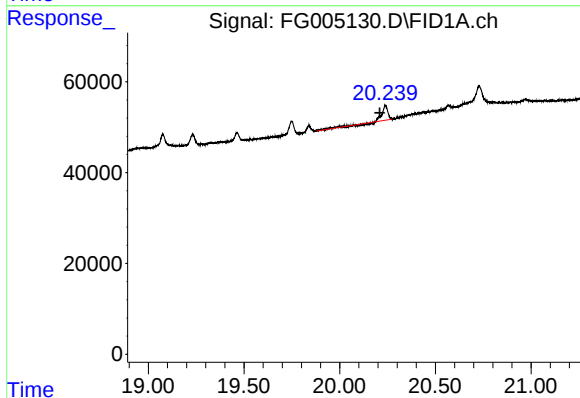

#16 N-HEXATRIACONTANE

R.T.: 20.238 min
Delta R.T.: 0.029 min
Response: 66788
Conc: 0.54 ug/ml

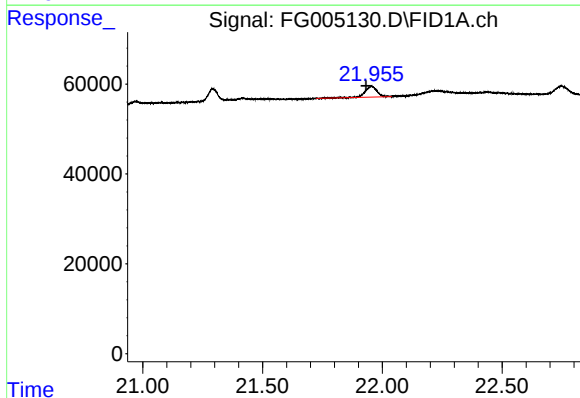

#18 N-TETRACONTANE

R.T.: 21.956 min
Delta R.T.: 0.023 min
Response: 82636
Conc: 0.76 ug/ml